


Data Path : Z:\HPCHEM1\BNA F\Data\BF072117\
 Data File : BF096936.D
 Acq On : 21 Jul 2017 11:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 24 14:10:38 2017

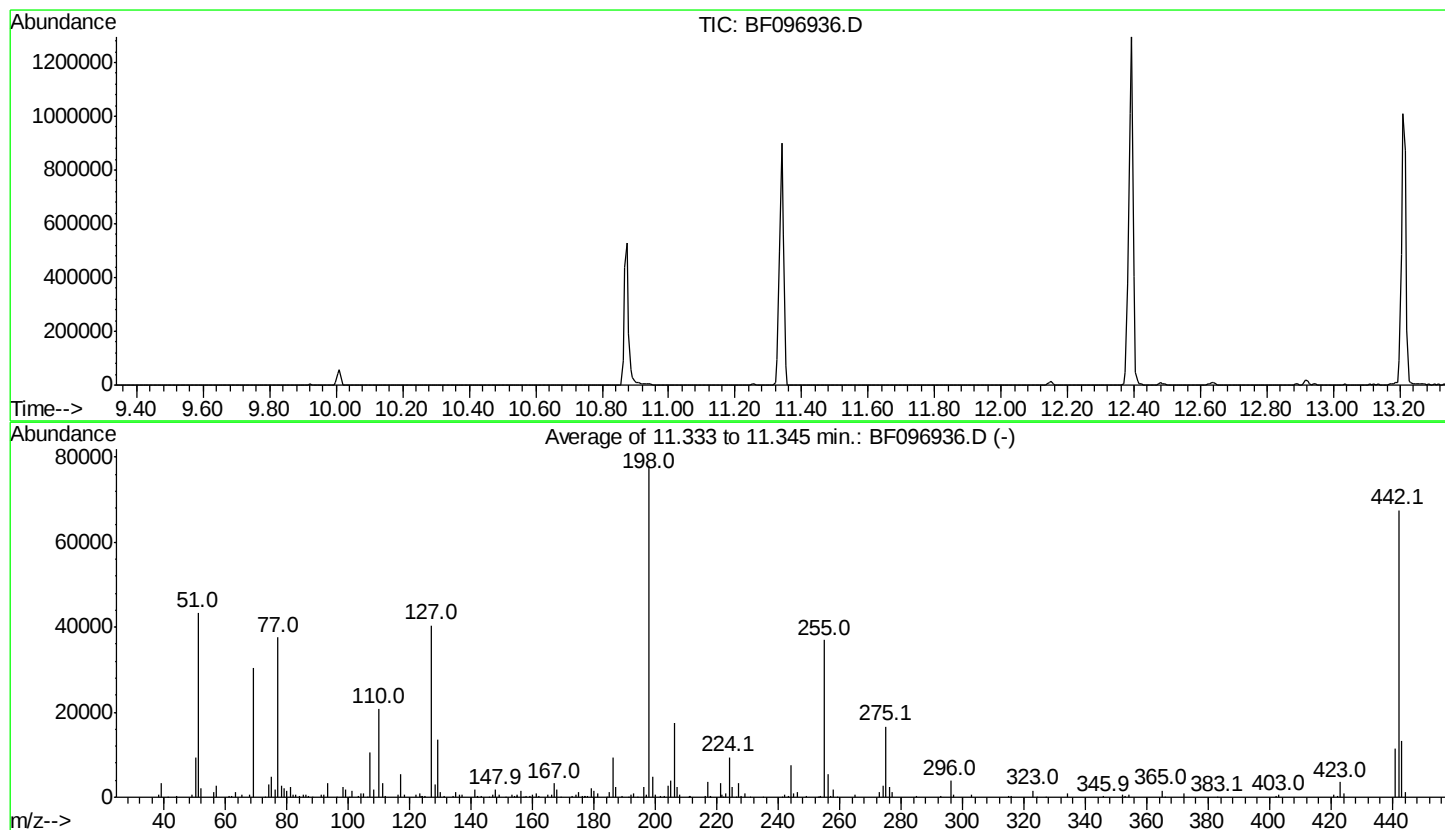

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.7	43453	PASS
68	69	0.00	2	1.8	544	PASS
69	198	0.00	100	39.1	30480	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	40458	PASS
197	198	0.00	2	0.7	578	PASS
198	198	100	100	100.0	77978	PASS
199	198	5	9	6.1	4783	PASS
275	198	10	60	21.2	16560	PASS
365	198	1	100	2.0	1576	PASS
441	442	0.01	24	17.1	11573	PASS
442	198	50	100	86.5	67482	PASS
443	442	15	24	19.5	13170	PASS