
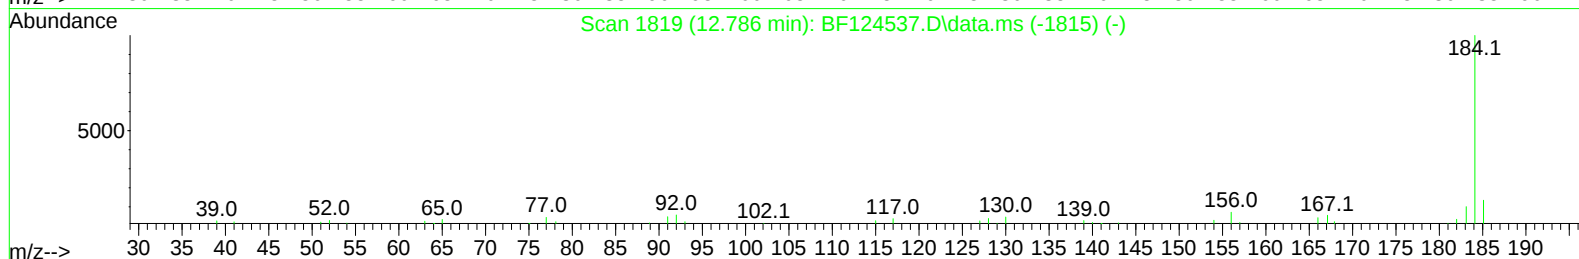
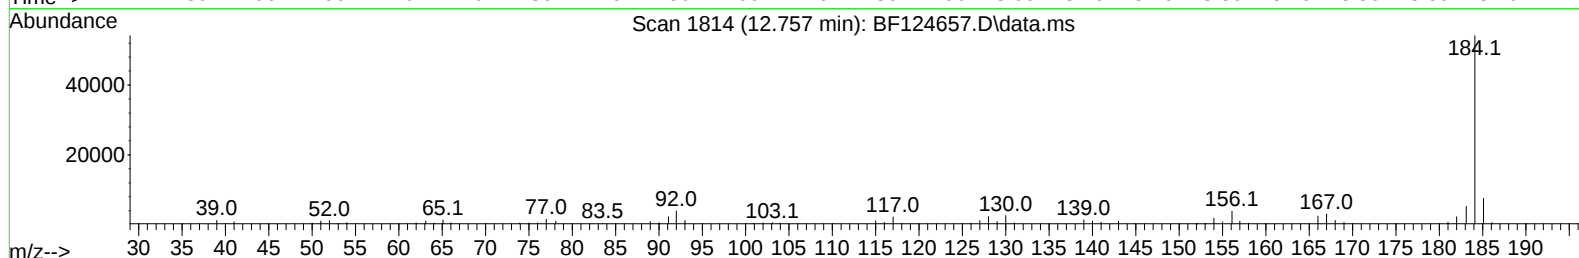


Quant Time: Jul 21 13:44:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:36:28 2021
Response via : Initial Calibration

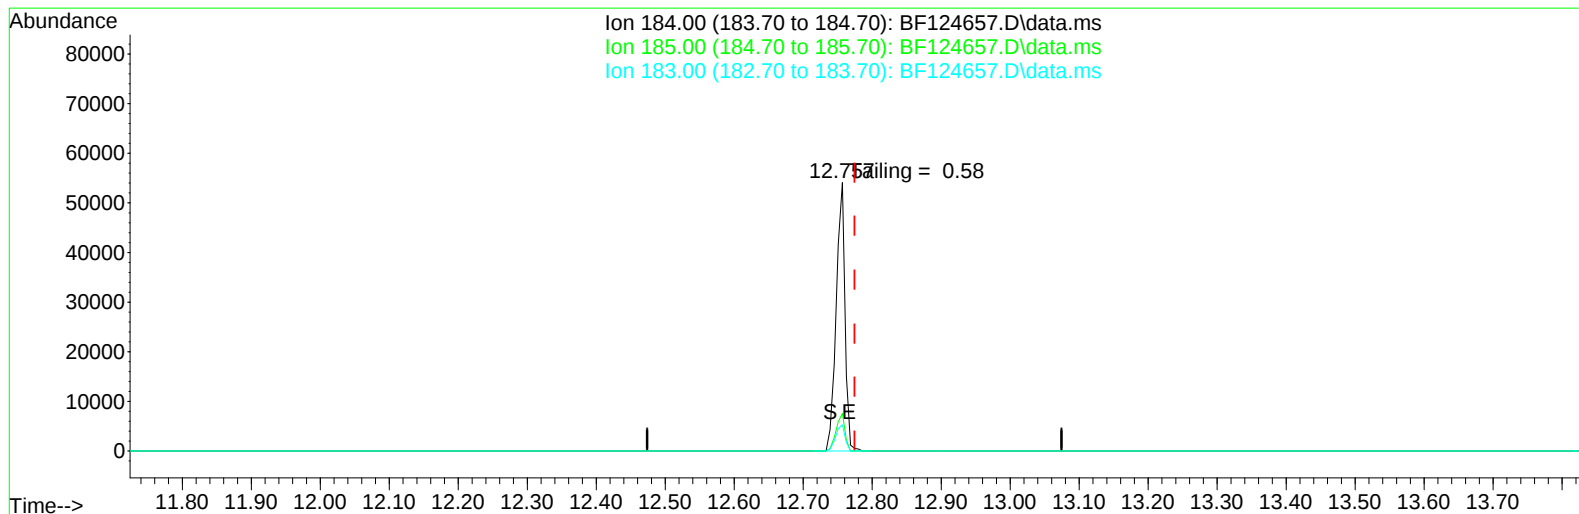

TIC: BF124657.D\data.ms

(77) Benzidine




12.757min (-0.018) 0.00 ng

response **47531**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.05
183.00	10.10	9.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072121\
Data File : BF124657.D
Acq On : 21 Jul 2021 11:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 13:44:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:36:28 2021
Response via : Initial Calibration

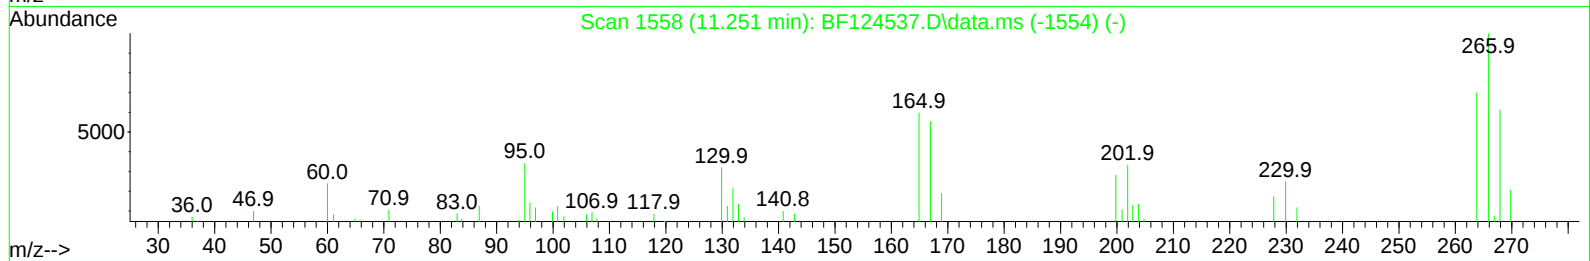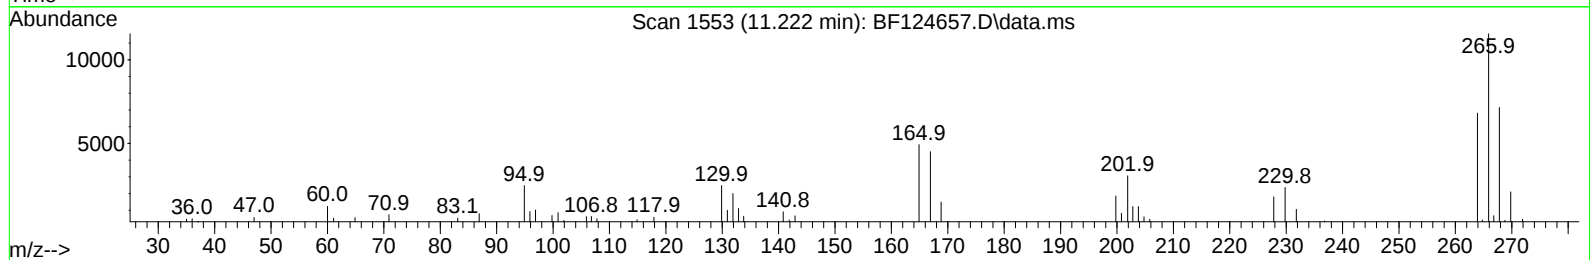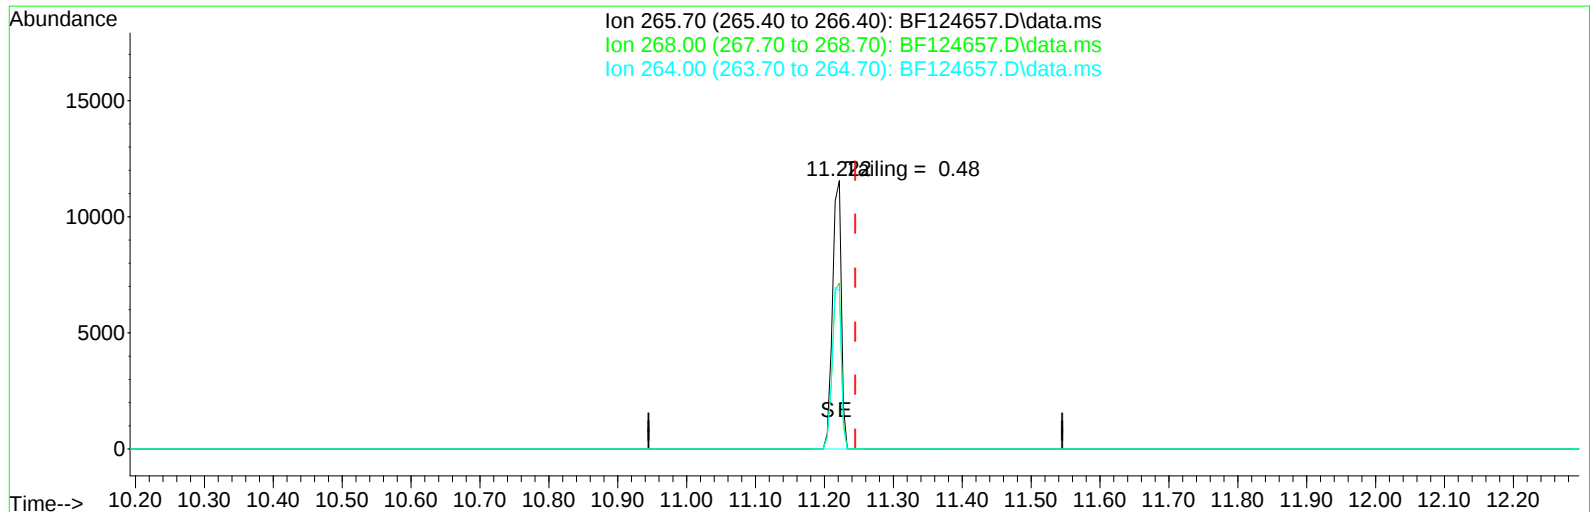

TIC: BF124657.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.023) 0.00 ng

response 10260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.86
264.00	69.90	58.94
0.00	0.00	0.00