


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072121\
 Data File : BF124664.D
 Acq On : 21 Jul 2021 16:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 16:08:04 2021

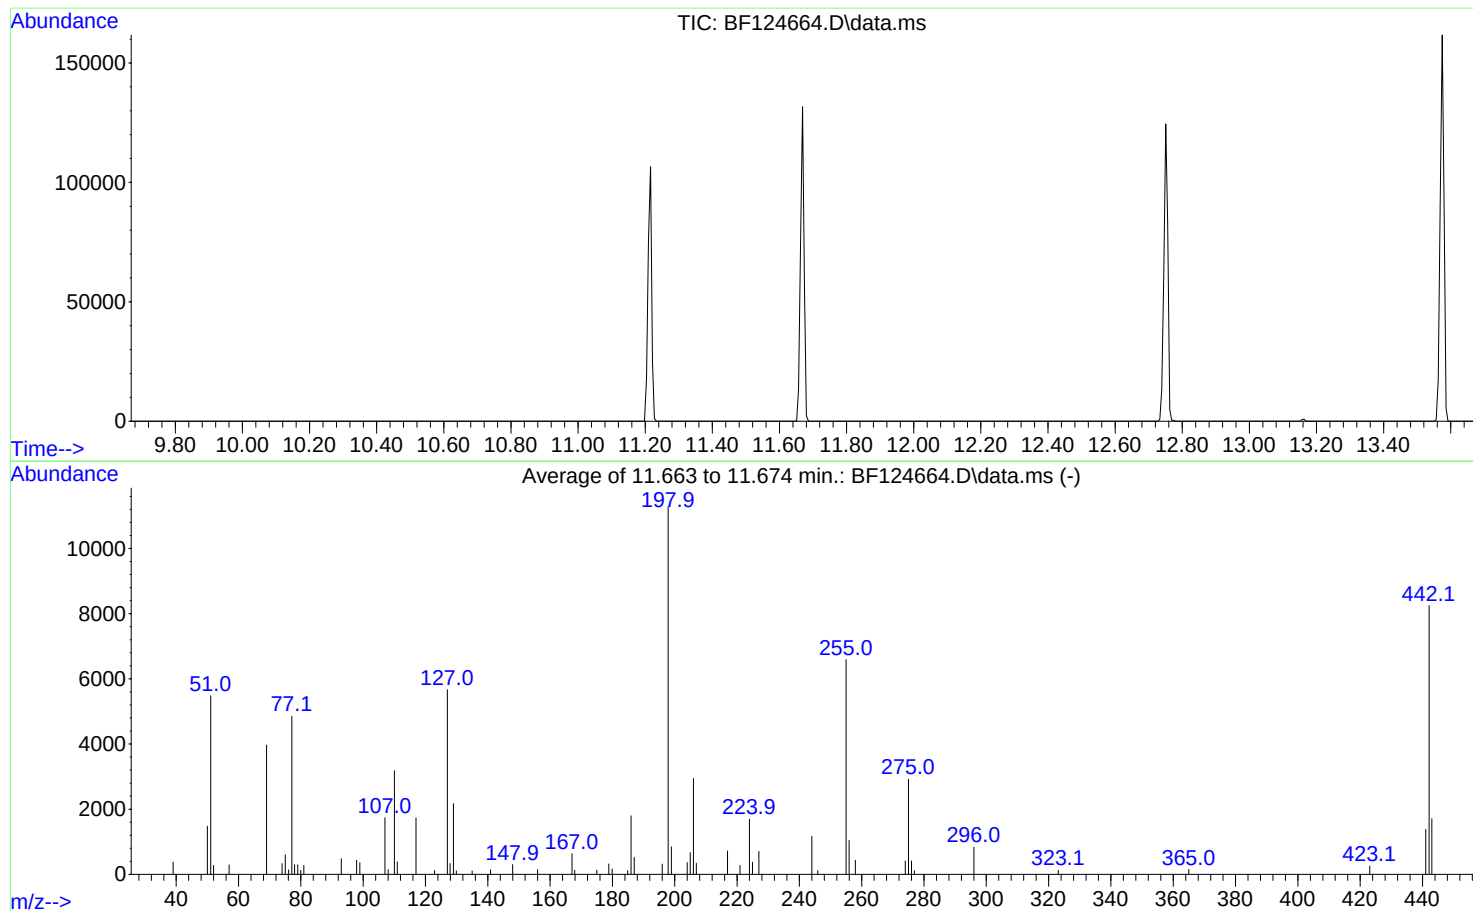




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	5482	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	3966	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	5665	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11289	PASS
199	198	5	9	7.5	847	PASS
275	198	10	60	25.9	2919	PASS
365	198	1	100	1.3	151	PASS
441	198	0.01	100	12.2	1379	PASS
442	442	50	100	100.0	8250	PASS
443	442	15	24	20.7	1710	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072121\
 Data File : BF124664.D
 Acq On : 21 Jul 2021 16:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 17:28:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 21 16:08:04 2021
 Response via : Initial Calibration

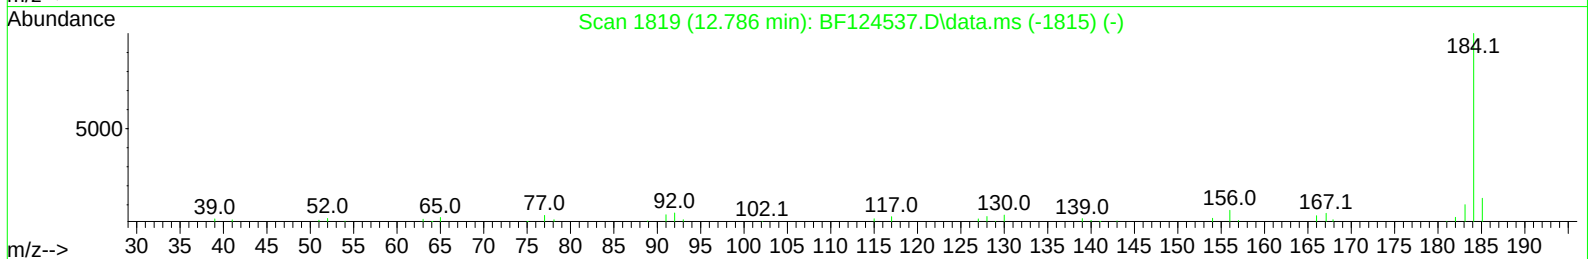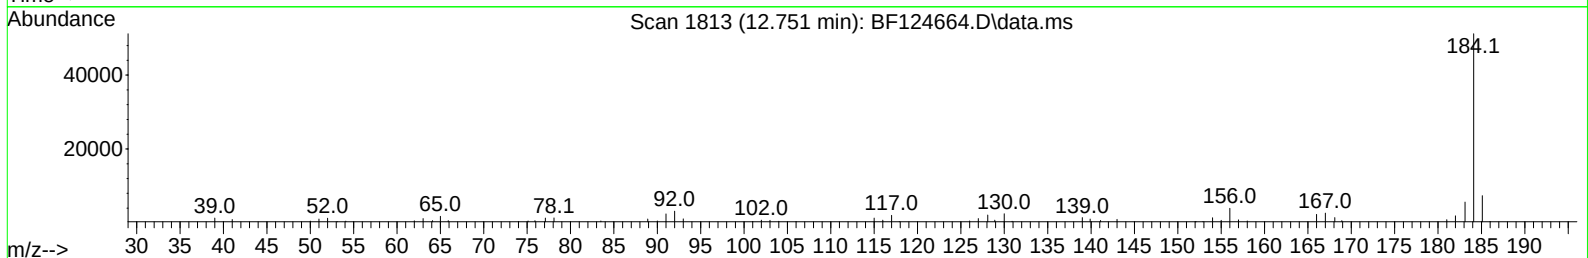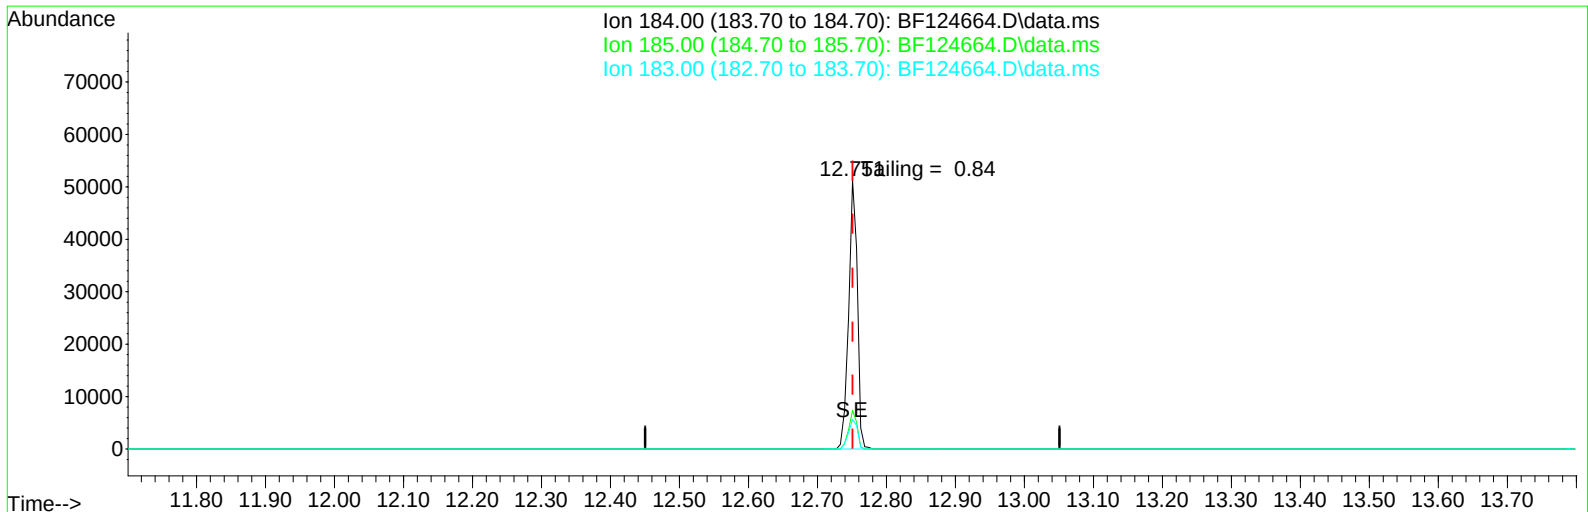

TIC: BF124664.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng




response 45043

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.39
183.00	10.10	11.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072121\
Data File : BF124664.D
Acq On : 21 Jul 2021 16:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 21 17:28:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:08:04 2021
Response via : Initial Calibration

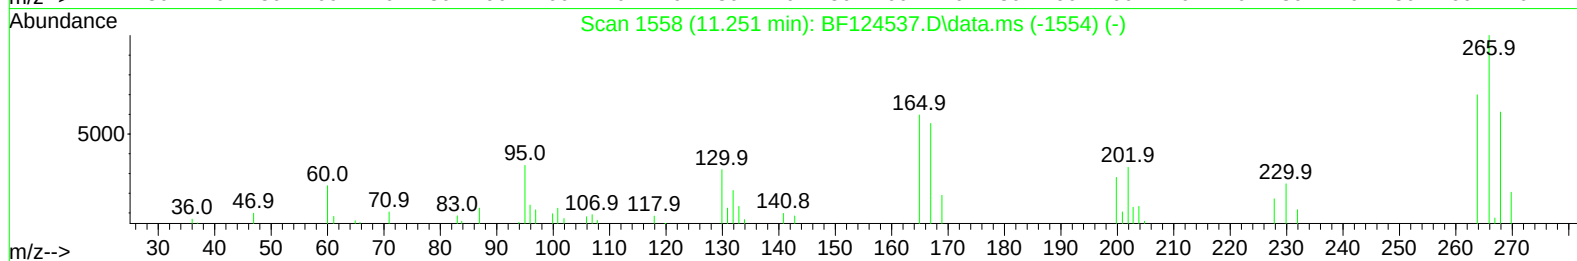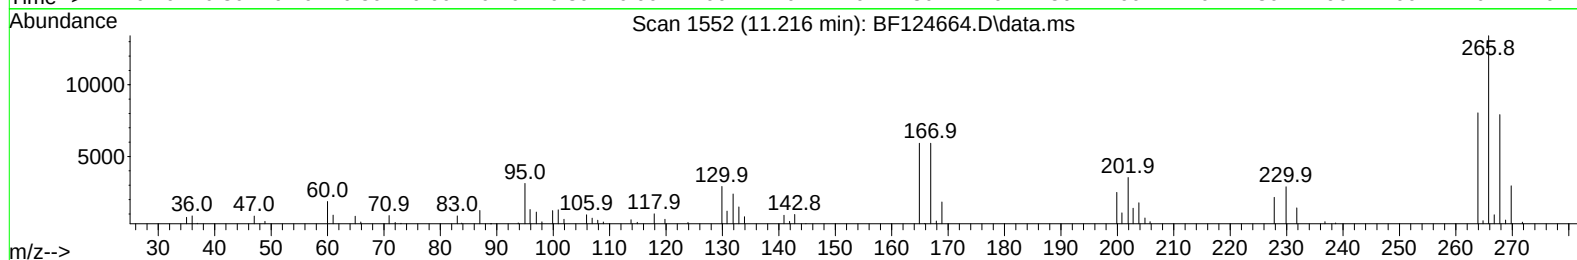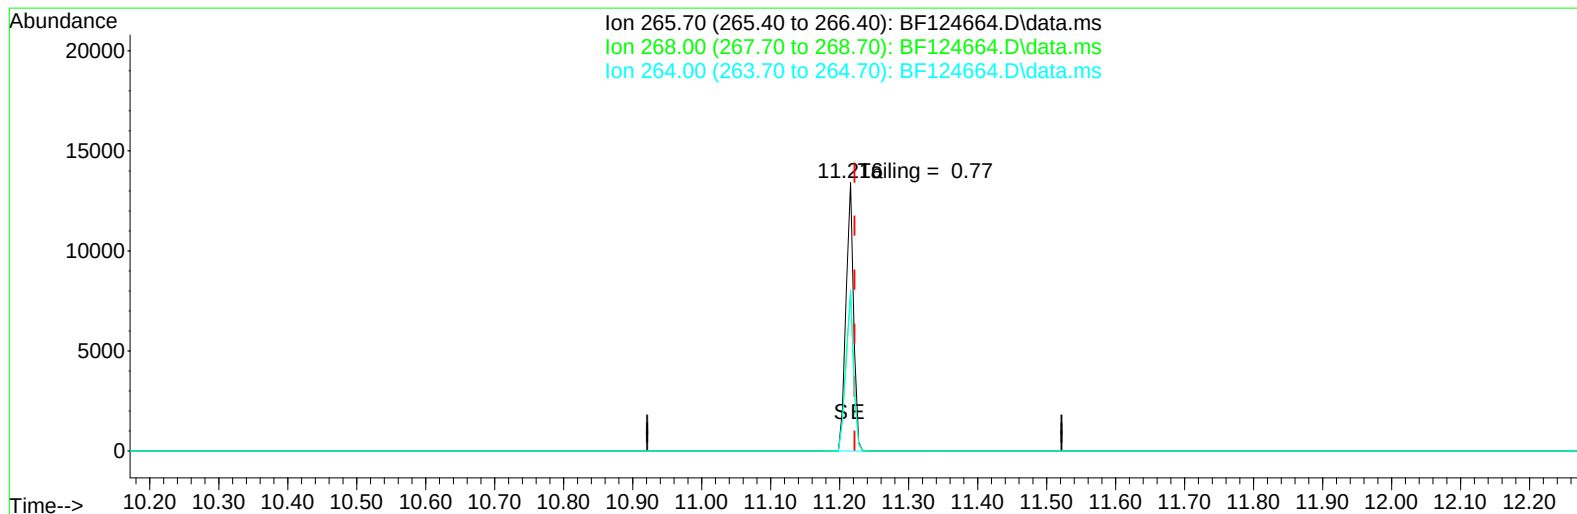

TIC: BF124664.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 0.00 ng

response 10318

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	59.01
264.00	69.90	59.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/21/2021	BNA_F	<u>BF124664.D</u>
Compound Name	Response	Retention Time
DDT	2086126000	13.57
DDD	0	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	2086126000	0.00