
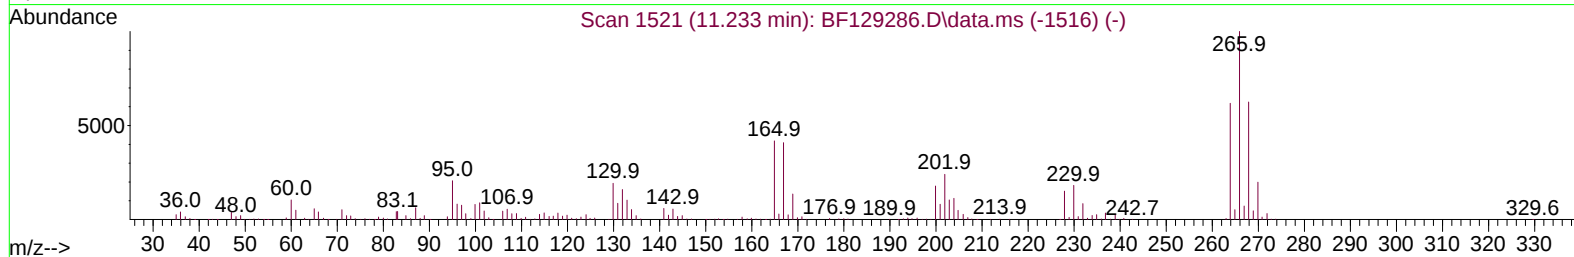
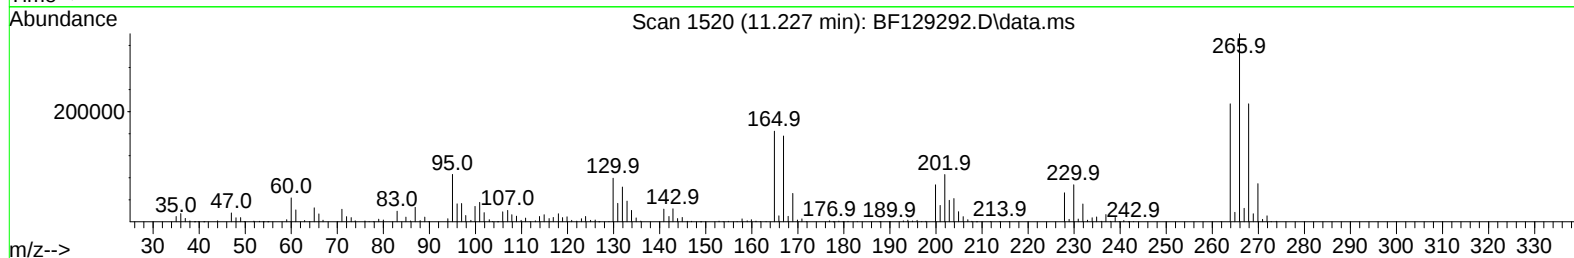


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129292.D
Acq On : 21 Jul 2022 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 14:23:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

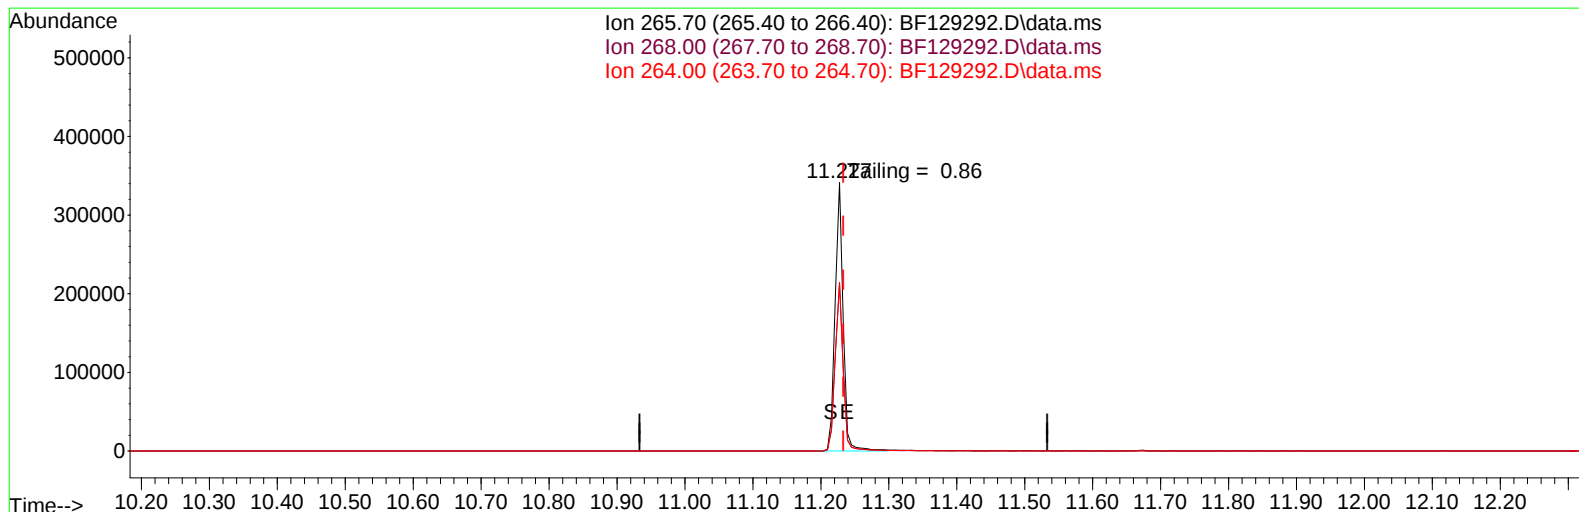

TIC: BF129292.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 334238.08 ng

response 282300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.74
264.00	61.80	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129292.D
Acq On : 21 Jul 2022 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 14:23:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

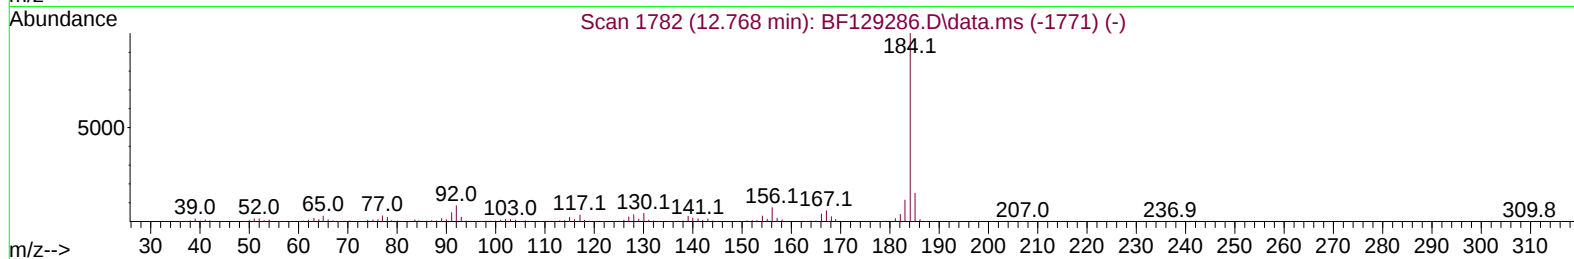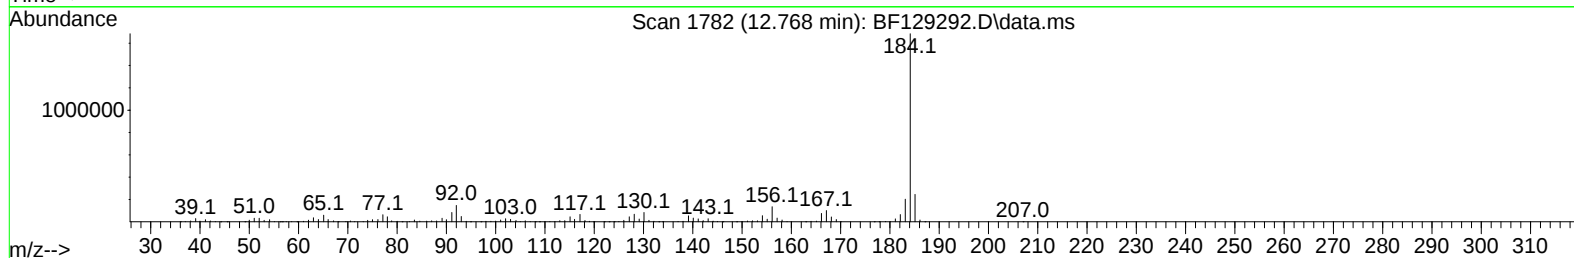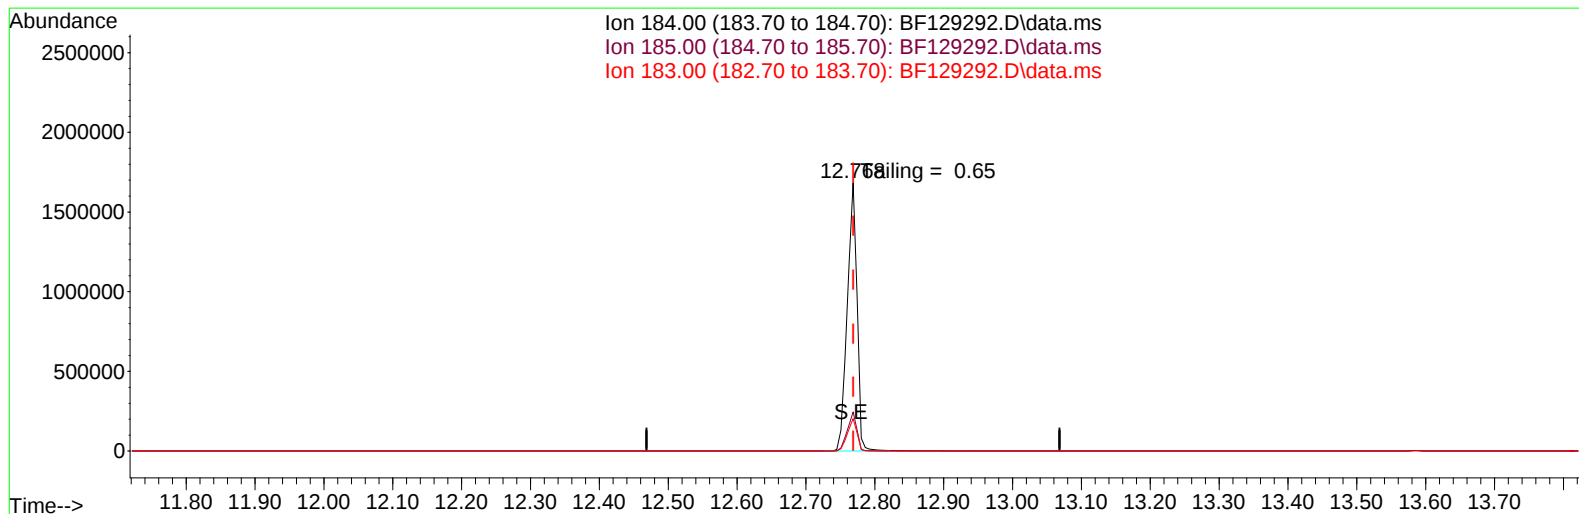

TIC: BF129292.D\data.ms

(77) Benzidine

12.768min (-0.000) 4008.96 ng m

response 1657233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.57
183.00	11.60	12.05
0.00	0.00	0.00