

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
 Data File : BF129294.D
 Acq On : 21 Jul 2022 13:11
 Operator : CG\JU
 Sample : PB145921BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145921BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	545	551	554	rBV	4705939	5154890	78.82%	13.162%
2	6.522	714	720	723	rBV	4664862	5225973	79.91%	13.344%
3	6.892	779	783	787	rBV	1323750	1053742	16.11%	2.691%
4	7.457	873	879	882	rBV	3299170	3446752	52.70%	8.801%
5	8.175	996	1001	1005	rBV	1596509	1418581	21.69%	3.622%
6	9.251	1178	1184	1187	rBV	6170005	6176092	94.43%	15.770%
7	9.933	1294	1300	1303	rBV	1982458	1613705	24.67%	4.120%
8	10.727	1428	1435	1438	rBV	4512533	4186001	64.01%	10.688%
9	11.422	1549	1553	1557	rBV	1811012	1653652	25.28%	4.222%
10	13.016	1819	1824	1827	rBV	6800827	6540059	100.00%	16.699%
11	14.068	1999	2003	2007	rBV	1652234	1443518	22.07%	3.686%
12	15.562	2251	2257	2266	rBV	999916	1250780	19.12%	3.194%




Sum of corrected areas: 39163745

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129294.D
Acq On : 21 Jul 2022 13:11
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

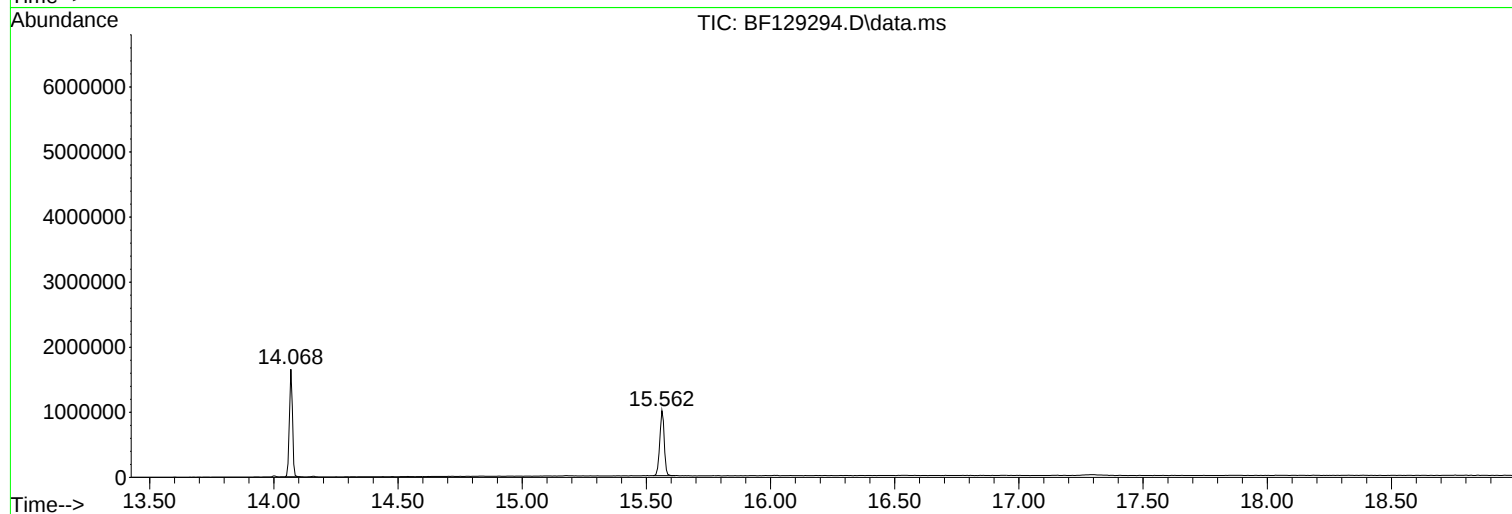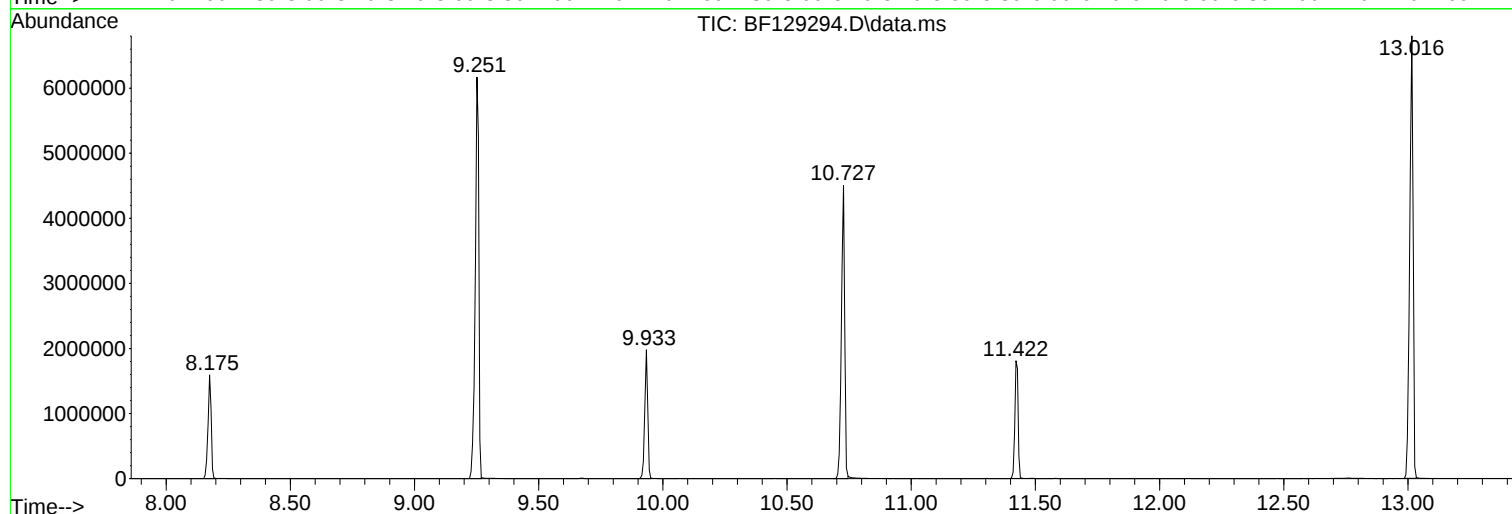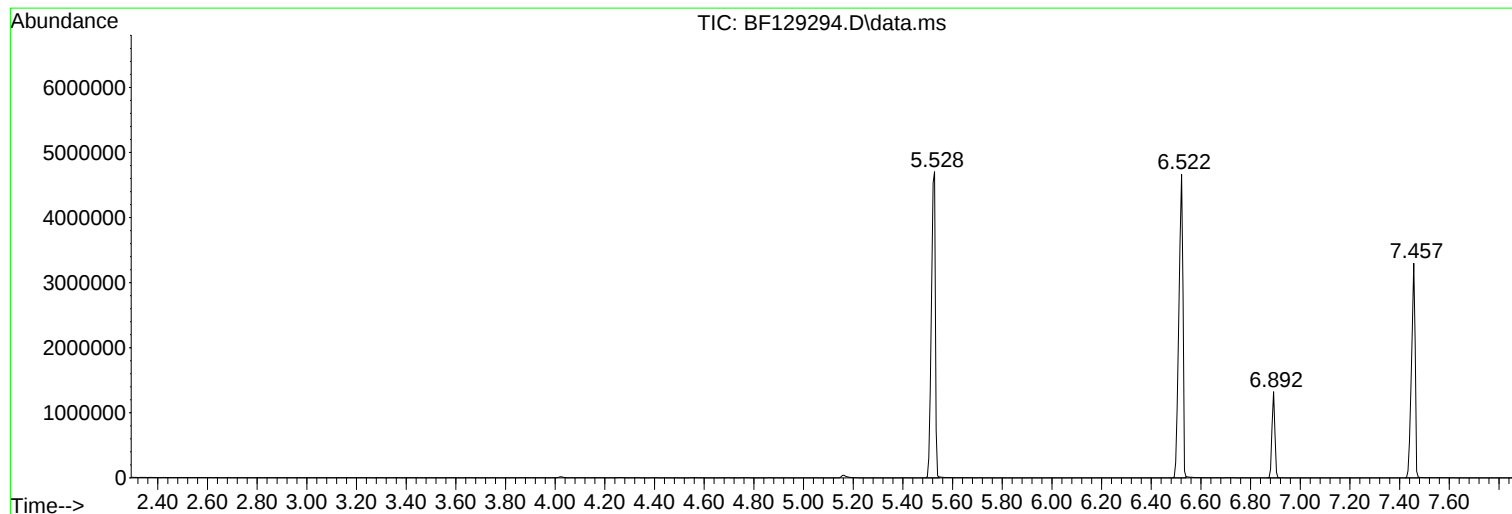

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129294.D
Acq On : 21 Jul 2022 13:11
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129294.D
Acq On : 21 Jul 2022 13:11
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------