

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
 Data File : BF129299.D
 Acq On : 21 Jul 2022 16:34
 Operator : CG\JU
 Sample : PB145925BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145925BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	545	551	554	rBV	4379798	4813369	78.12%	13.169%
2	6.522	714	720	723	rBV	4403147	4885819	79.29%	13.367%
3	6.892	779	783	786	rBV	1243191	975056	15.82%	2.668%
4	7.457	873	879	882	rBV	3131533	3206369	52.04%	8.772%
5	8.175	996	1001	1004	rBV	1524873	1321254	21.44%	3.615%
6	9.251	1178	1184	1187	rBV	5913825	5799735	94.12%	15.868%
7	9.933	1294	1300	1303	rBV	1778037	1494420	24.25%	4.089%
8	10.727	1428	1435	1438	rBV	4214105	3939645	63.94%	10.779%
9	11.421	1549	1553	1557	rBV	1810610	1507195	24.46%	4.124%
10	13.015	1819	1824	1827	rBV	6415820	6161747	100.00%	16.858%
11	14.068	1999	2003	2006	rBV	1481155	1315386	21.35%	3.599%
12	15.562	2251	2257	2265	rBV	918816	1130933	18.35%	3.094%




Sum of corrected areas: 36550928

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129299.D
Acq On : 21 Jul 2022 16:34
Operator : CG\JU
Sample : PB145925BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145925BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

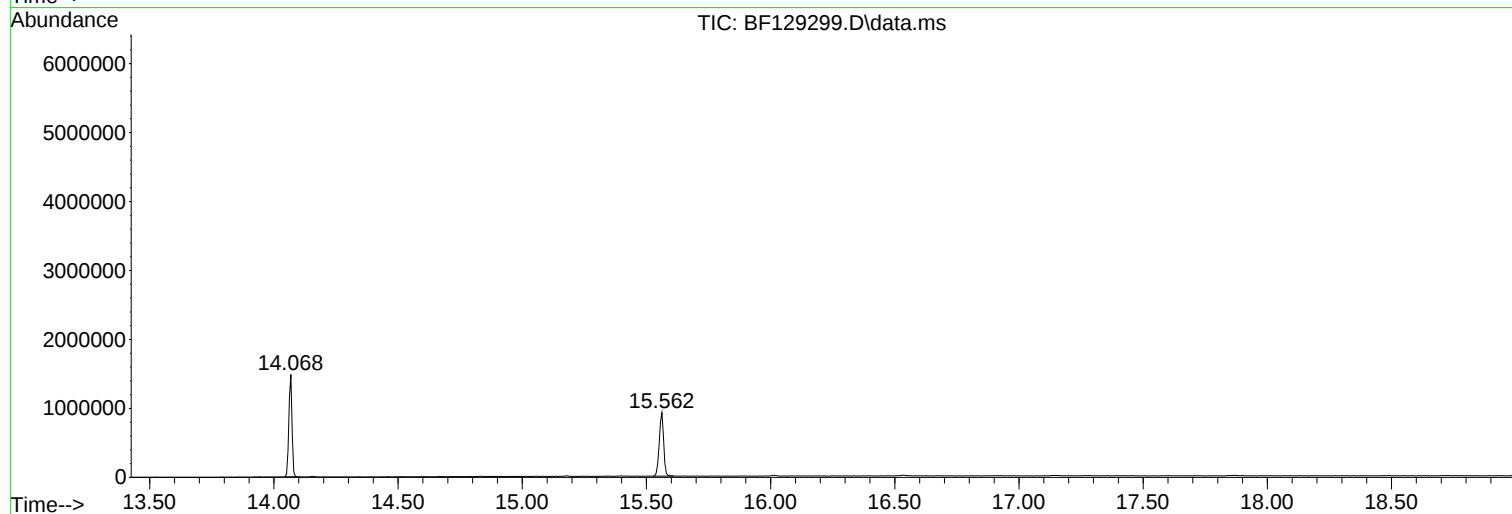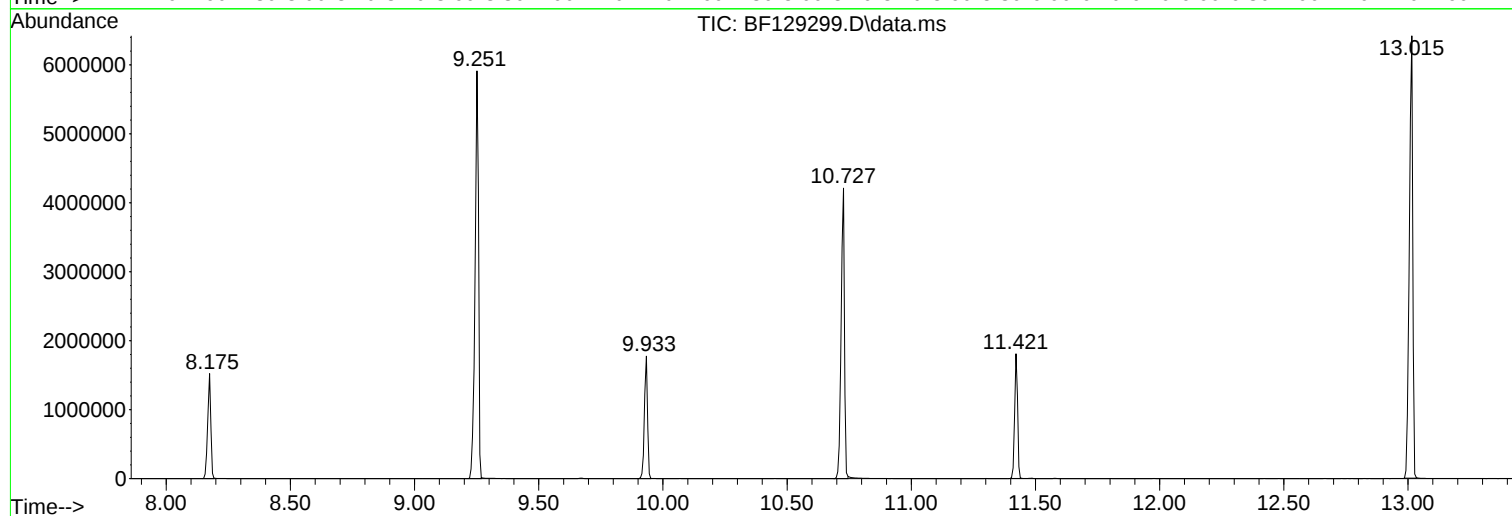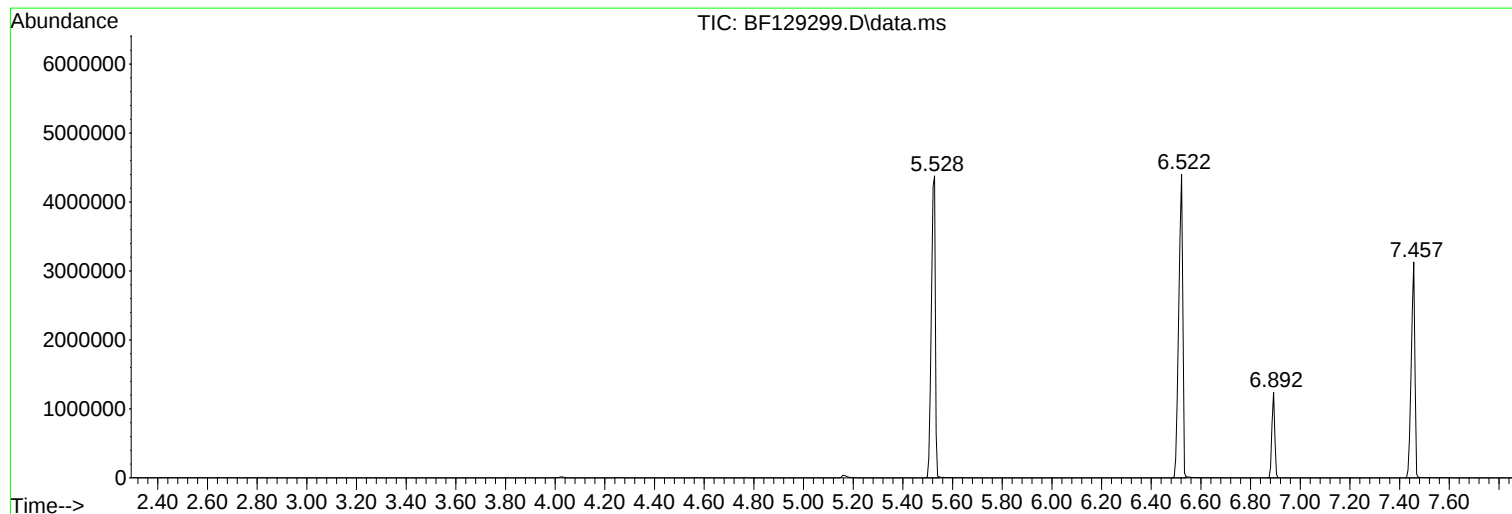

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129299.D
Acq On : 21 Jul 2022 16:34
Operator : CG\JU
Sample : PB145925BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145925BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129299.D
Acq On : 21 Jul 2022 16:34
Operator : CG\JU
Sample : PB145925BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145925BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------