


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
 Data File : BF129292.D
 Acq On : 21 Jul 2022 12:06
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 13:42:18 2022

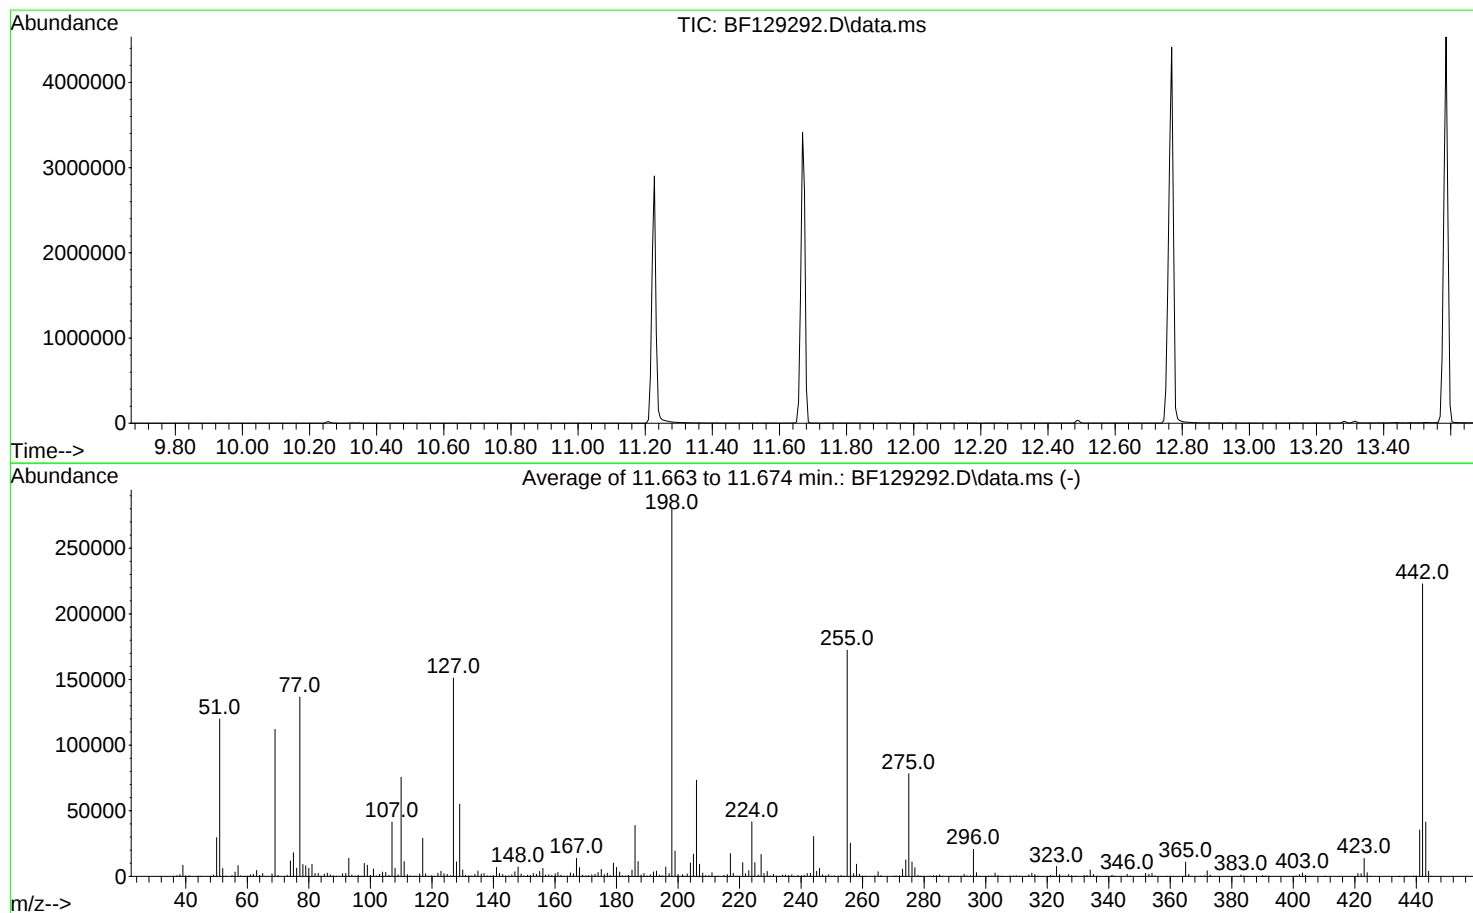




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	119907	PASS
68	69	0.00	2	1.7	1925	PASS
69	198	0.00	100	40.0	112104	PASS
70	69	0.00	2	0.7	738	PASS
127	198	10	80	53.9	151160	PASS
197	198	0.00	2	0.8	2247	PASS
198	198	100	100	100.0	280299	PASS
199	198	5	9	6.9	19258	PASS
275	198	10	60	27.9	78259	PASS
365	198	1	100	3.9	10918	PASS
441	198	0.01	100	12.6	35335	PASS
442	442	50	100	100.0	222816	PASS
443	442	15	24	18.5	41280	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
 Data File : BF129292.D
 Acq On : 21 Jul 2022 12:06
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 14:23:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 13:42:18 2022
 Response via : Initial Calibration

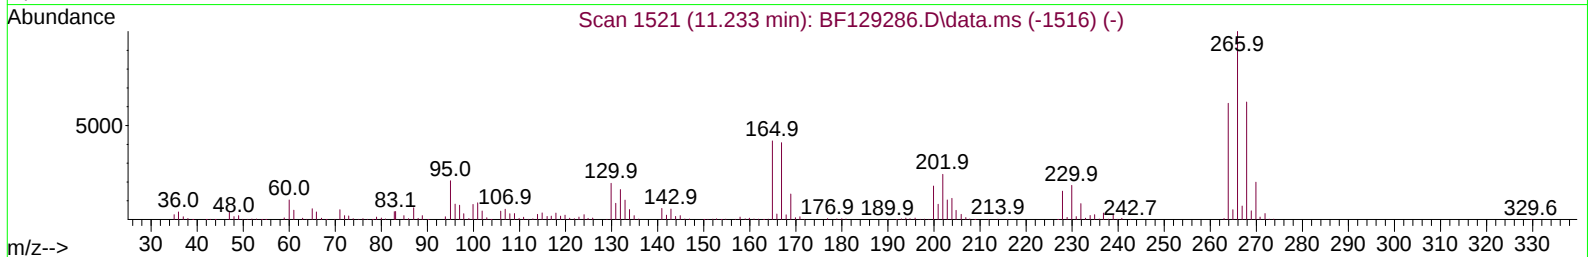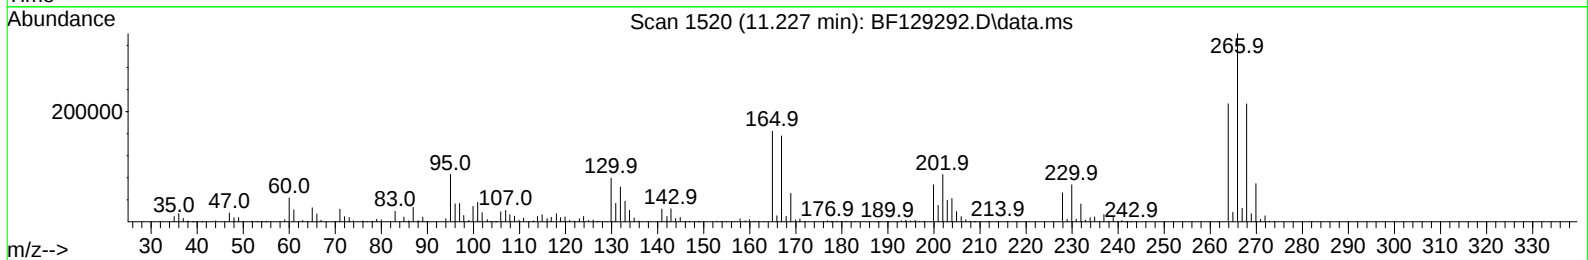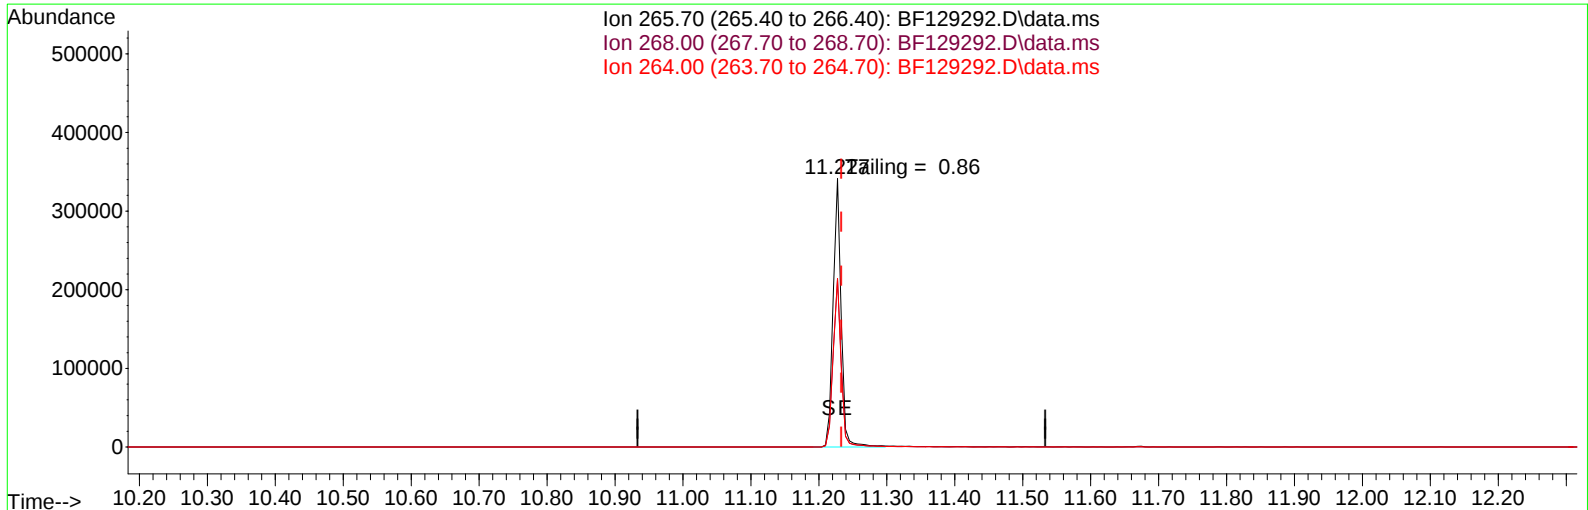

TIC: BF129292.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 334238.08 ng




response 282300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.74
264.00	61.80	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072122\
Data File : BF129292.D
Acq On : 21 Jul 2022 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 21 14:23:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

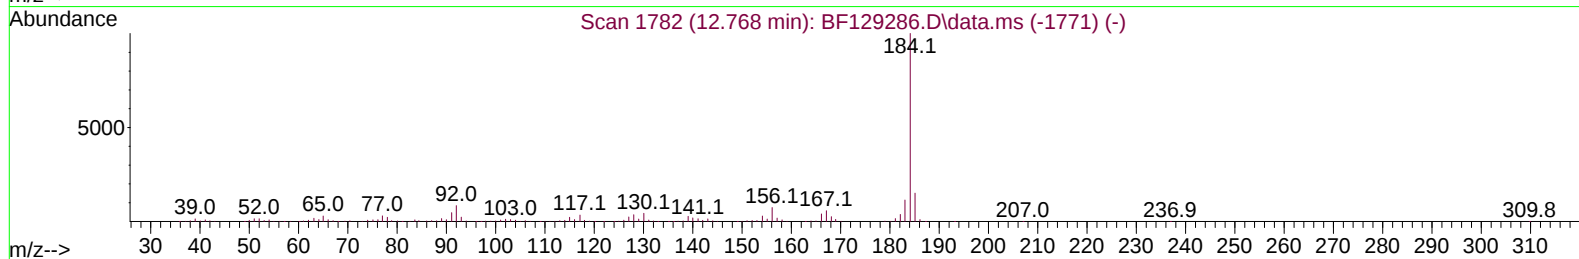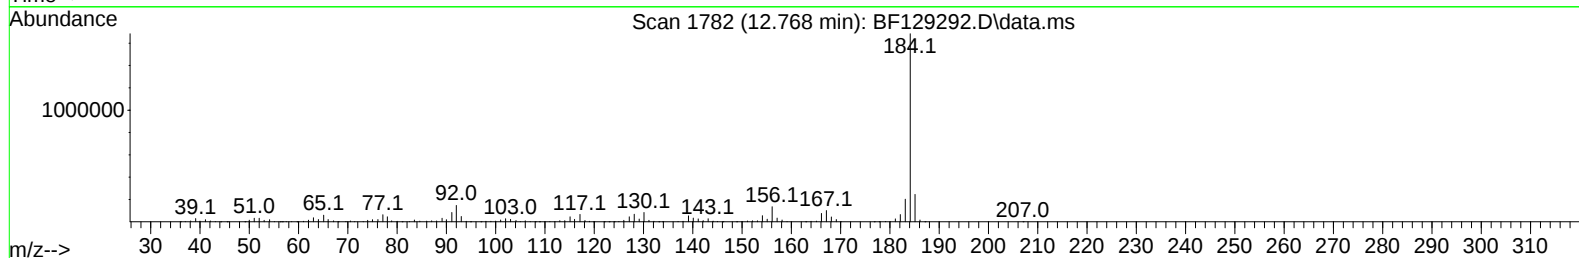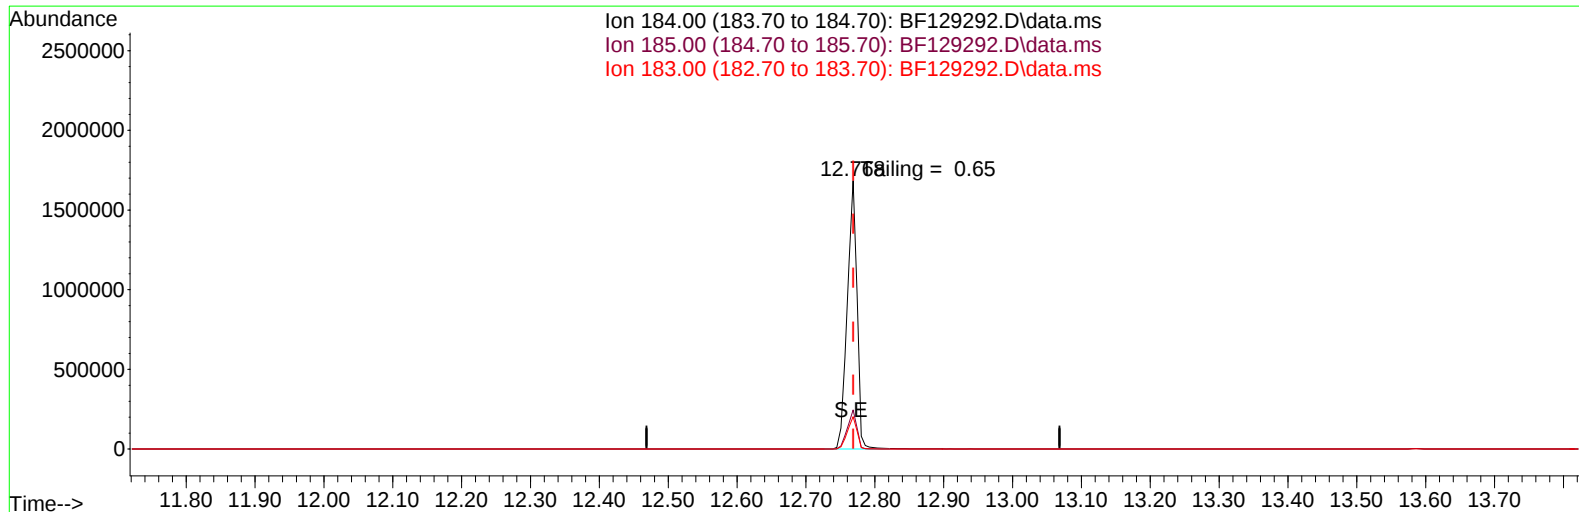

TIC: BF129292.D\data.ms

(77) Benzidine

12.768min (-0.000) 4008.96 ng m

response 1657233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.57
183.00	11.60	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/21/2022	BNA_F	<u>BF129292.D</u>
Compound Name	Response	Retention Time
DDT	706635	13.58
DDD	3310	13.28
DDE	192	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3502	710137	0.49

Instrument :
BNA_F
ClientSampleId :
DFTPP