

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072215\
 Data File : BF080574.D
 Acq On : 23 Jul 2015 1:06
 Operator : TP/UM
 Sample : G3027-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-03-12.5-13.0

Quant Time: Jul 23 06:28:01 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 23 05:13:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	34786	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	131529	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	55779	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	101405	20.00	ng	0.00
75) Chrysene-d12	14.31	240	65828	20.00	ng	-0.01
86) Perylene-d12	15.99	264	40026	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	296392	151.10	ng	0.01
7) Phenol-d6	6.57	99	426401	176.50	ng	0.00
23) Nitrobenzene-d5	7.52	82	232336	113.78	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	74562	176.09	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	404450	104.27	ng	0.00
78) Terphenyl-d14	13.13	244	362340	112.88	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.72	163	58405	14.91	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072215\
Data File : BF080574.D
Acq On : 23 Jul 2015 1:06
Operator : TP/UM
Sample : G3027-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-03-12.5-13.0

Quant Time: Jul 23 06:28:01 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 23 05:13:42 2015
Response via : Initial Calibration

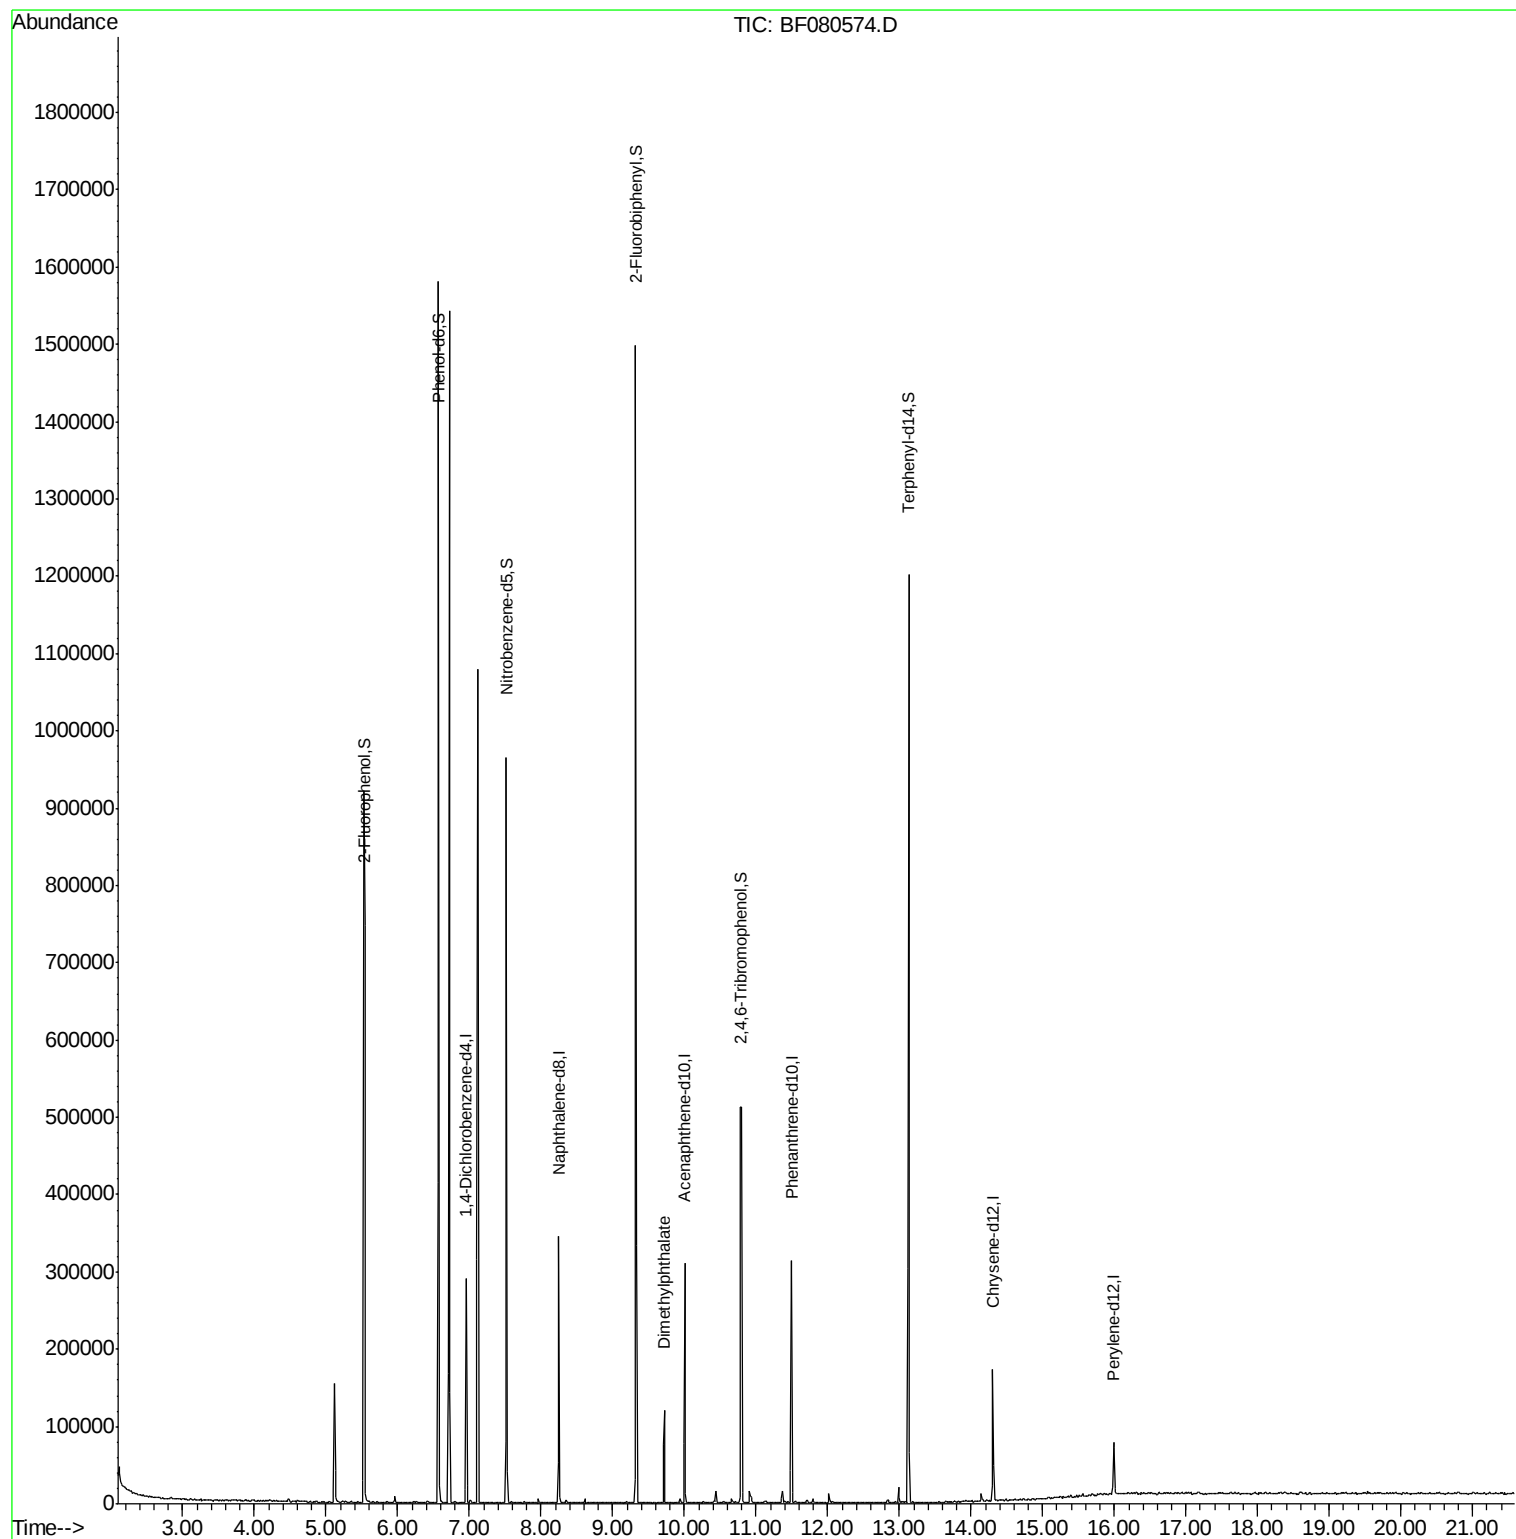


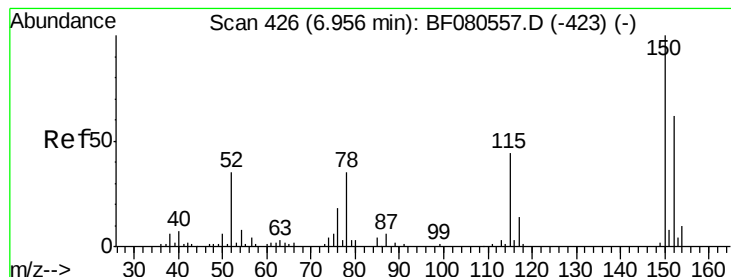




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.96 min Scan# 426
 Delta R.T. 0.00 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-03-12.5-13.0

Tgt Ion:152 Resp: 34786
 Ion Ratio Lower Upper
 152 100
 150 160.6 128.7 193.1
 115 65.6 56.8 85.2

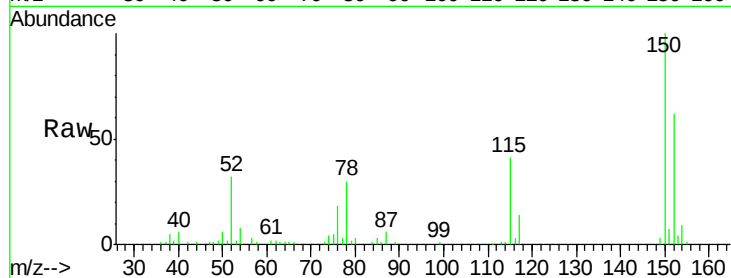


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

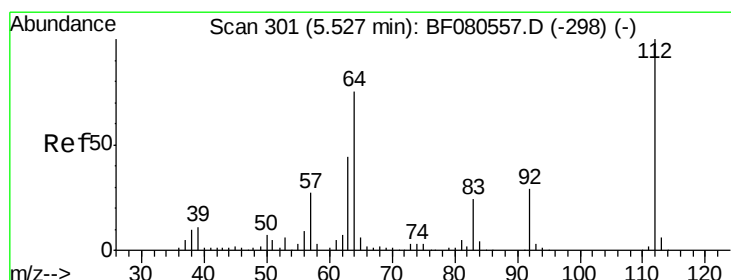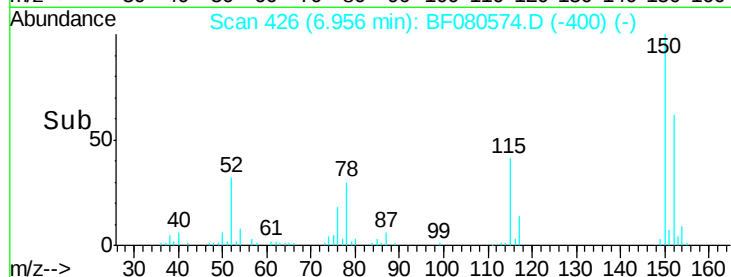
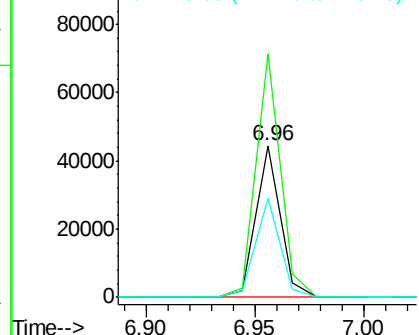



#5
 2-Fluorophenol
 Concen: 151.10 ng
 RT: 5.54 min Scan# 302
 Delta R.T. 0.01 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Tgt Ion:112 Resp: 296392
 Ion Ratio Lower Upper
 112 100
 64 53.7 60.2 90.2#
 63 30.9 34.8 52.2#

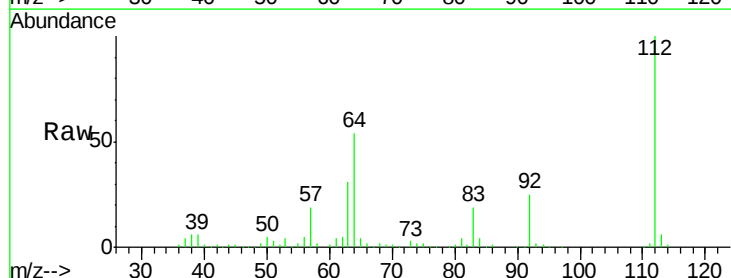

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

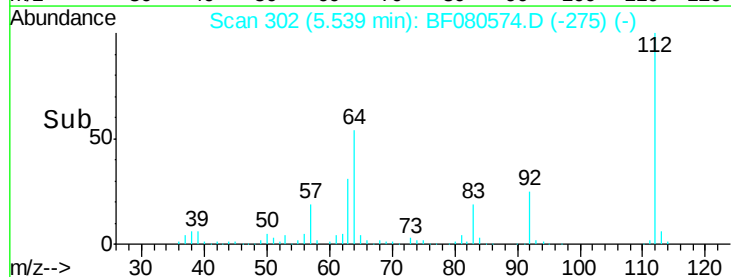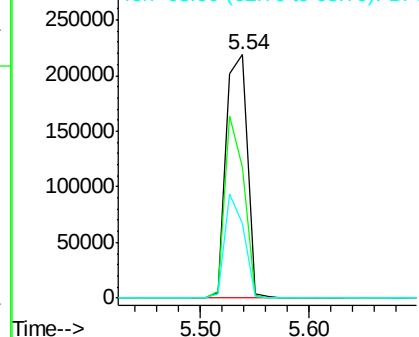

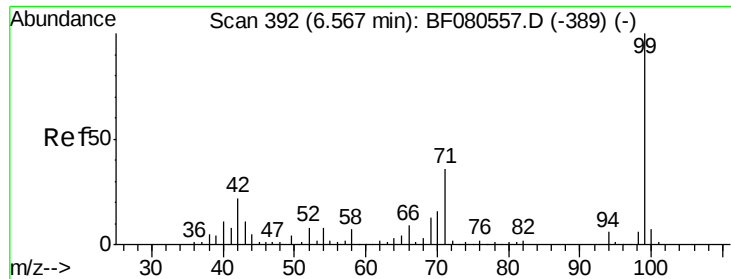

#7

Phenol-d6

Concen: 176.50 ng

RT: 6.57 min Scan# 392

Delta R.T. -0.00 min

Lab File: BF080574.D

Acq: 23 Jul 2015 1:06

Instrument :

BNA_F

ClientSampleId :

SB-03-12.5-13.0





Tgt Ion: 99 Resp: 426401

Ion Ratio Lower Upper

99 100

42 23.7 17.4 26.2

71 40.4 29.0 43.6

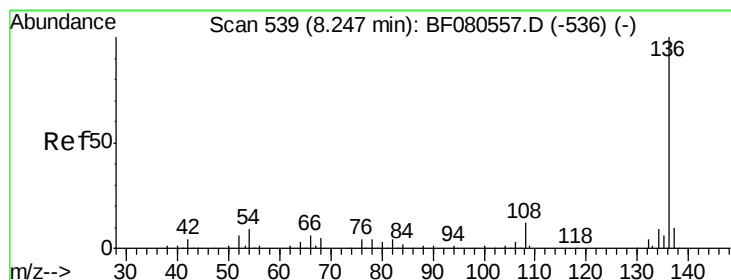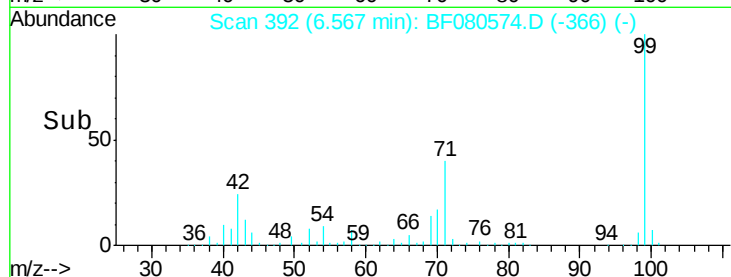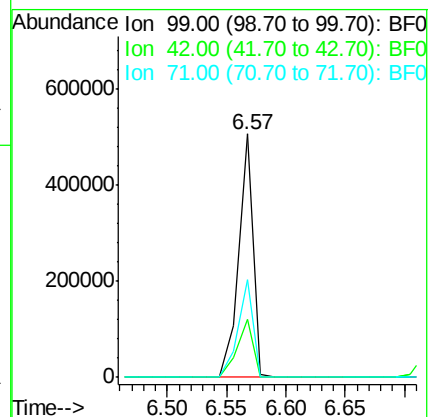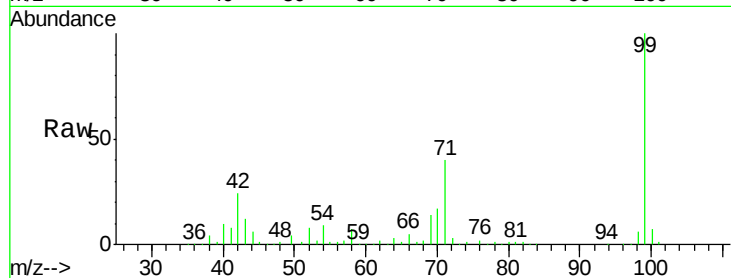

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.25 min Scan# 539

Delta R.T. -0.00 min

Lab File: BF080574.D

Acq: 23 Jul 2015 1:06

Tgt Ion: 136 Resp: 131529




Ion Ratio Lower Upper


136 100

137 10.0 7.8 11.8

54 8.6 7.2 10.8

68 4.1 3.8 5.6

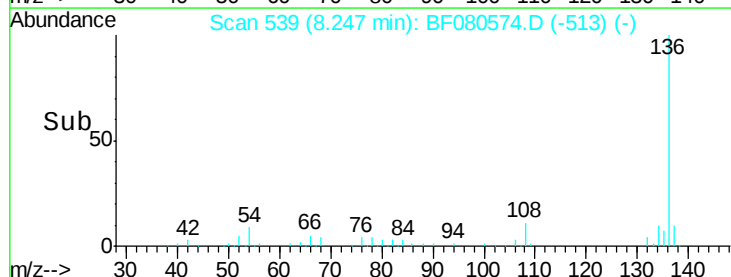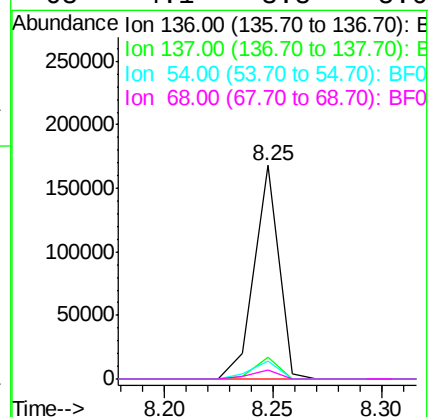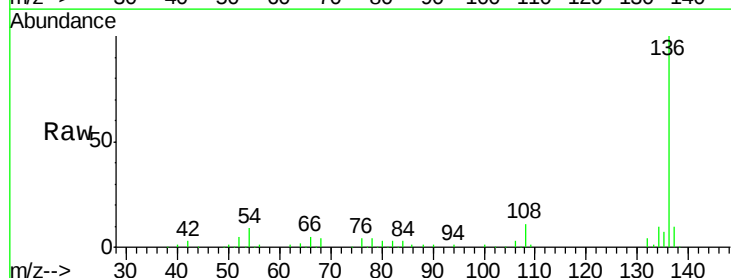


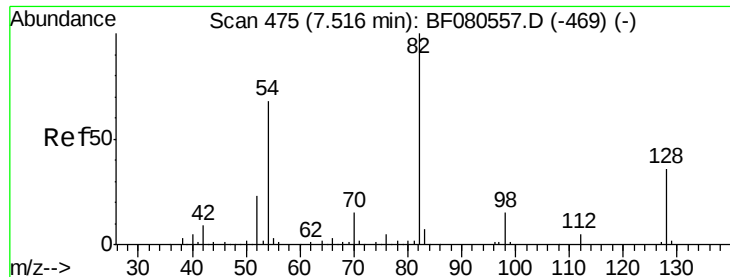




#23
 Nitrobenzene-d5
 Concen: 113.78 ng
 RT: 7.52 min Scan# 475
 Delta R.T. 0.00 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-03-12.5-13.0

Tgt Ion	Ratio	Lower	Upper
82	100		
128	35.6	28.9	43.3
54	63.9	54.5	81.7

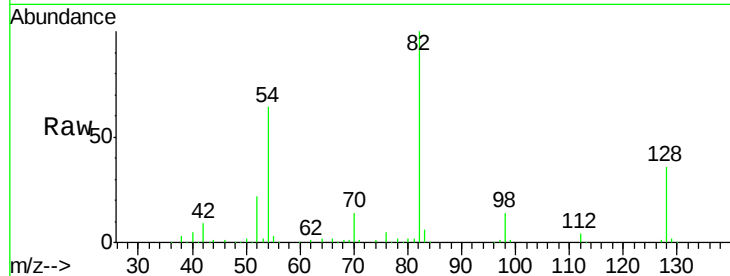


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

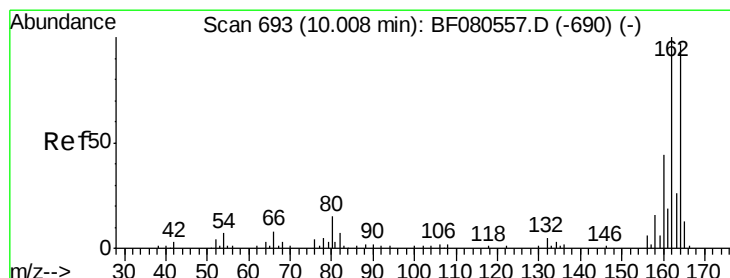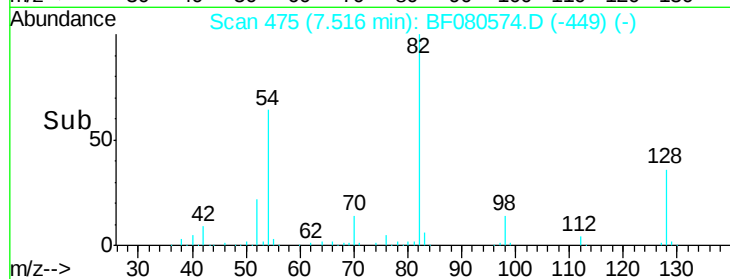
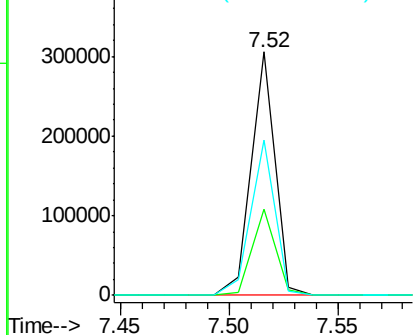



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.01 min Scan# 693
 Delta R.T. 0.00 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Tgt Ion	Ratio	Lower	Upper
164	100		
162	113.1	82.2	123.4
160	49.1	36.1	54.1

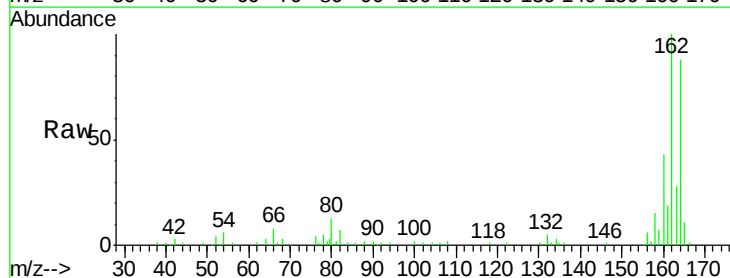

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

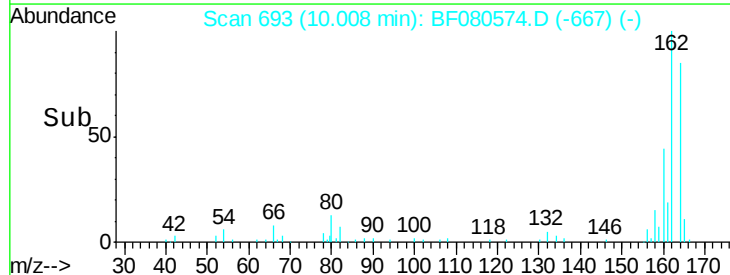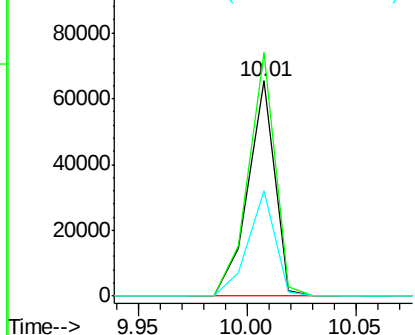


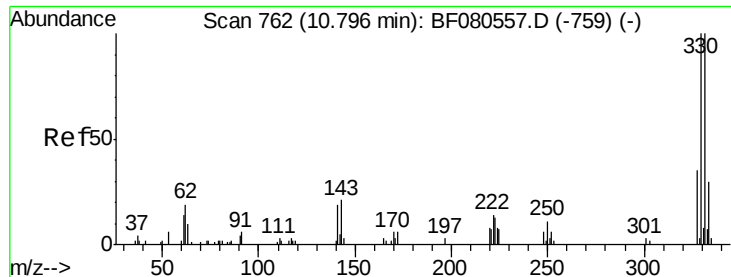

#41
 2,4,6-Tribromophenol
 Concen: 176.09 ng
 RT: 10.80 min Scan# 762
 Delta R.T. 0.00 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-03-12.5-13.0

Tgt Ion	Ratio	Lower	Upper
330	100		
332	98.7	78.3	117.5
141	45.5	37.9	56.9



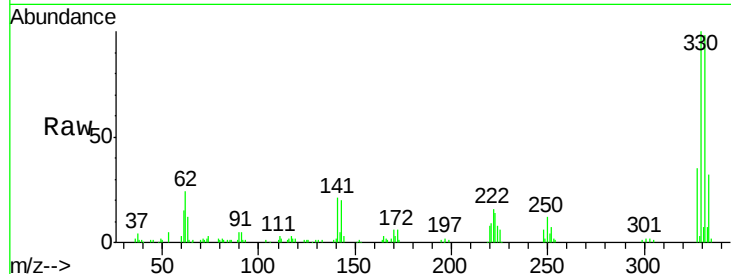


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

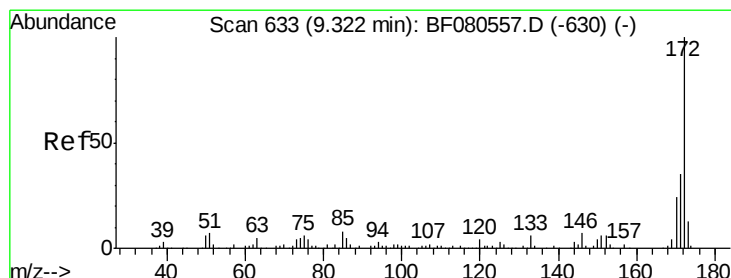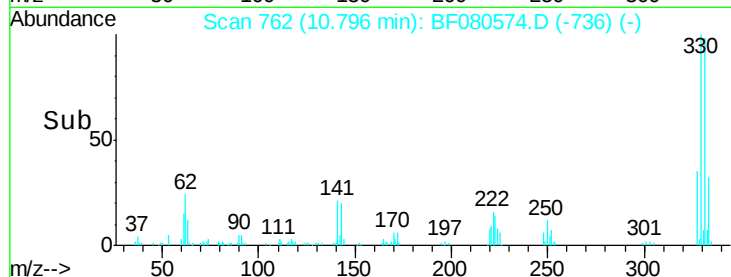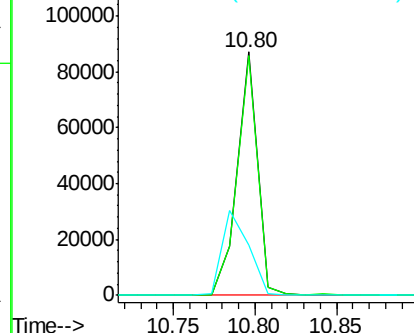

#44
 2-Fluorobiphenyl
 Concen: 104.27 ng
 RT: 9.32 min Scan# 633
 Delta R.T. 0.00 min
 Lab File: BF080574.D
 Acq: 23 Jul 2015 1:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	27.7	41.5
170	25.1	19.1	28.7


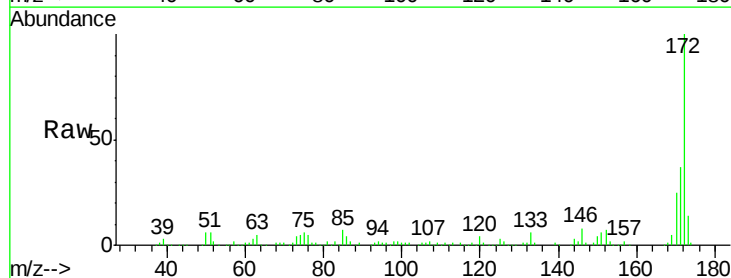



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

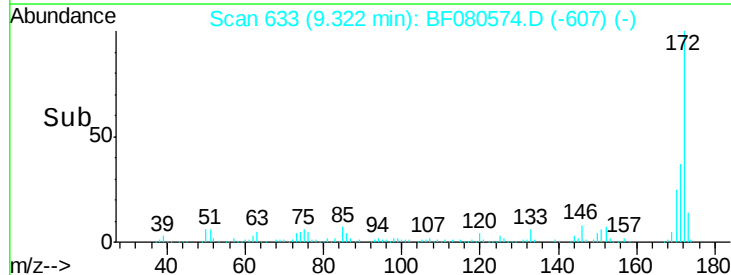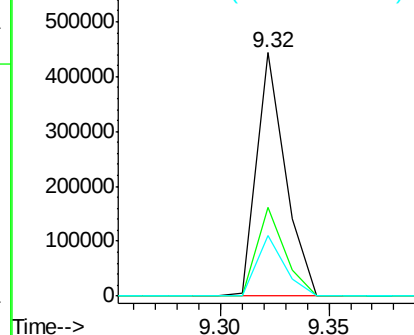


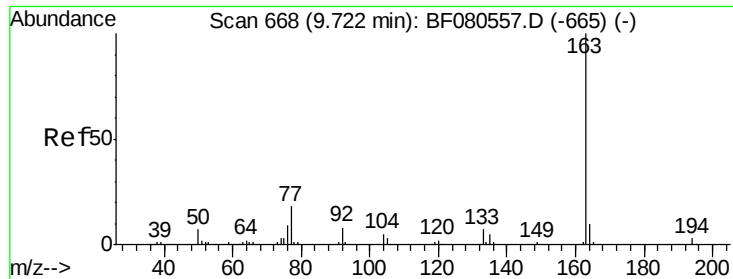




#49
Dimethylphthalate
Concen: 14.91 ng
RT: 9.72 min Scan# 668
Delta R.T. 0.00 min
Lab File: BF080574.D
Acq: 23 Jul 2015 1:06

Instrument :
BNA_F
ClientSampleId :
SB-03-12.5-13.0

Tgt Ion:163 Resp: 58405
Ion Ratio Lower Upper
163 100
194 4.2 2.5 3.7#
164 9.1 8.1 12.1

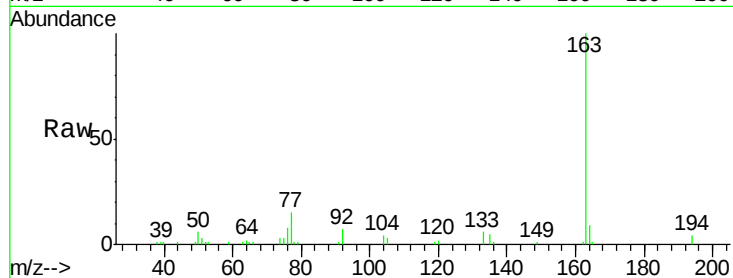


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

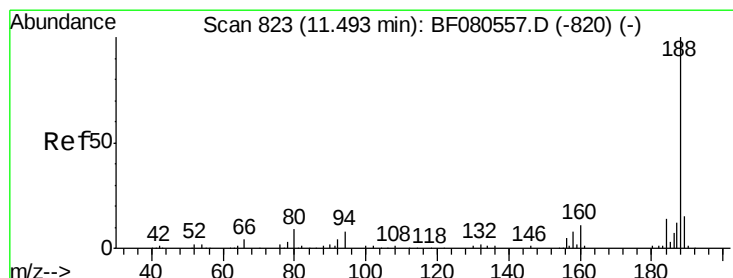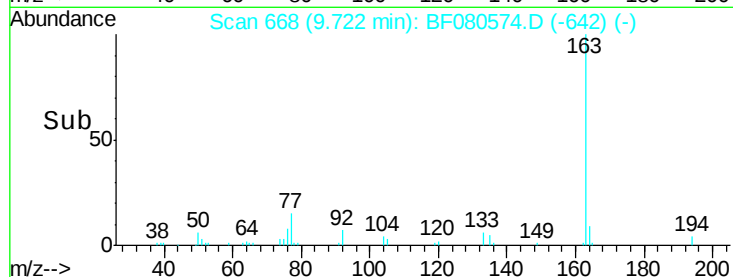
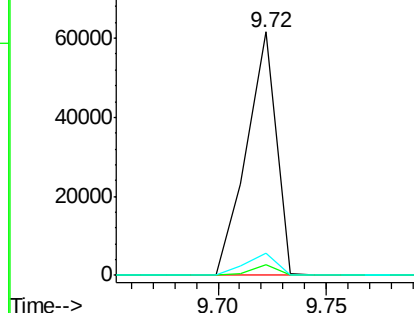



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.49 min Scan# 823
Delta R.T. -0.00 min
Lab File: BF080574.D
Acq: 23 Jul 2015 1:06

Tgt Ion:188 Resp: 101405
Ion Ratio Lower Upper
188 100
94 7.2 6.1 9.1
80 8.3 7.0 10.6

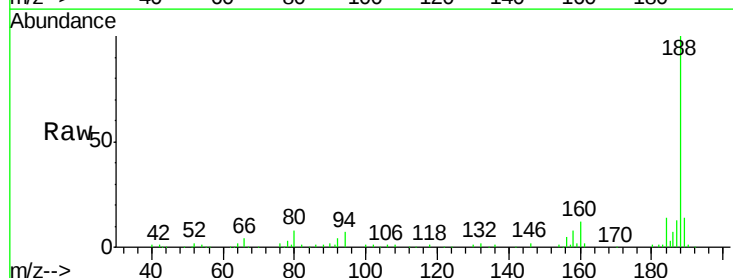

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

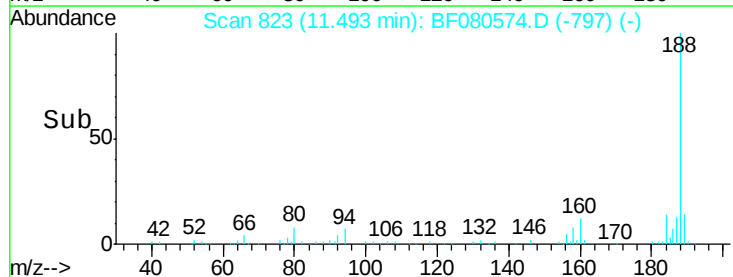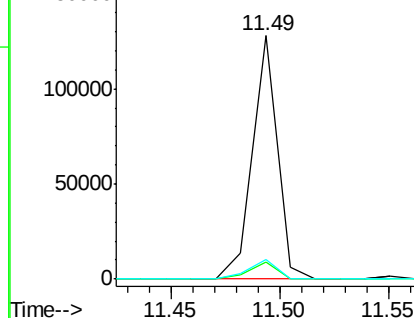

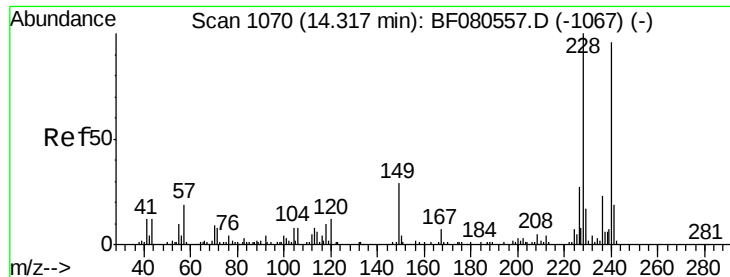

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.31 min Scan# 1069

Delta R.T. -0.01 min

Lab File: BF080574.D

Acq: 23 Jul 2015 1:06

Instrument :

BNA_F

ClientSampleId :

SB-03-12.5-13.0


Tgt Ion:240 Resp: 65828

Ion Ratio Lower Upper

240 100

120 9.0 9.9 14.9#




236 23.9 19.1 28.7

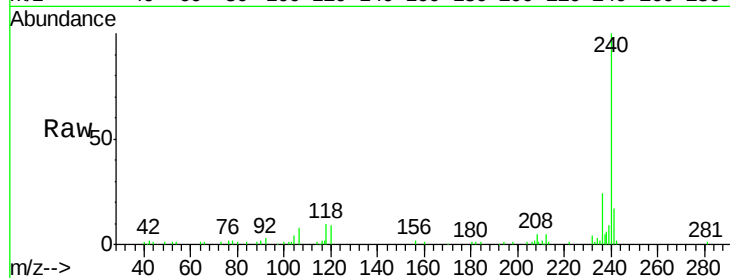

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

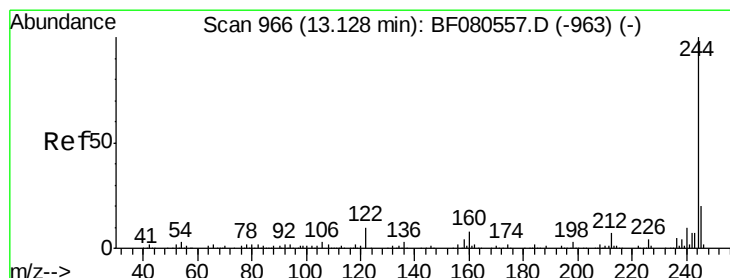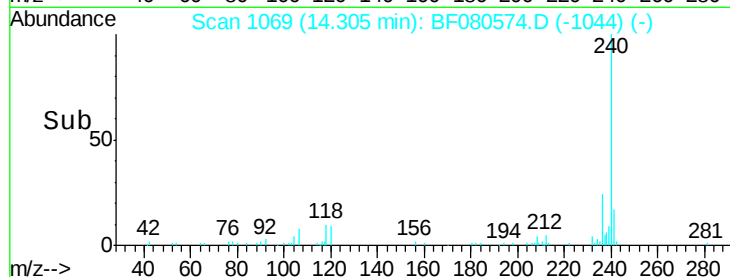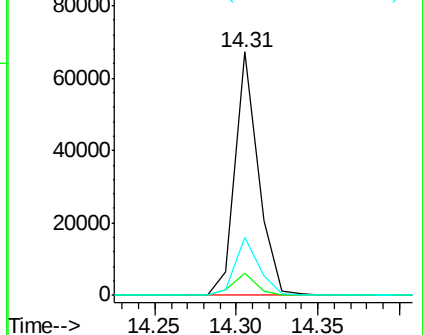

#78

Terphenyl-d14

Concen: 112.88 ng

RT: 13.13 min Scan# 966

Delta R.T. -0.00 min

Lab File: BF080574.D

Acq: 23 Jul 2015 1:06


Tgt Ion:244 Resp: 362340

Ion Ratio Lower Upper

244 100

212 7.7 6.0 9.0



122 8.6 8.2 12.2

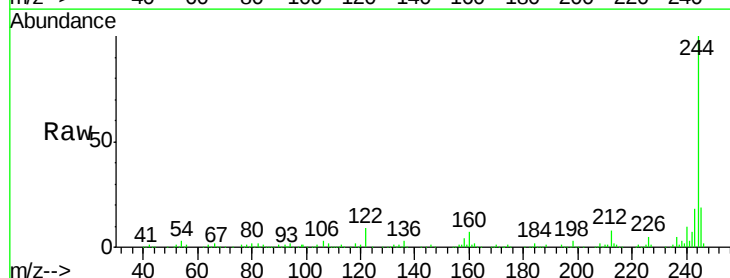


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

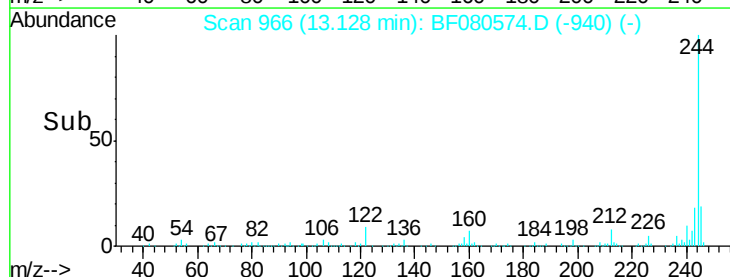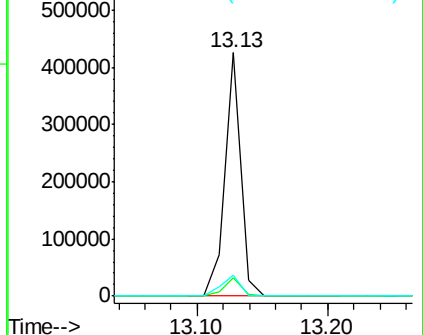

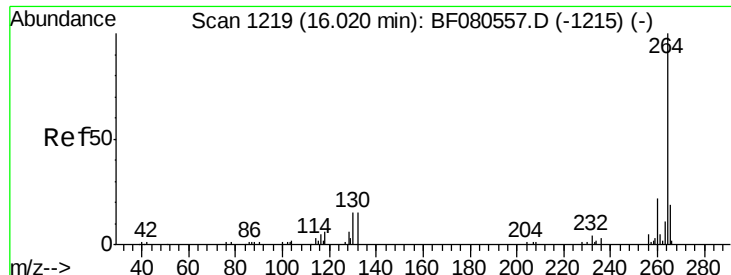

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.99 min Scan# 1216
Delta R.T. -0.03 min
Lab File: BF080574.D
Acq: 23 Jul 2015 1:06

Instrument :
BNA_F
ClientSampleId :
SB-03-12.5-13.0

Tgt Ion: 264 Resp: 40026
Ion Ratio Lower Upper
264 100
260 25.7 17.8 26.8
265 24.2 15.6 23.4#

