


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072215\
 Data File : BF080556.D
 Acq On : 22 Jul 2015 11:45
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 23 05:13:42 2015

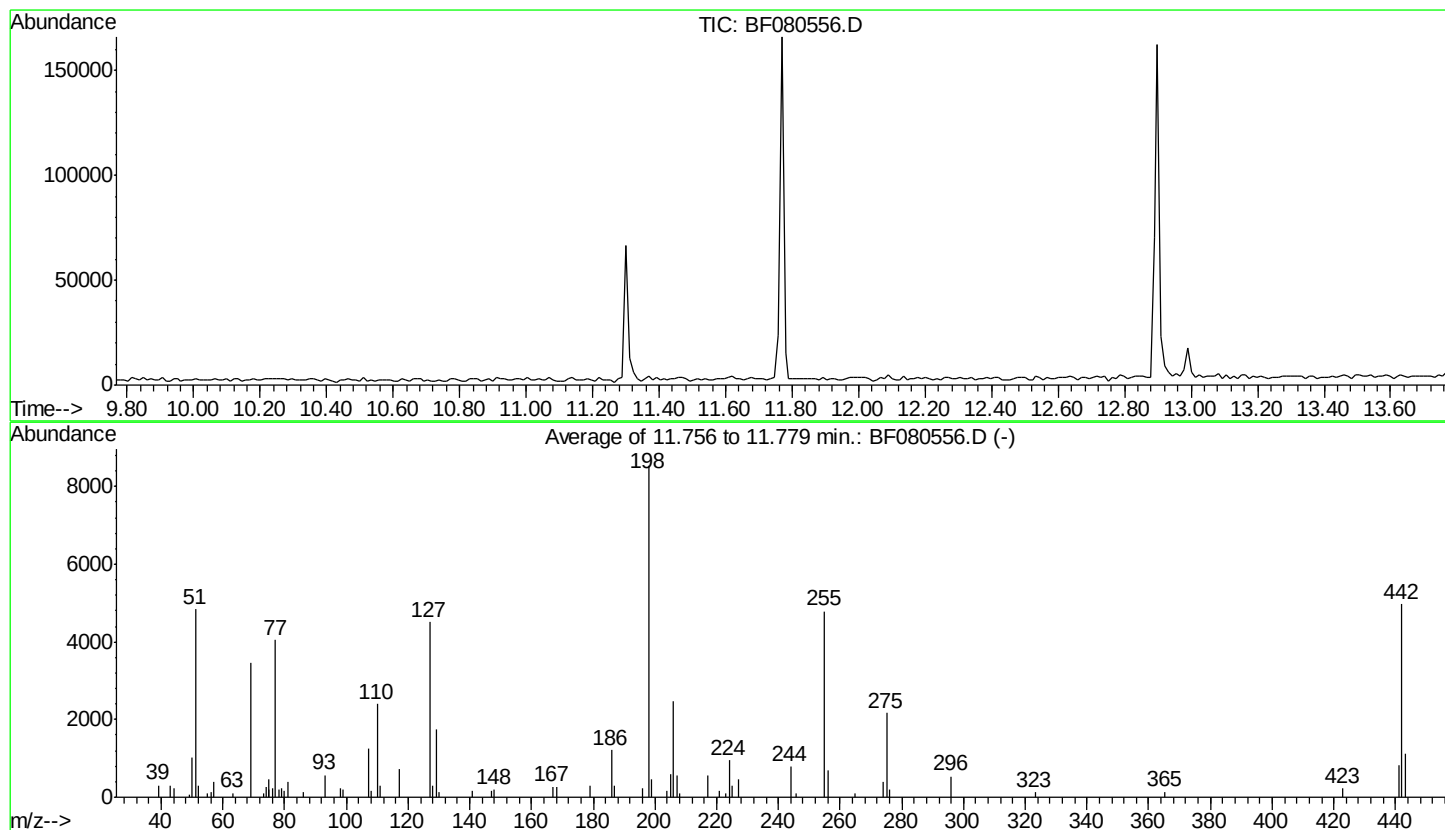

AutoFind: Scans 846, 847, 848; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	4845	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.4	3450	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	4505	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8539	PASS
199	198	5	9	5.5	466	PASS
275	198	10	60	25.4	2170	PASS
365	198	1	100	1.6	136	PASS
441	442	0.01	24	16.4	813	PASS
442	198	50	100	58.2	4969	PASS
443	442	15	24	22.5	1117	PASS