


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072215\
Data File : BF080565.D
Acq On : 22 Jul 2015 20:14
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 23 05:13:42 2015

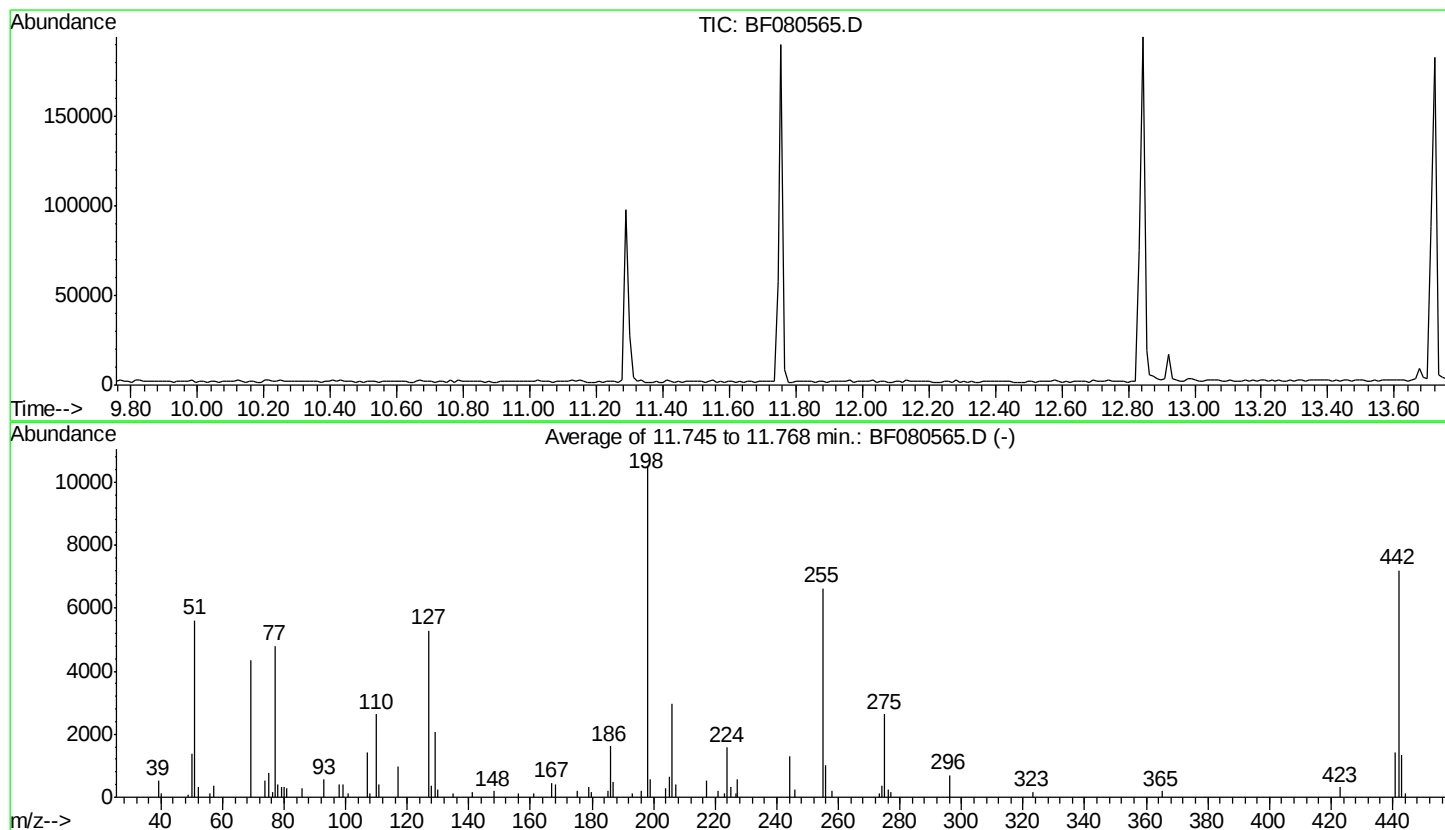

AutoFind: Scans 845, 846, 847; Background Corrected with Scan 842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	5626	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.2	4340	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	5282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10522	PASS
199	198	5	9	5.2	551	PASS
275	198	10	60	25.1	2637	PASS
365	198	1	100	1.8	187	PASS
441	442	0.01	24	19.6	1409	PASS
442	198	50	100	68.5	7205	PASS
443	442	15	24	18.5	1334	PASS