


Data Path : Z:\HPCHEM1\BNA_F\Data\BF072216\
 Data File : BF089197.D
 Acq On : 22 Jul 2016 15:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 19:03:15 2016

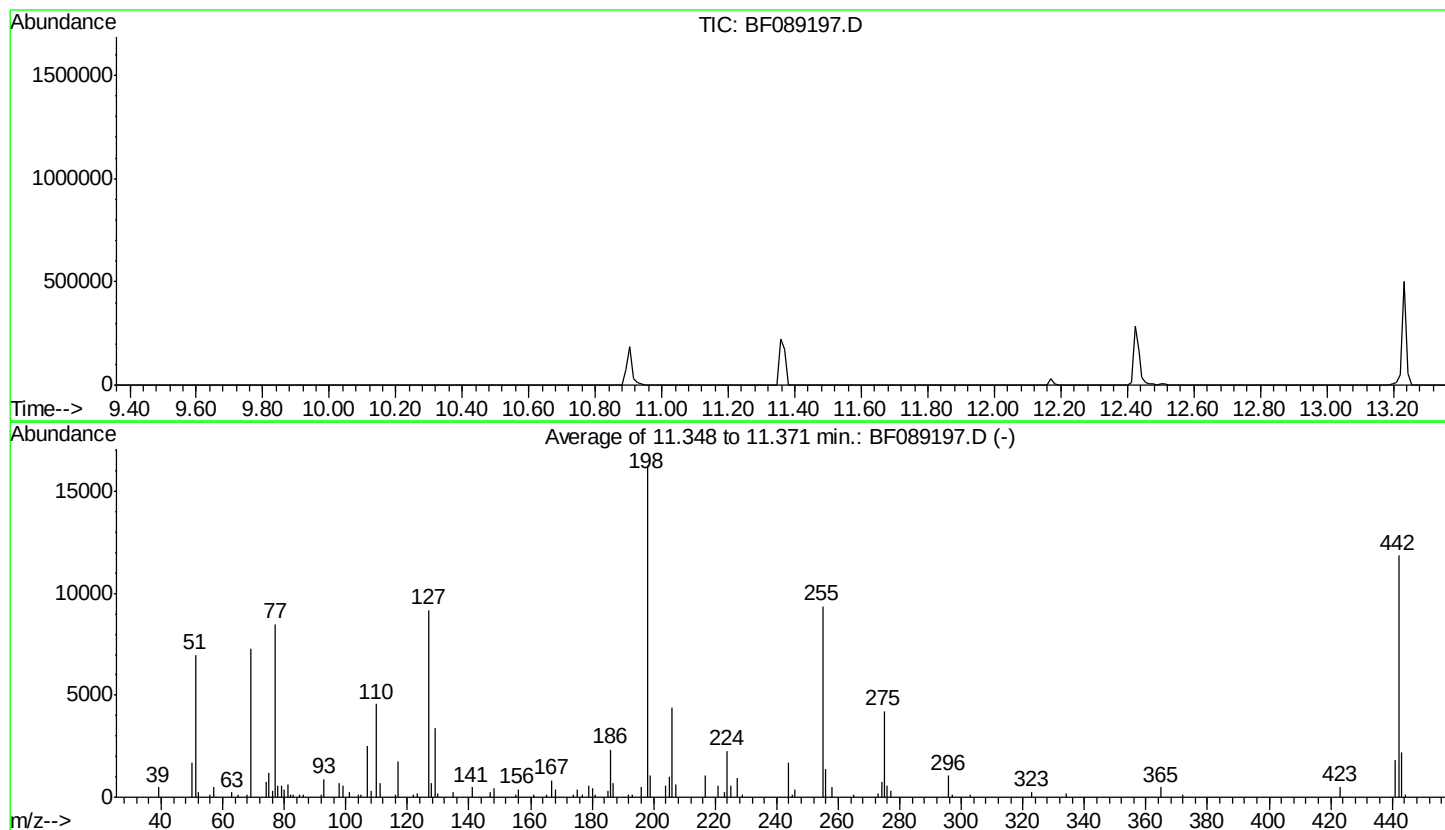

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	6994	PASS
68	69	0.00	2	1.6	119	PASS
69	198	0.00	100	44.9	7302	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.5	9182	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16265	PASS
199	198	5	9	6.6	1075	PASS
275	198	10	60	26.0	4230	PASS
365	198	1	100	3.0	490	PASS
441	442	0.01	24	15.4	1823	PASS
442	198	50	100	72.8	11841	PASS
443	442	15	24	18.6	2205	PASS