
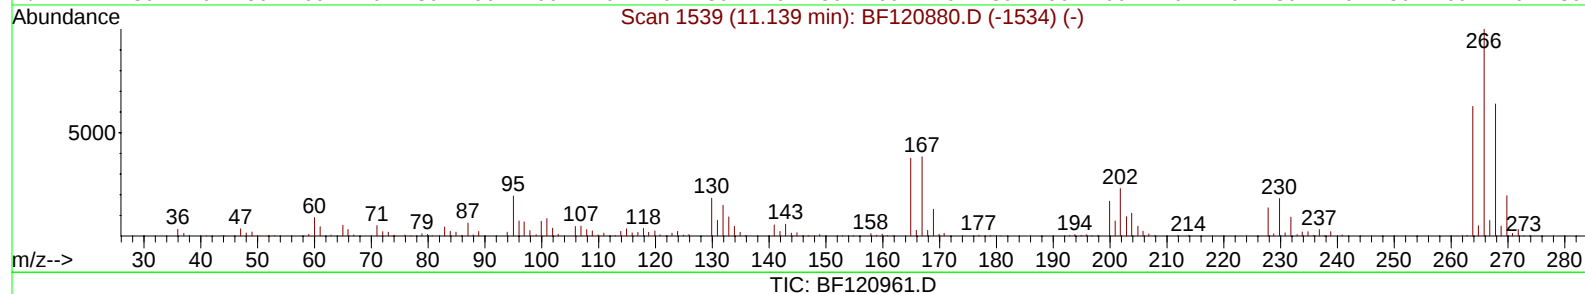
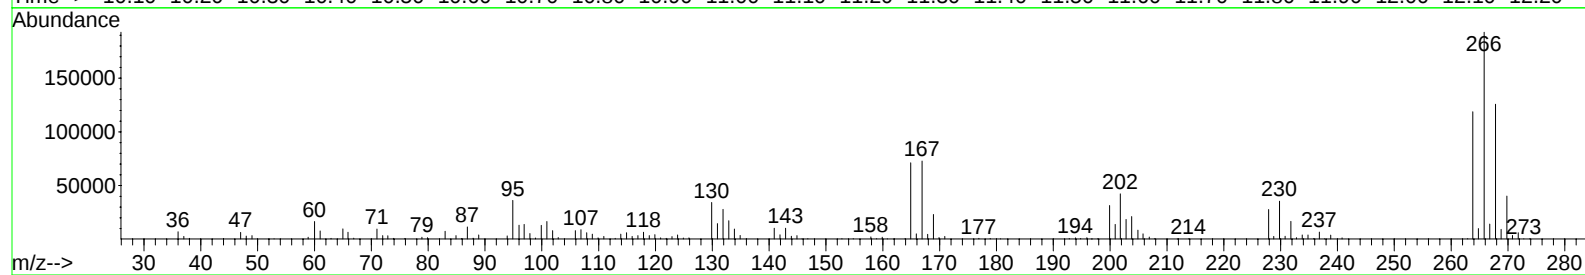


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072220\
Data File : BF120961.D
Acq On : 22 Jul 2020 10:52
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 18:24:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

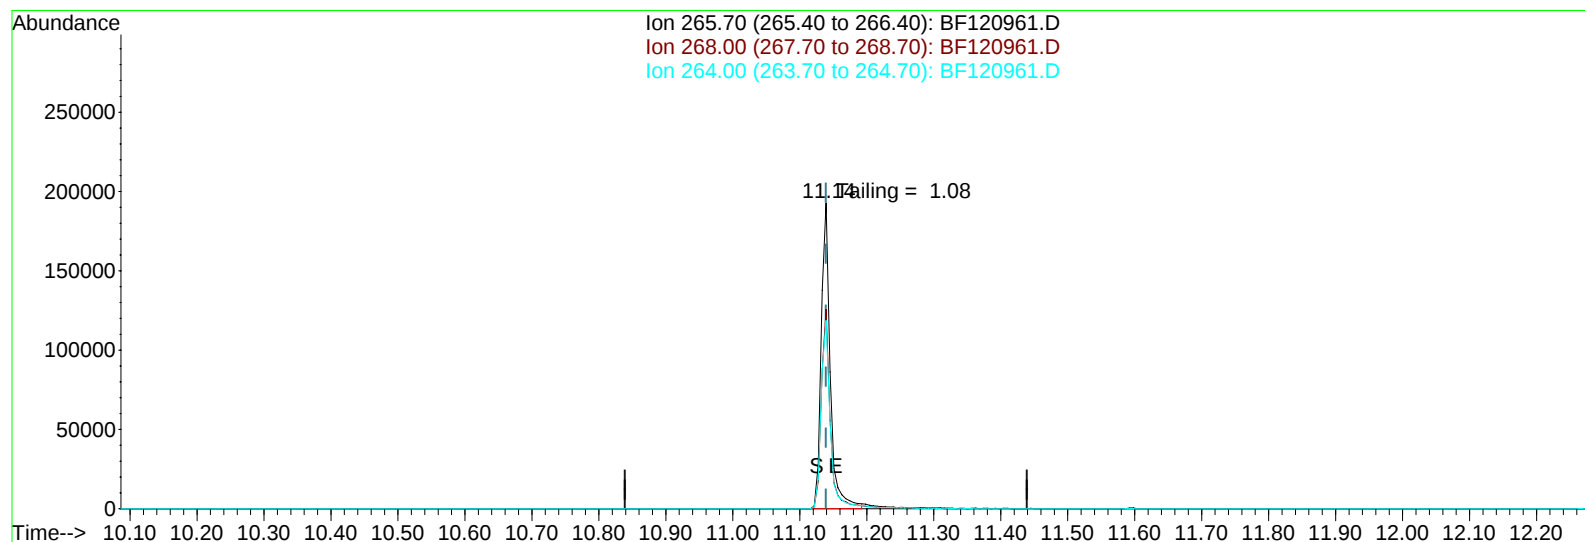

(70) Pentachlorophenol (C)




11.139min (+0.000) 197329.22ng

response 188150

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.20
264.00	62.70	61.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072220\
 Data File : BF120961.D
 Acq On : 22 Jul 2020 10:52
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 18:24:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

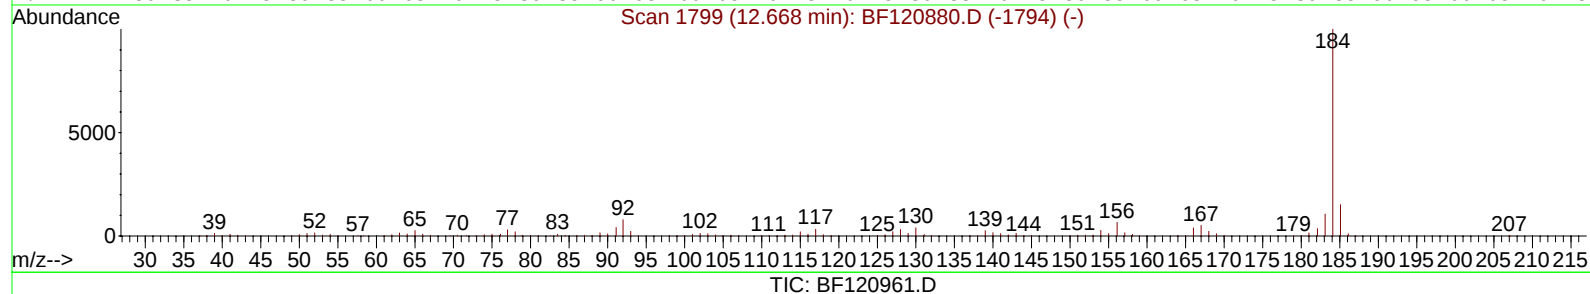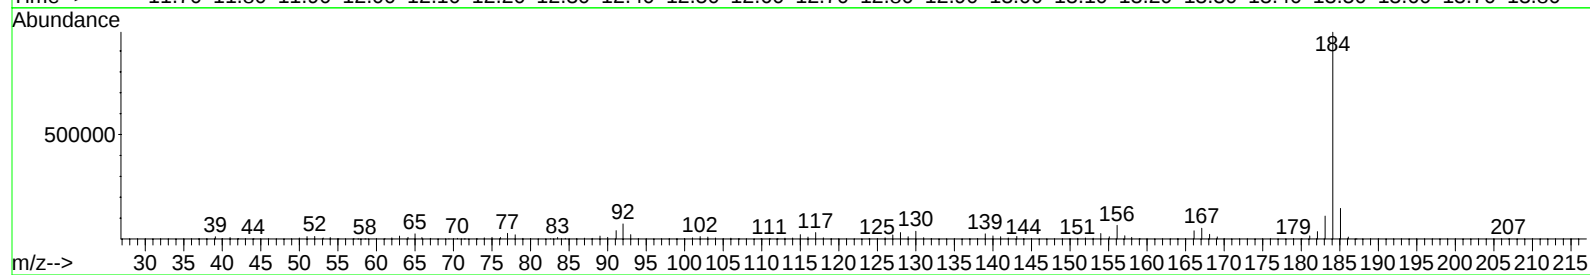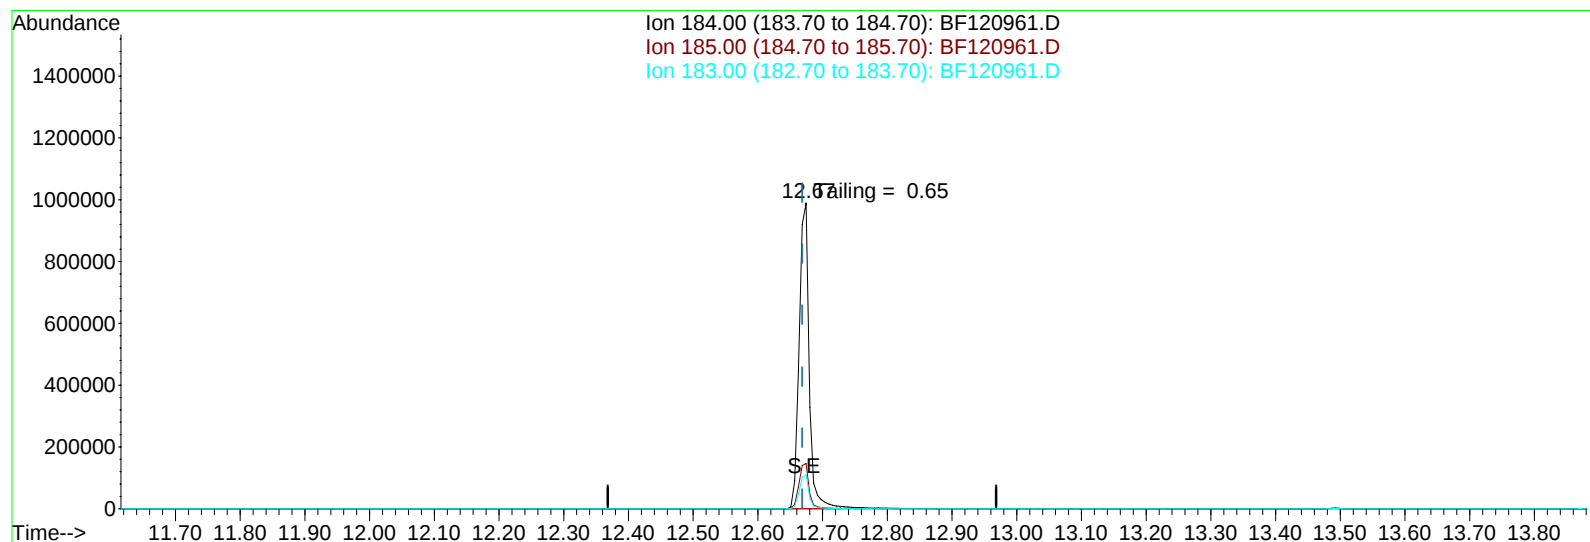

(77) Benzidine

12.674min (+0.006) 162201.27ng

response 1078934

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.80
183.00	10.60	11.09
0.00	0.00	0.00