

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072220\
 Data File : BF120974.D
 Acq On : 22 Jul 2020 20:11
 Operator : JU/CG
 Sample : L3368-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20200421-SITE-WATER

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	563	567	580	rBV	2221402	2141938	43.32%	7.797%
2	6.440	735	740	743	rBV	1823906	1710496	34.59%	6.227%
3	6.640	771	774	786	rBV	71039	91088	1.84%	0.332%
4	6.810	800	803	807	rBV	1273843	1003521	20.29%	3.653%
5	7.375	894	899	902	rBV	2494487	2623427	53.05%	9.550%
6	8.092	1017	1021	1025	rBV	1398601	1285265	25.99%	4.679%
7	9.169	1200	1204	1208	rBV	4017134	4330254	87.57%	15.764%
8	9.286	1220	1224	1237	rVB	149528	174839	3.54%	0.636%
9	9.563	1268	1271	1284	rVB	237166	223651	4.52%	0.814%
10	9.845	1315	1319	1331	rBV	1532733	1527880	30.90%	5.562%
11	10.633	1449	1453	1470	rBV	2484409	2858466	57.81%	10.406%
12	11.333	1568	1572	1579	rBV	1767896	1641765	33.20%	5.977%
13	12.921	1837	1842	1845	rBV2	4354556	4944774	100.00%	18.001%
14	13.968	2015	2020	2036	rBV	1493422	1553603	31.42%	5.656%
15	15.415	2260	2266	2282	rBV	881307	1358713	27.48%	4.946%


Sum of corrected areas: 27469680

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072220\
Data File : BF120974.D
Acq On : 22 Jul 2020 20:11
Operator : JU/CG
Sample : L3368-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20200421-SITE-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

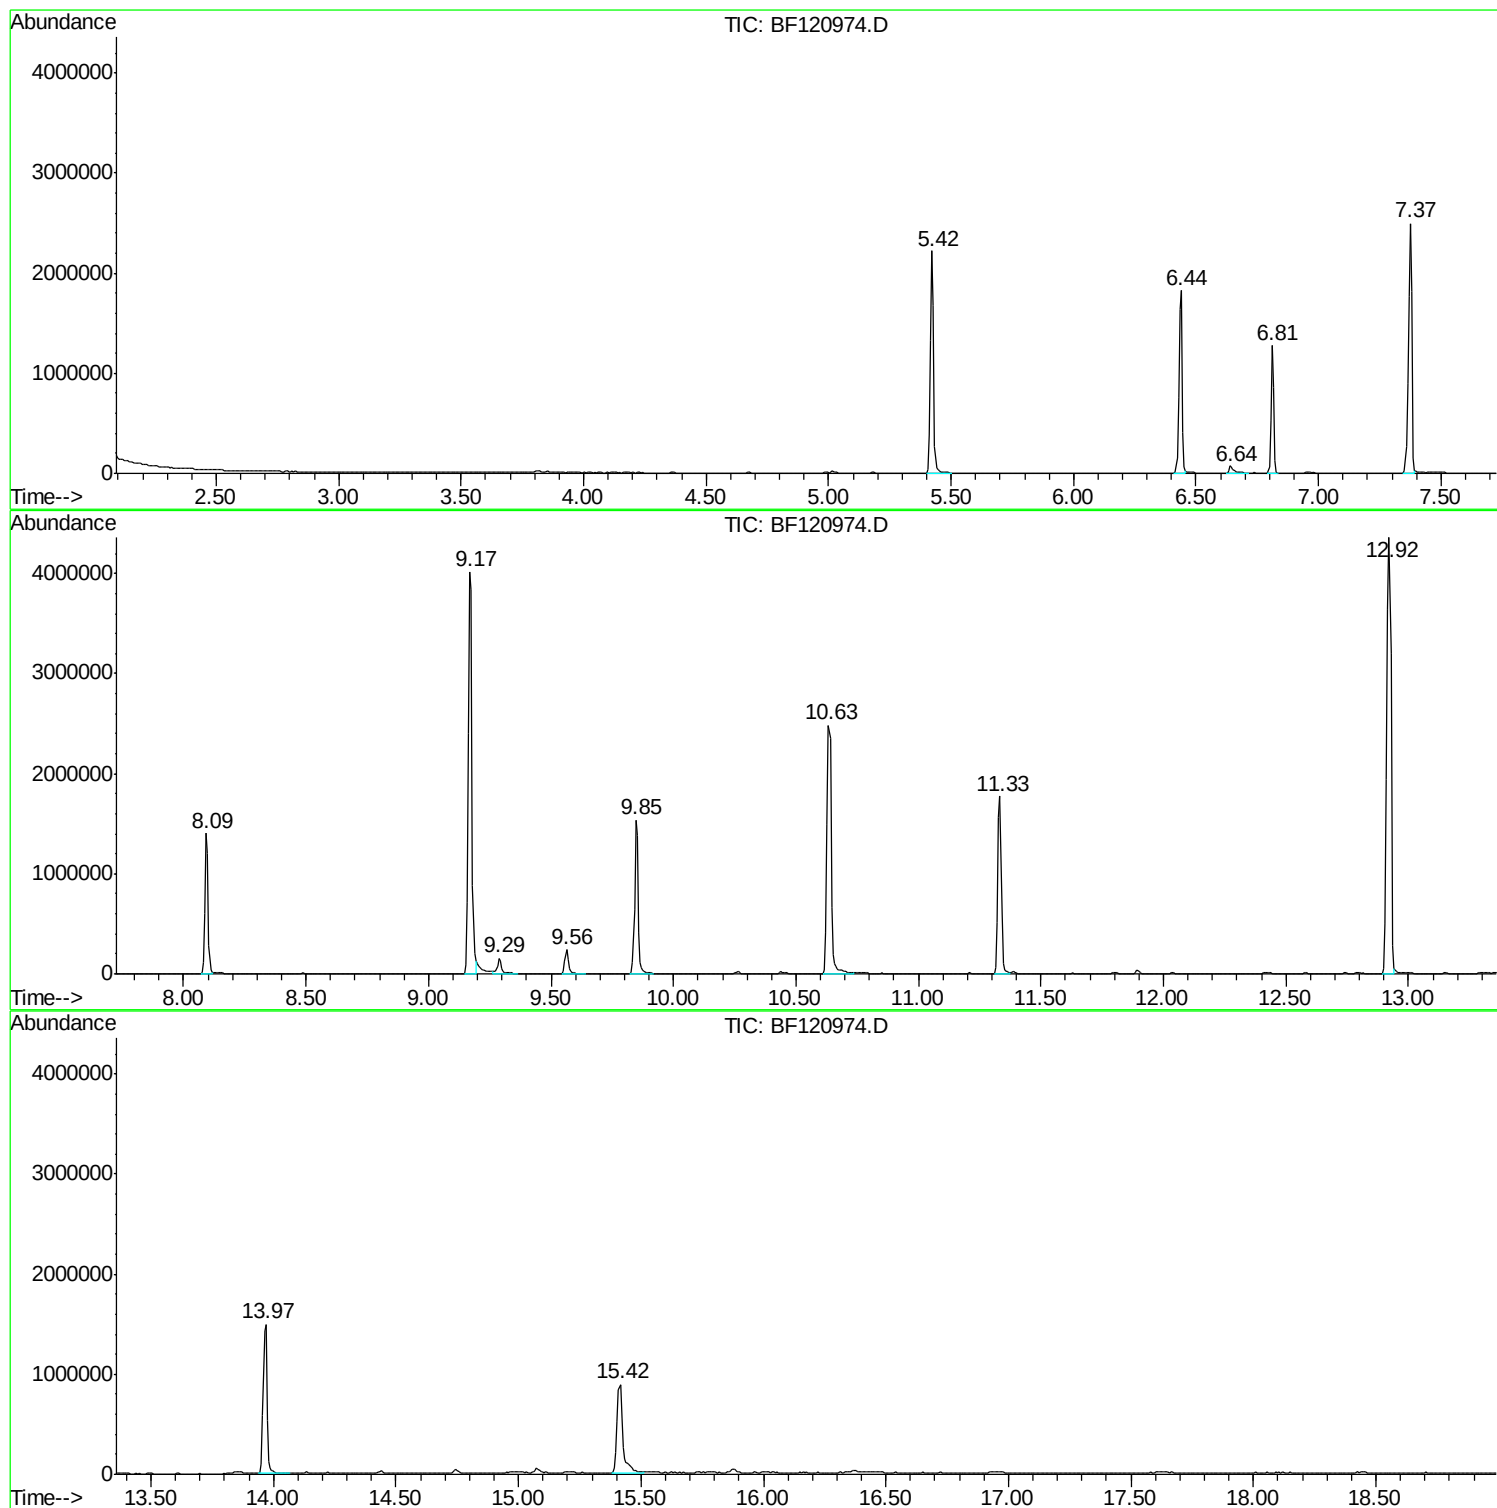

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072220\
Data File : BF120974.D
Acq On : 22 Jul 2020 20:11
Operator : JU/CG
Sample : L3368-02
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
20200421-SITE-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
9.29	2.29 ng	174839	Acenaphthene-d10	9.85	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	87
2	Metacetamol	151	C8H9NO2	000621-42-1	52
3	Acetaminophen	151	C8H9NO2	000103-90-2	40
4	Cyclohexanol, 3,3,5-trimethyl-	142	C9H18O	000116-02-9	38
5	Pyridine, 2-butyl-, 1-oxide	151	C9H13NO	031396-32-4	36

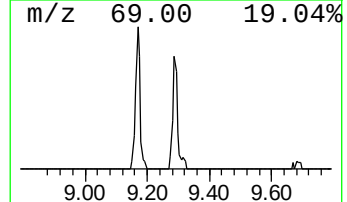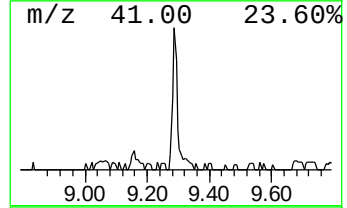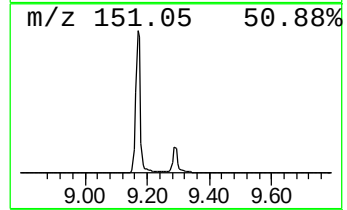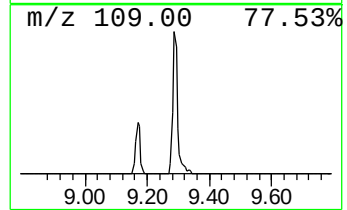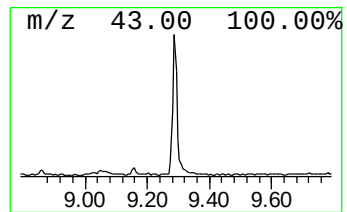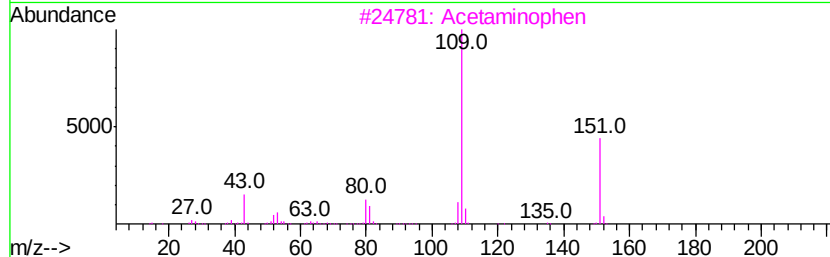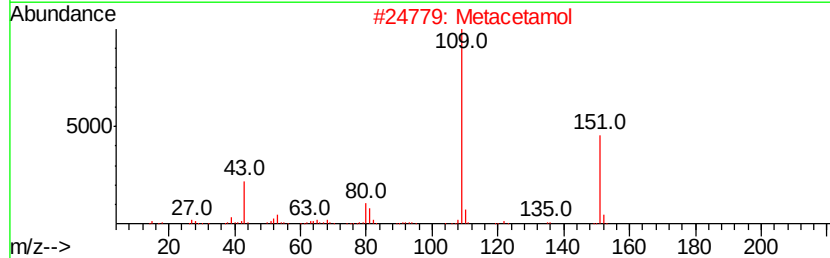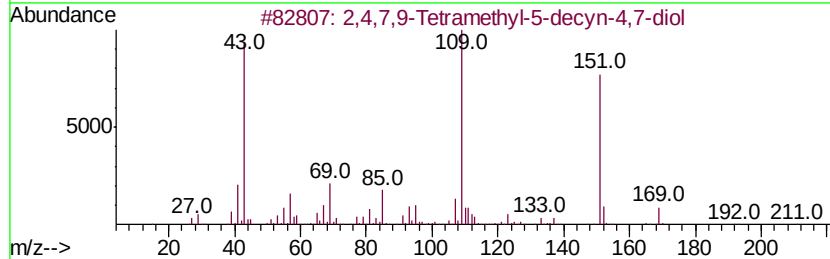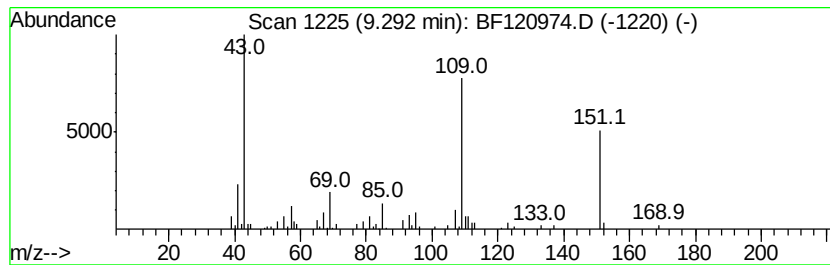

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072220\
Data File : BF120974.D
Acq On : 22 Jul 2020 20:11
Operator : JU/CG
Sample : L3368-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20200421-SITE-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2,4,7,9-Tetrameth...	9.29	2.3	ng	174839	3	9.85	1527880	20.0