

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
 Data File : BF124691.D
 Acq On : 22 Jul 2021 15:56
 Operator : JU/CG
 Sample : PB137815BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137815BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	512	515	519	rBB	2526	3297	1.18%	0.211%
2	5.492	574	579	582	rBB	196507	191351	68.75%	12.255%
3	6.492	743	749	752	rBB	173755	195505	70.24%	12.521%
4	6.869	810	813	816	rBB	55647	40123	14.42%	2.570%
5	7.433	904	909	911	rBB	137588	126767	45.55%	8.119%
6	8.151	1027	1031	1034	rBB	72831	57550	20.68%	3.686%
7	9.227	1209	1214	1217	rBB	273964	257149	92.39%	16.469%
8	9.904	1326	1329	1332	rBB	73610	67365	24.20%	4.314%
9	10.698	1459	1464	1467	rBB	176123	149259	53.63%	9.560%
10	11.392	1579	1582	1586	rVB	81975	68426	24.59%	4.382%
11	12.986	1848	1853	1856	rBB	317998	278324	100.00%	17.826%
12	13.868	1999	2003	2005	rBV	3175	3566	1.28%	0.228%
13	13.898	2005	2008	2011	rVB	11924	10057	3.61%	0.644%
14	14.033	2027	2031	2034	rBB	73322	60313	21.67%	3.863%
15	15.504	2276	2281	2285	rBV2	46061	52316	18.80%	3.351%




Sum of corrected areas: 1561368

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
Data File : BF124691.D
Acq On : 22 Jul 2021 15:56
Operator : JU/CG
Sample : PB137815BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137815BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

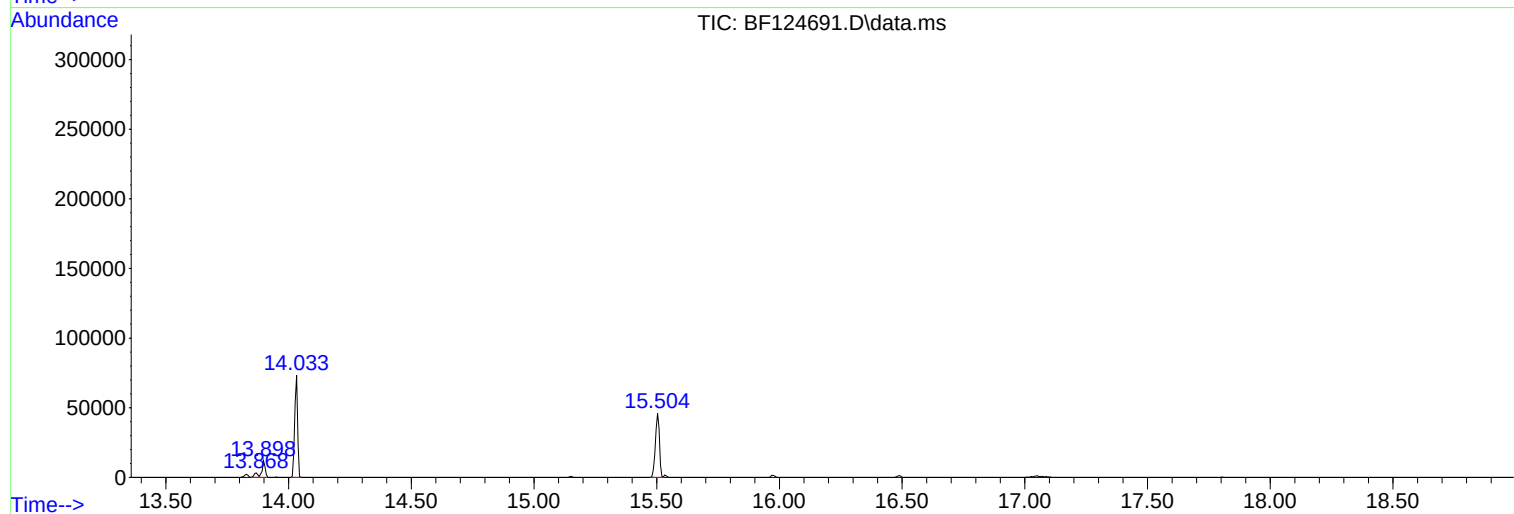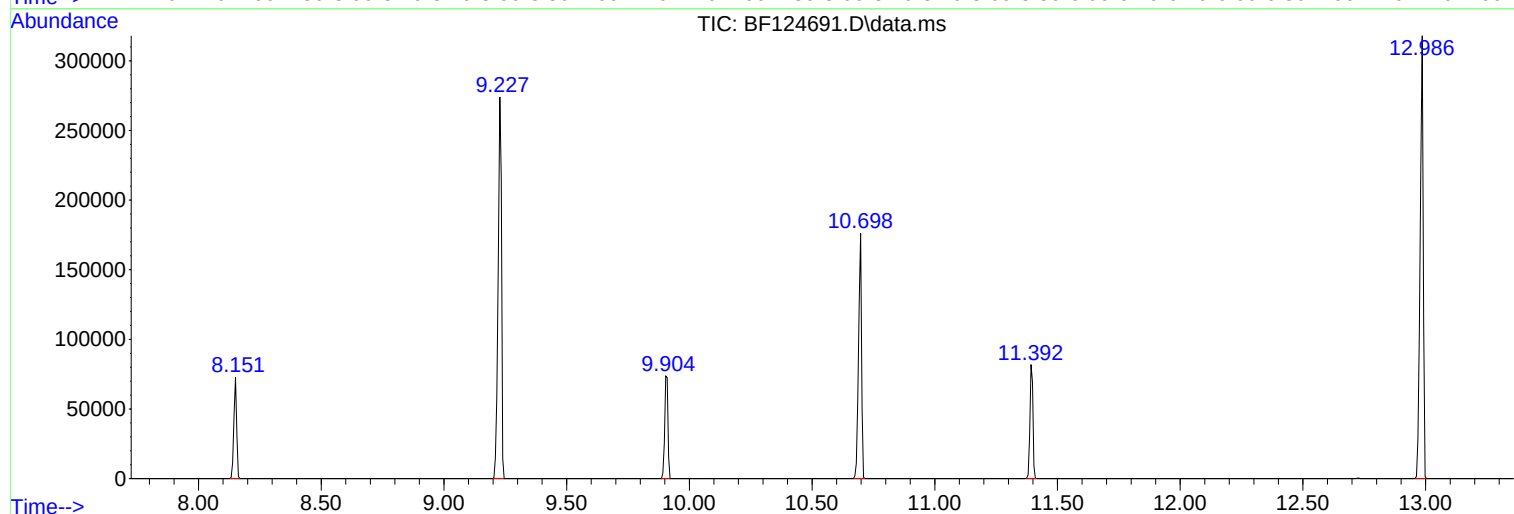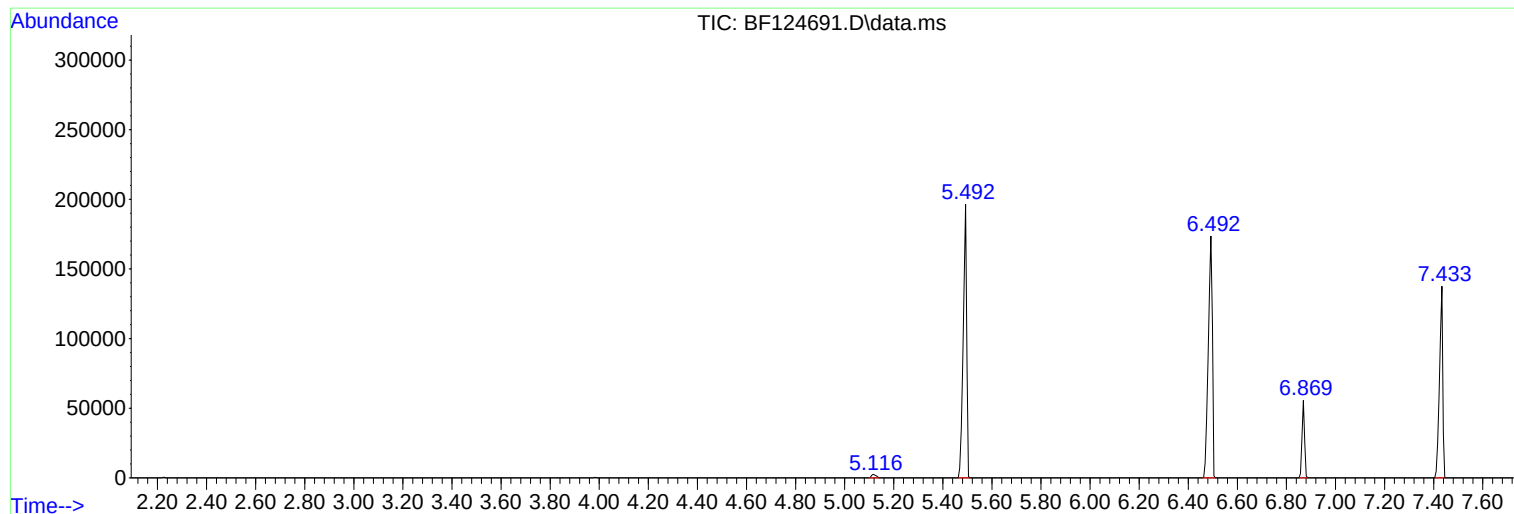

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
Data File : BF124691.D
Acq On : 22 Jul 2021 15:56
Operator : JU/CG
Sample : PB137815BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137815BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,2'-(Ethane-1,...	13.898	3.3	ng	10057	5	14.033	60313	20.0