


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
 Data File : BF124682.D
 Acq On : 22 Jul 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

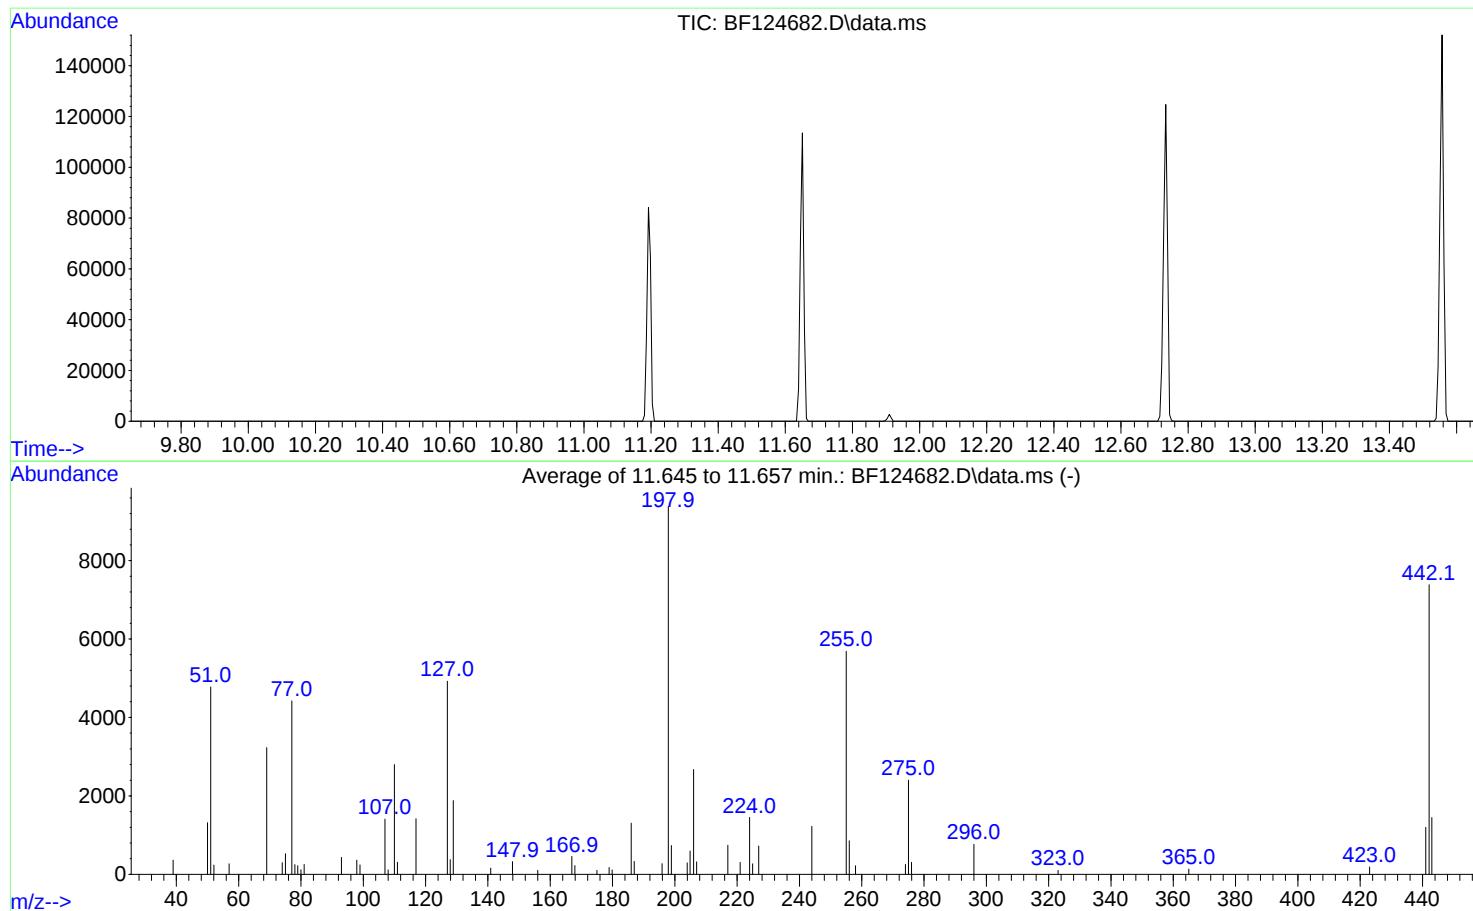




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	4778	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.4	3229	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	4923	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9378	PASS
199	198	5	9	7.8	736	PASS
275	198	10	60	25.6	2403	PASS
365	198	1	100	1.4	133	PASS
441	198	0.01	100	12.8	1201	PASS
442	442	50	100	100.0	7384	PASS
443	442	15	24	19.6	1450	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
 Data File : BF124682.D
 Acq On : 22 Jul 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 11:21:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:14:11 2021
 Response via : Initial Calibration

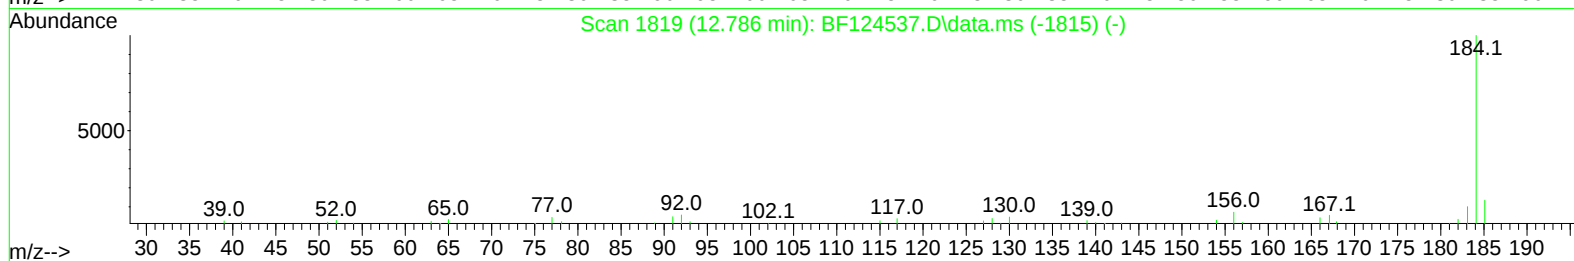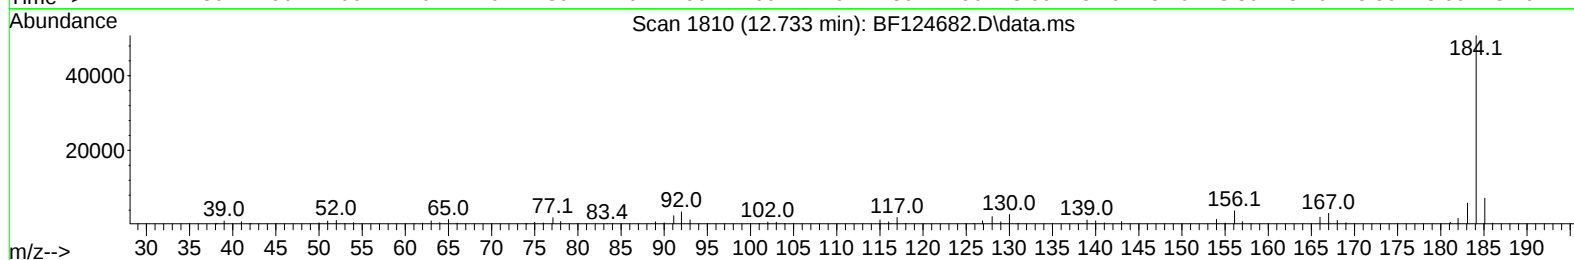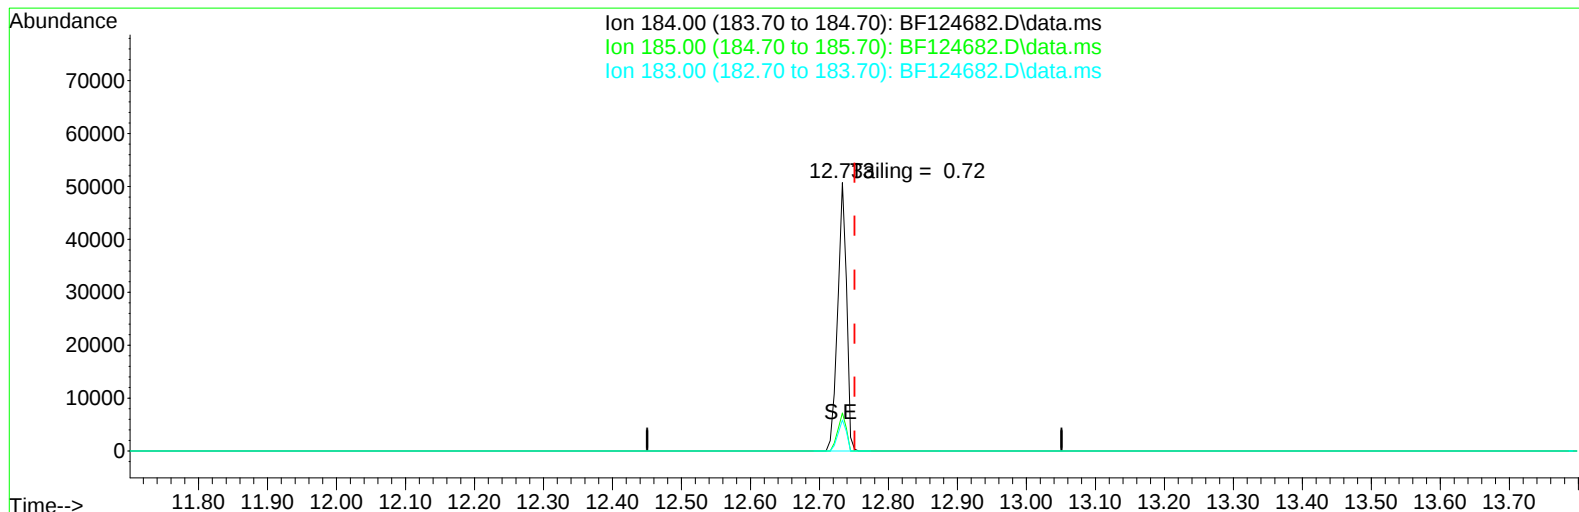

TIC: BF124682.D\data.ms

(77) Benzidine

12.733min (-0.018) 0.00 ng




response 45407

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.23
183.00	10.10	11.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072221\
 Data File : BF124682.D
 Acq On : 22 Jul 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 11:21:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:14:11 2021
 Response via : Initial Calibration

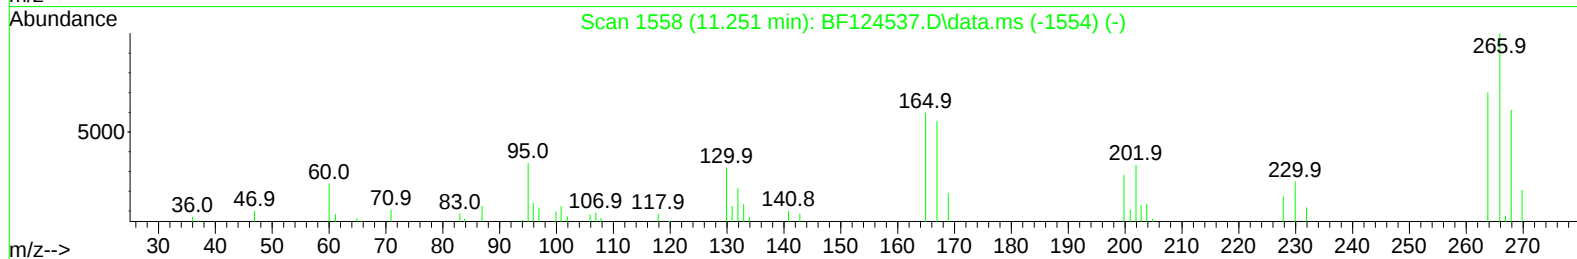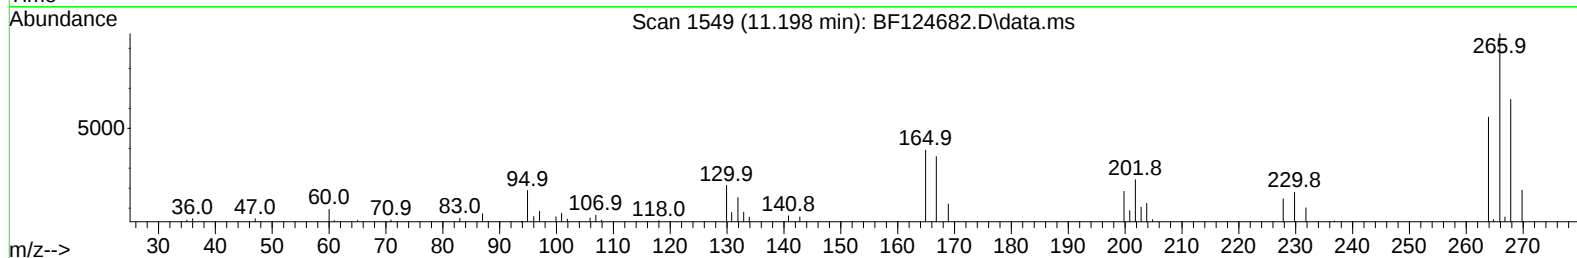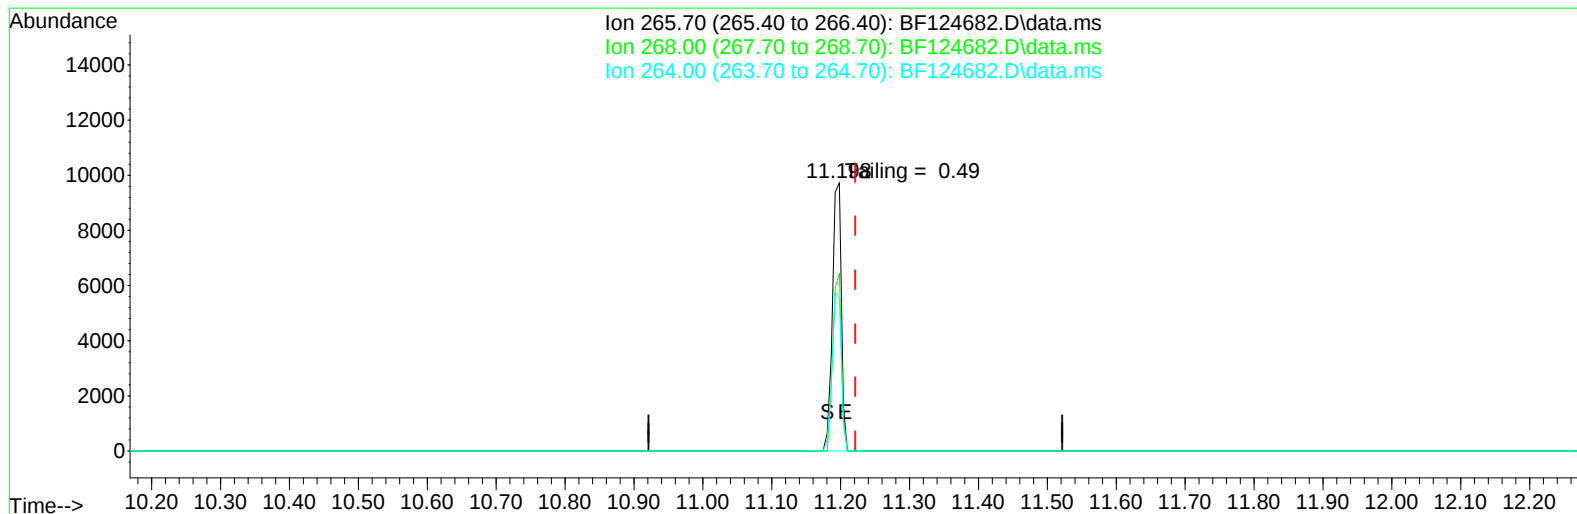

TIC: BF124682.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.023) 0.00 ng

response 8755

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	66.19
264.00	69.90	57.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2021	BNA_F	<u>BF124682.D</u>
Compound Name	Response	Retention Time
DDT	24612	13.55
DDD	0	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	24612	0.00