
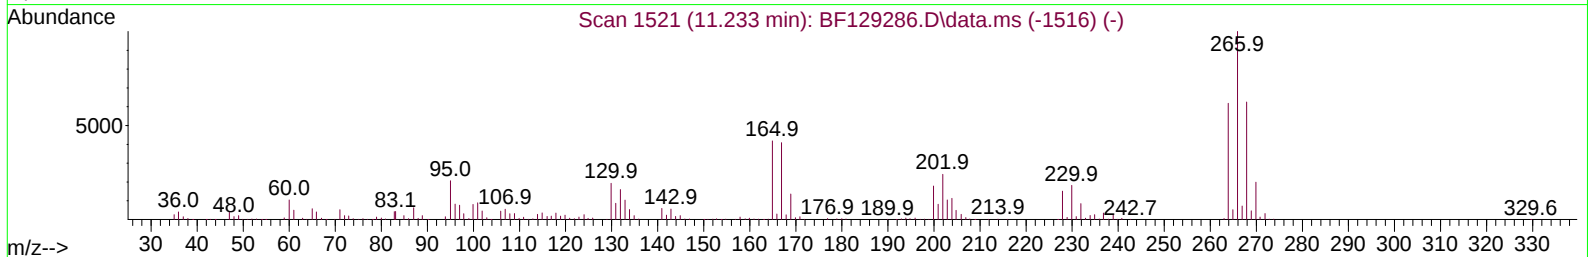
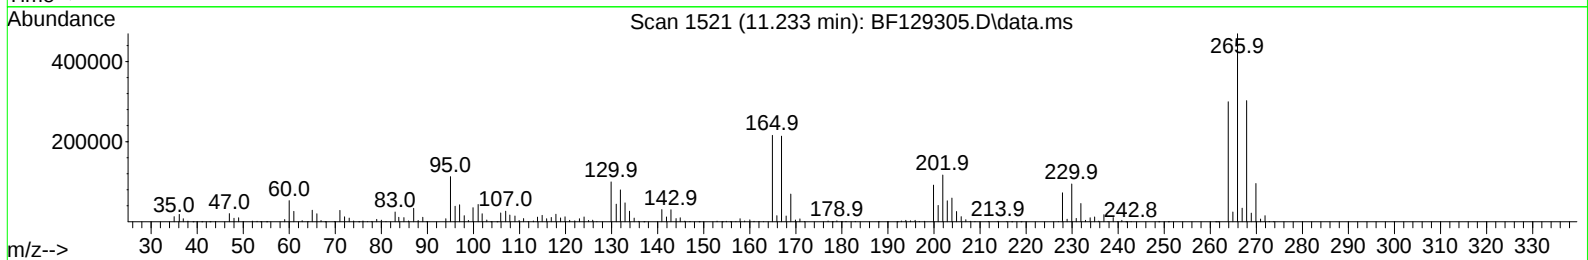


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129305.D
 Acq On : 22 Jul 2022 08:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 16:54:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 13:42:18 2022
 Response via : Initial Calibration

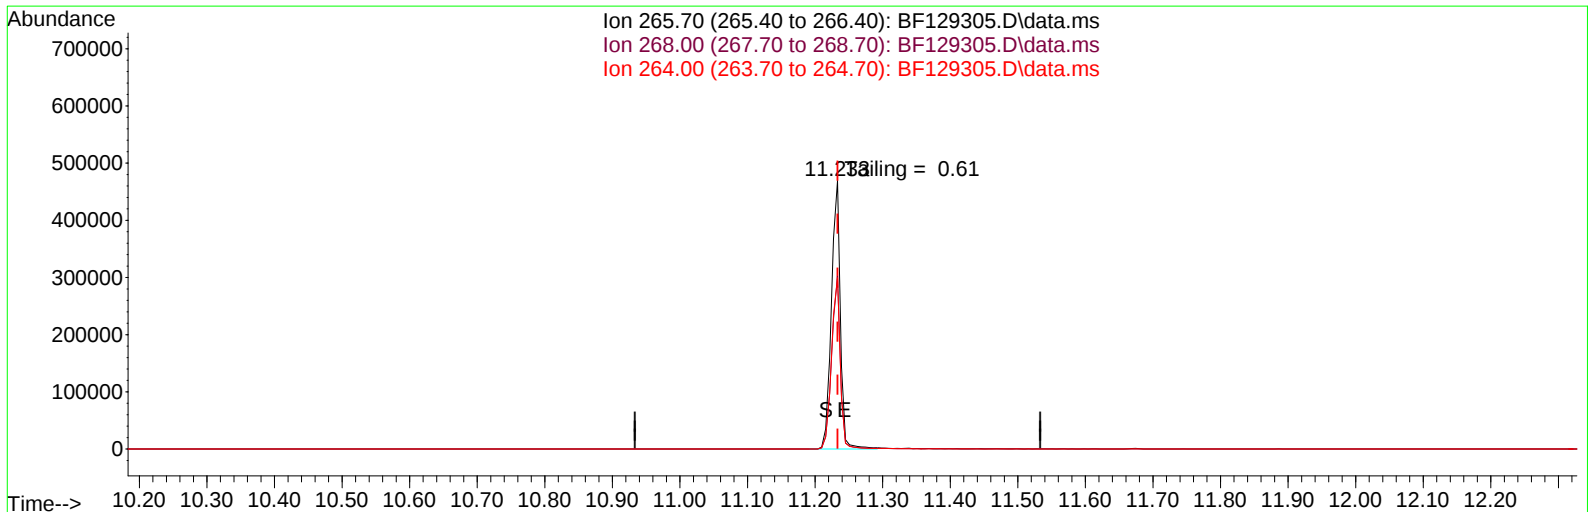

TIC: BF129305.D\data.ms

(70) Pentachlorophenol (C)




11.233min (-0.000) 376986.68 ng

response 435971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.40
264.00	61.80	63.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129305.D
Acq On : 22 Jul 2022 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 16:54:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

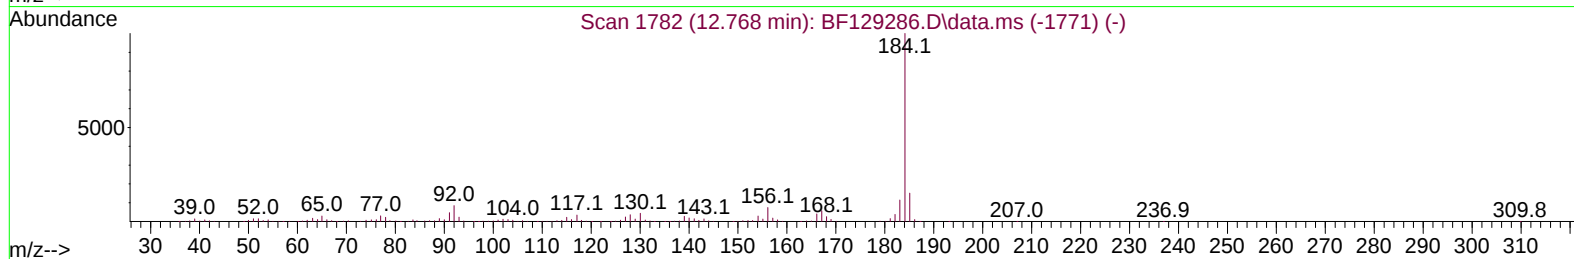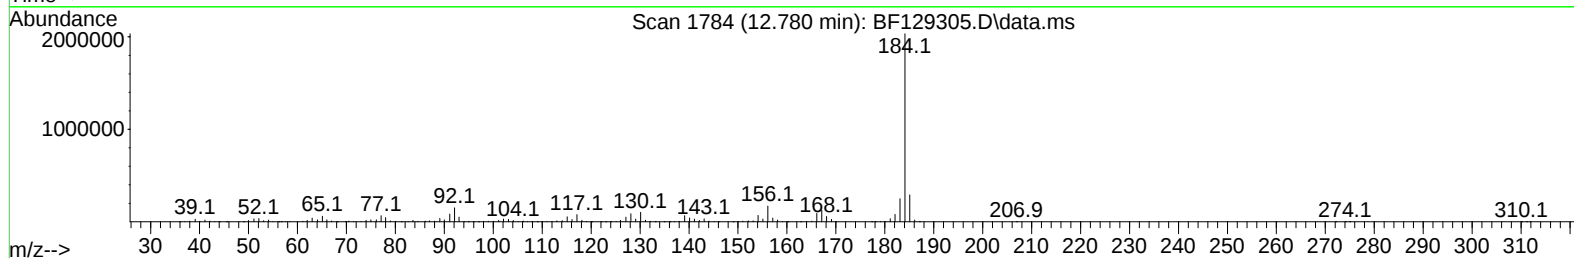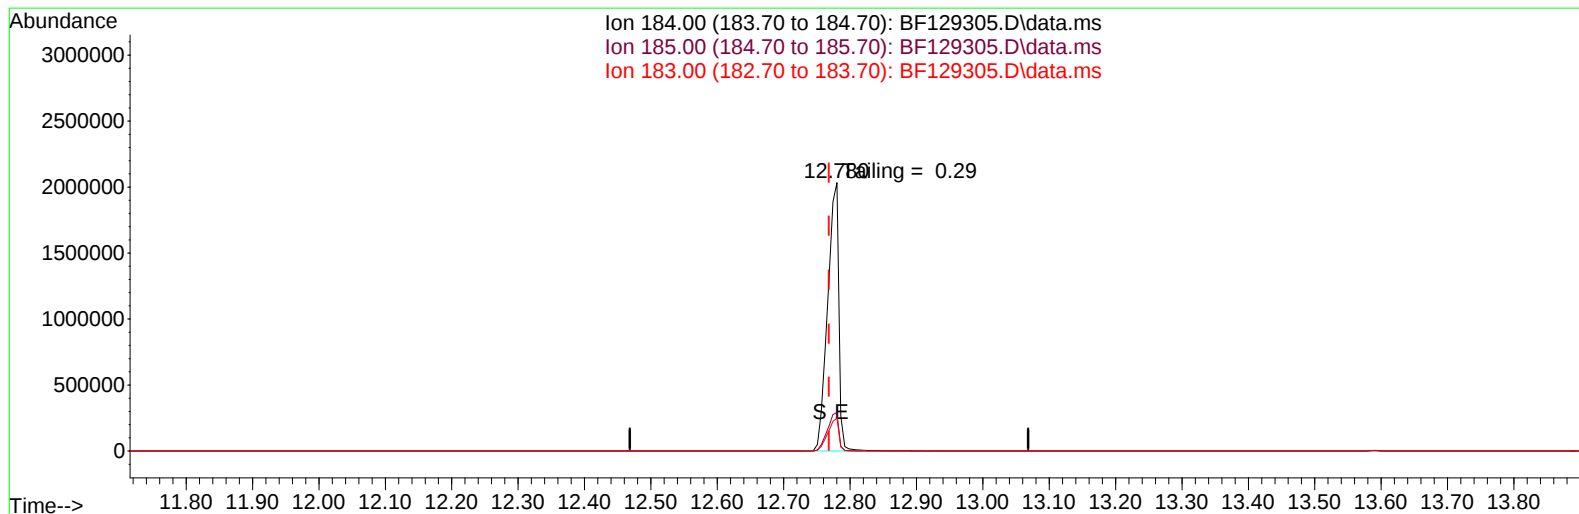

TIC: BF129305.D\data.ms

(77) Benzidine

12.780min (+ 0.012) 76143.97 ng

response 2379024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.31
183.00	11.60	12.24
0.00	0.00	0.00