

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129307.D
 Acq On : 22 Jul 2022 09:45
 Operator : CG\JU
 Sample : PB145953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145953BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	545	551	553	rBV	4236535	4569165	76.10%	13.060%
2	6.522	714	720	723	rBV	4071225	4649164	77.44%	13.289%
3	6.892	779	783	786	rBV	1139378	925656	15.42%	2.646%
4	7.457	873	879	882	rBV	2917205	3060299	50.97%	8.747%
5	8.175	996	1001	1004	rBV	1412978	1246615	20.76%	3.563%
6	9.251	1178	1184	1187	rBV	5770478	5566826	92.72%	15.912%
7	9.933	1294	1300	1303	rBV	1667821	1398934	23.30%	3.999%
8	10.727	1428	1435	1438	rBV	4049645	3833961	63.86%	10.959%
9	11.421	1549	1553	1557	rBV	1771347	1441011	24.00%	4.119%
10	13.015	1818	1824	1827	rBV	6124060	6003886	100.00%	17.161%
11	14.068	1998	2003	2006	rBV	1415730	1247953	20.79%	3.567%
12	15.556	2251	2256	2265	rVB	827976	1041793	17.35%	2.978%




Sum of corrected areas: 34985263

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129307.D
Acq On : 22 Jul 2022 09:45
Operator : CG\JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

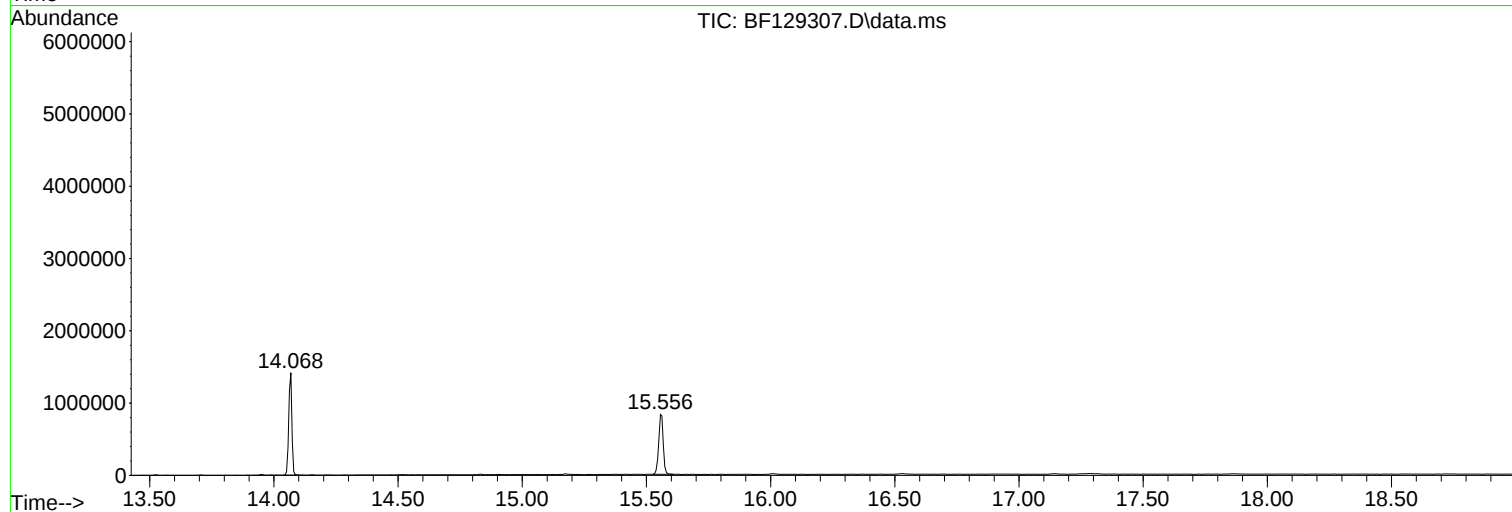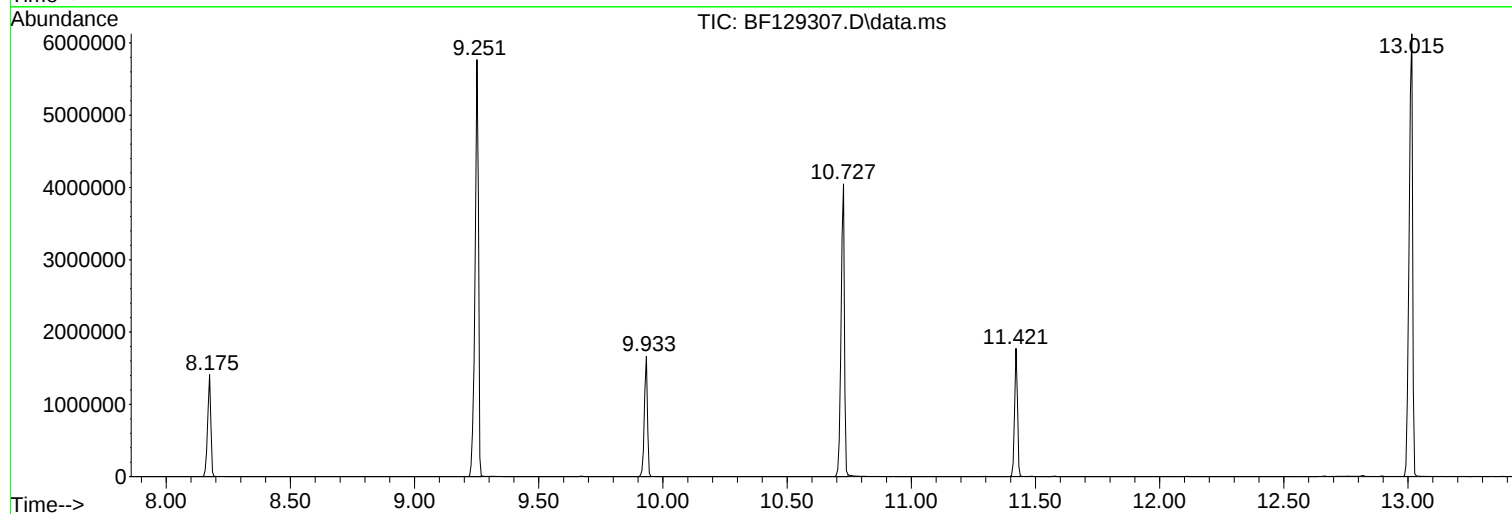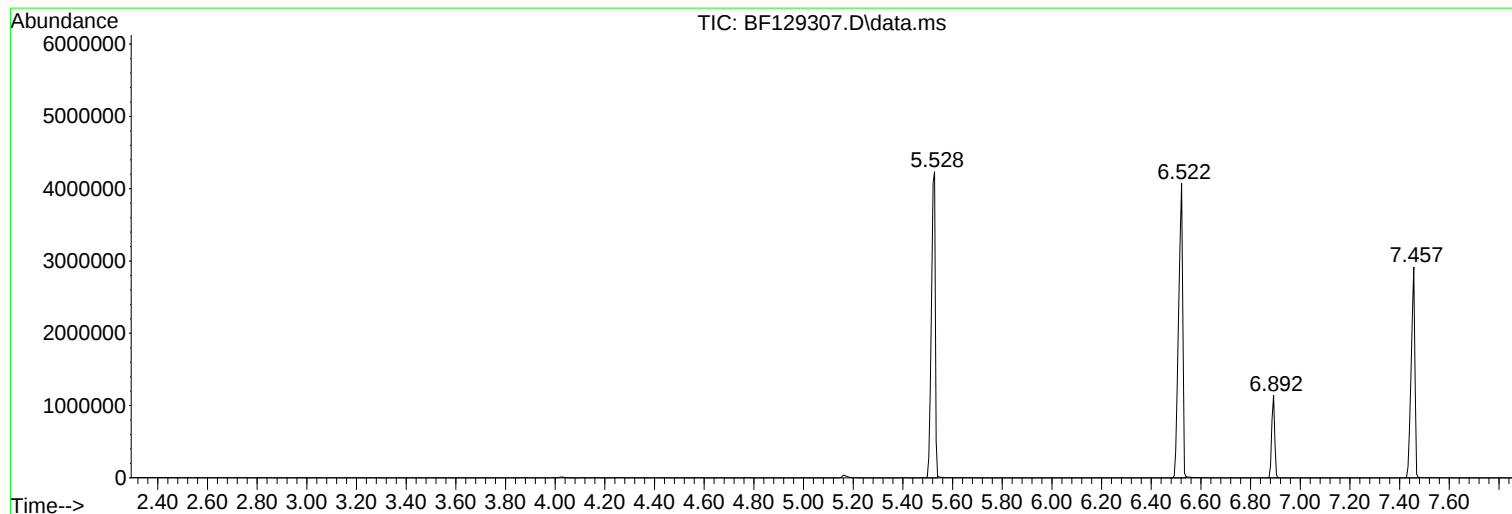

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129307.D
Acq On : 22 Jul 2022 09:45
Operator : CG\JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129307.D
Acq On : 22 Jul 2022 09:45
Operator : CG\JU
Sample : PB145953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------