

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129312.D
 Acq On : 22 Jul 2022 13:08
 Operator : CG\JU
 Sample : PB145957BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145957BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	545	550	553	rBV	3987039	4392965	75.52%	13.098%
2	6.522	714	720	723	rBV	4066759	4413250	75.87%	13.158%
3	6.892	779	783	786	rBV	1099358	880981	15.14%	2.627%
4	7.457	873	879	882	rBV	2883721	2940591	50.55%	8.767%
5	8.175	996	1001	1004	rBV	1360909	1179425	20.27%	3.516%
6	9.251	1178	1184	1187	rBV	5593311	5363535	92.20%	15.991%
7	9.933	1294	1300	1303	rBV	1594606	1360032	23.38%	4.055%
8	10.727	1428	1435	1438	rBV	3794516	3696708	63.55%	11.022%
9	11.421	1549	1553	1556	rBV	1735693	1375175	23.64%	4.100%
10	13.016	1818	1824	1827	rBV	5919716	5817234	100.00%	17.344%
11	14.068	1998	2003	2006	rBV	1223950	1164373	20.02%	3.472%
12	15.557	2250	2256	2265	rBV	771148	956008	16.43%	2.850%




Sum of corrected areas: 33540277

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129312.D
Acq On : 22 Jul 2022 13:08
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

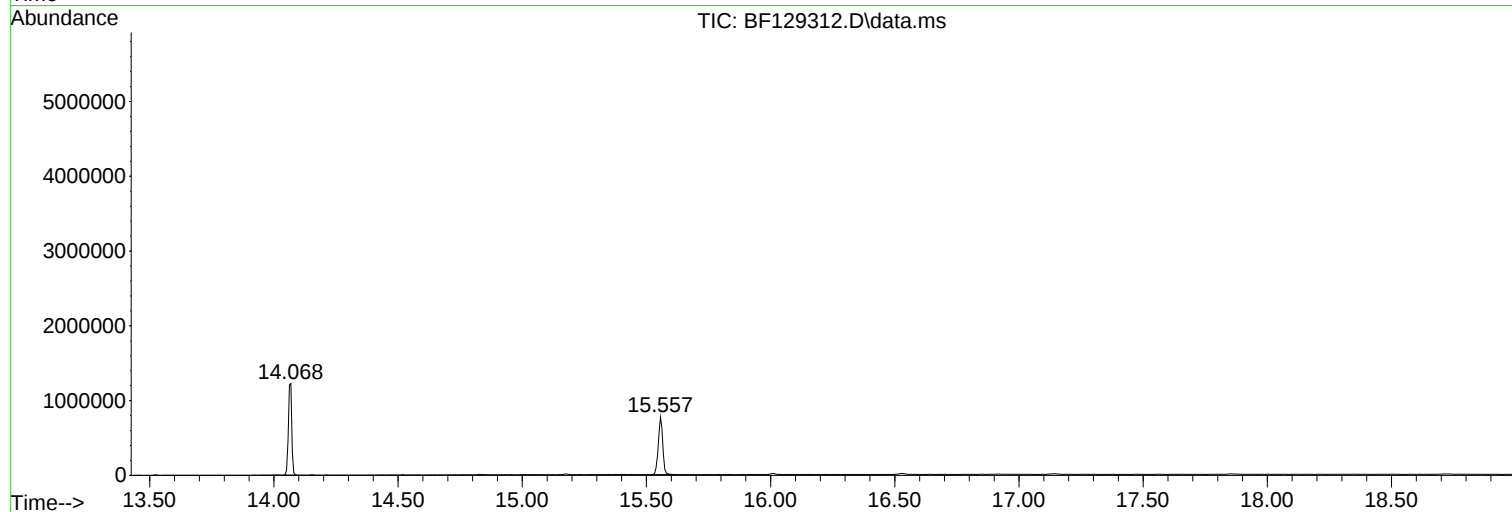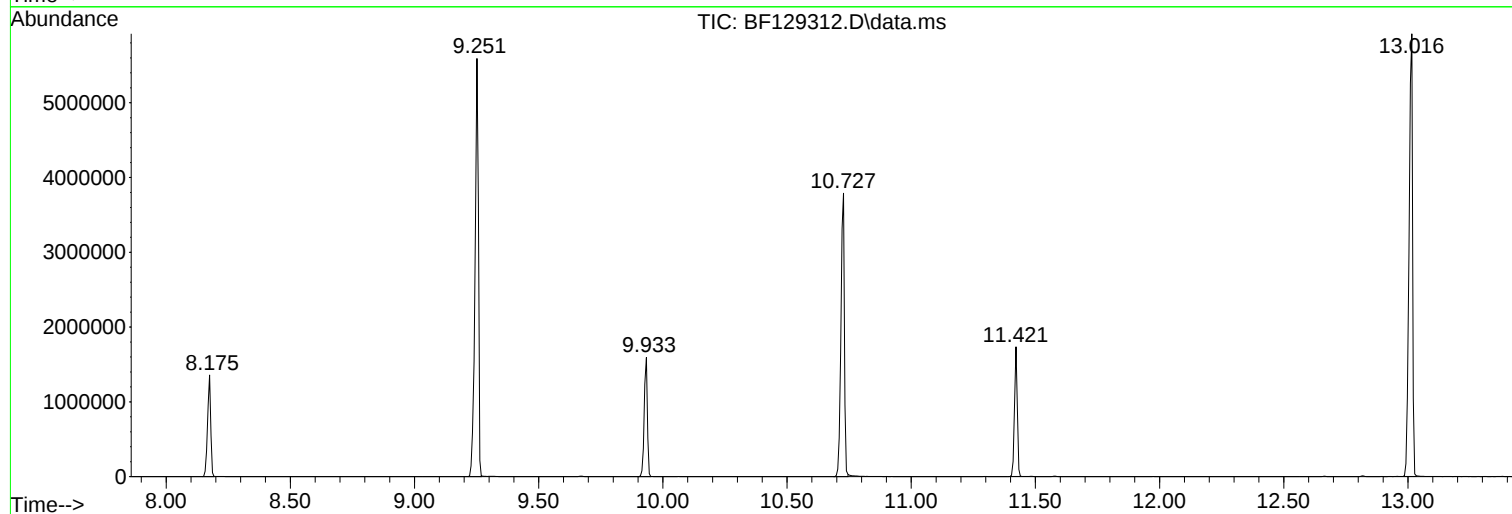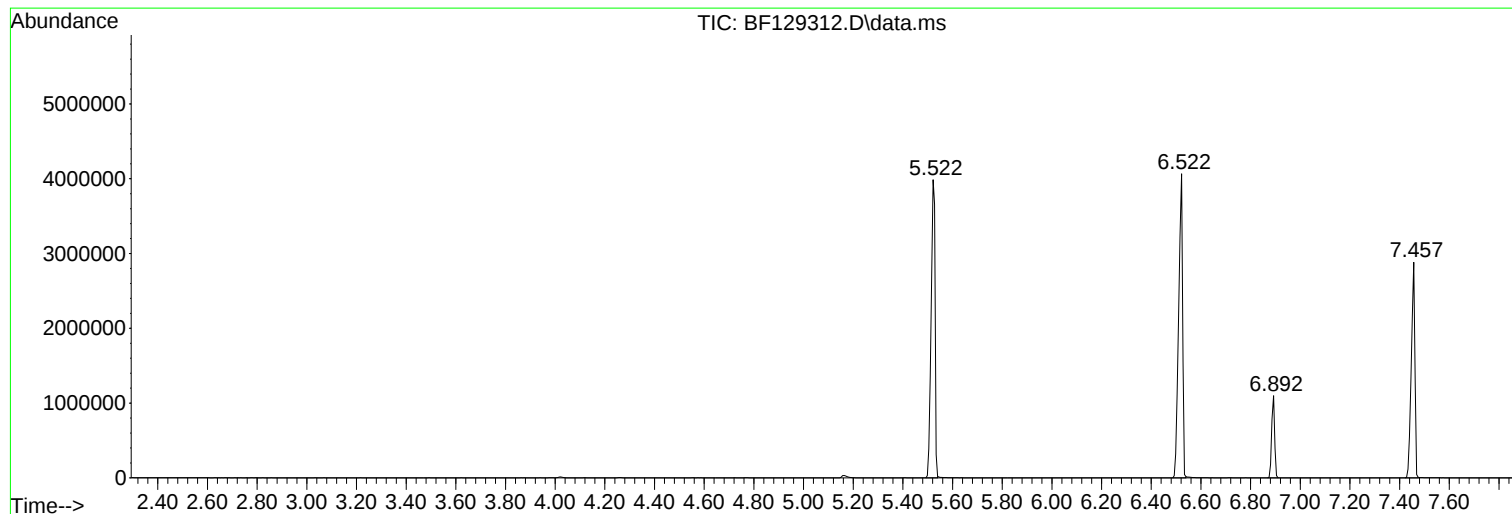

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129312.D
Acq On : 22 Jul 2022 13:08
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129312.D
Acq On : 22 Jul 2022 13:08
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------