


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129305.D
 Acq On : 22 Jul 2022 08:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 13:42:18 2022

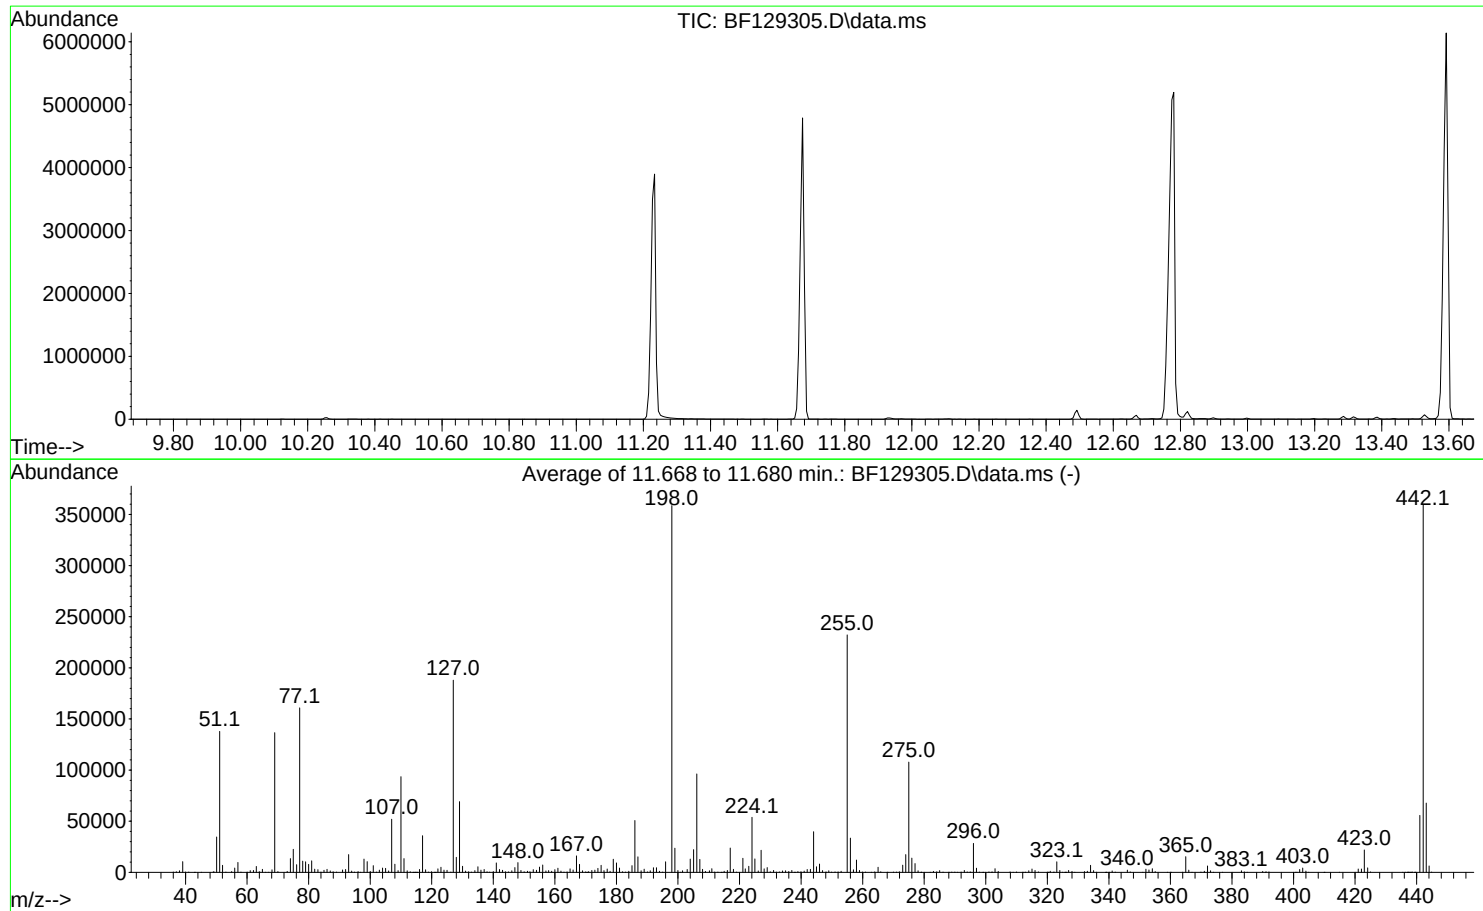




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	137901	PASS
68	69	0.00	2	1.8	2505	PASS
69	198	0.00	100	38.1	136605	PASS
70	69	0.00	2	0.5	744	PASS
127	198	10	80	52.4	187947	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	358613	PASS
199	198	5	9	6.6	23609	PASS
275	198	10	60	30.1	107819	PASS
365	198	1	100	4.3	15354	PASS
441	198	0.01	100	15.5	55696	PASS
442	442	50	100	100.0	359744	PASS
443	442	15	24	18.8	67680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129305.D
 Acq On : 22 Jul 2022 08:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 16:54:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 13:42:18 2022
 Response via : Initial Calibration

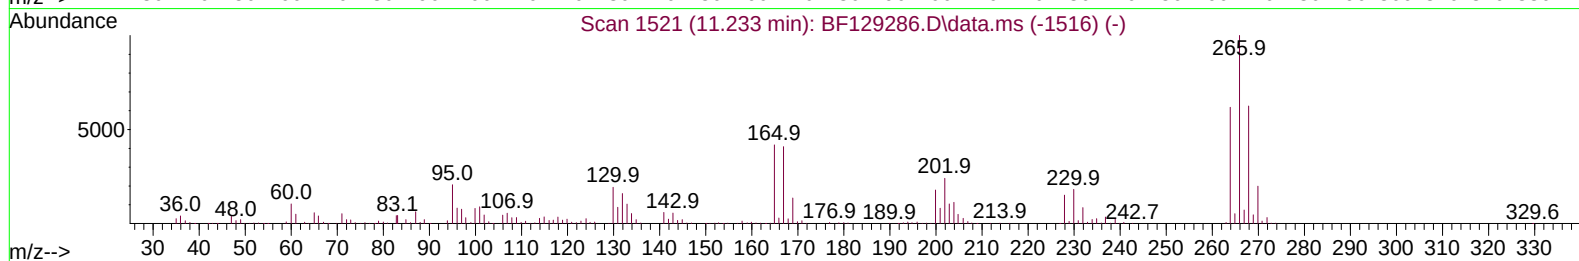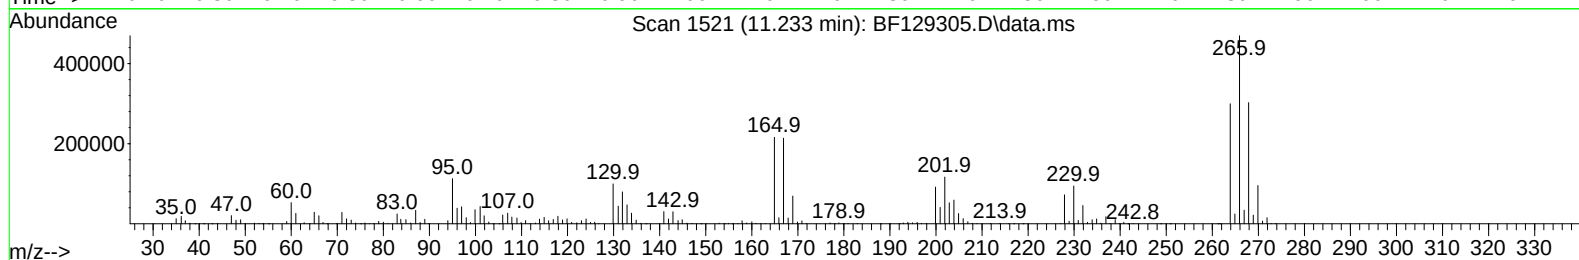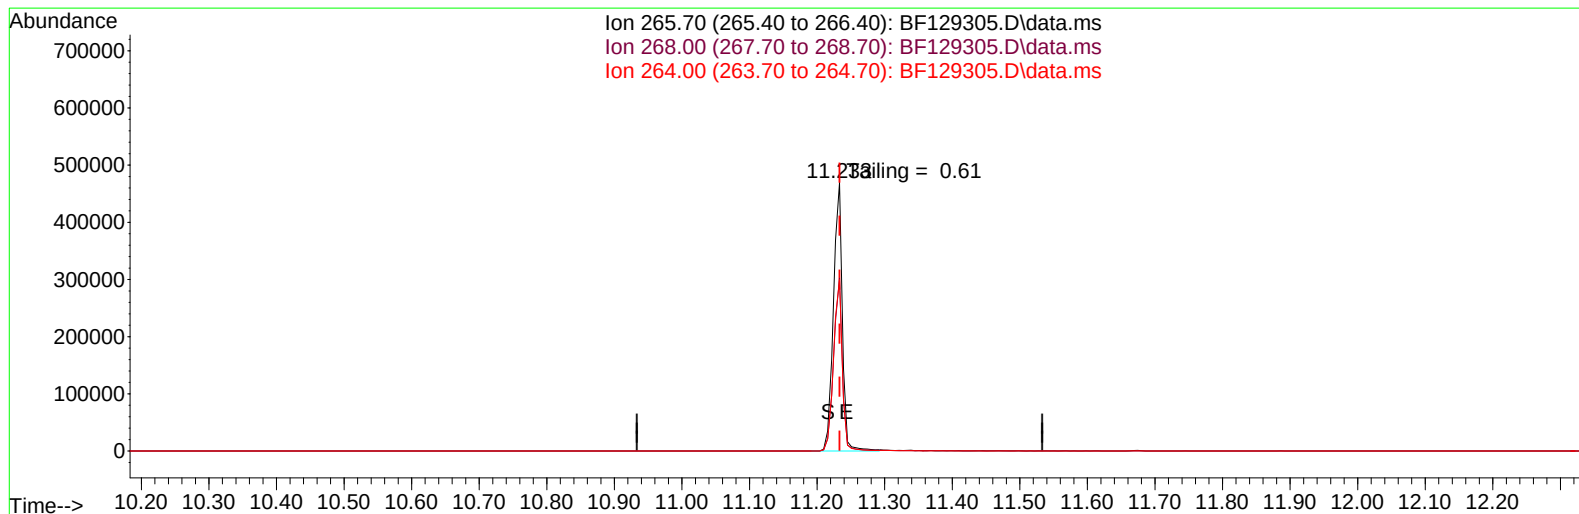

TIC: BF129305.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 376986.68 ng




response 435971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.40
264.00	61.80	63.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129305.D
Acq On : 22 Jul 2022 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 16:54:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

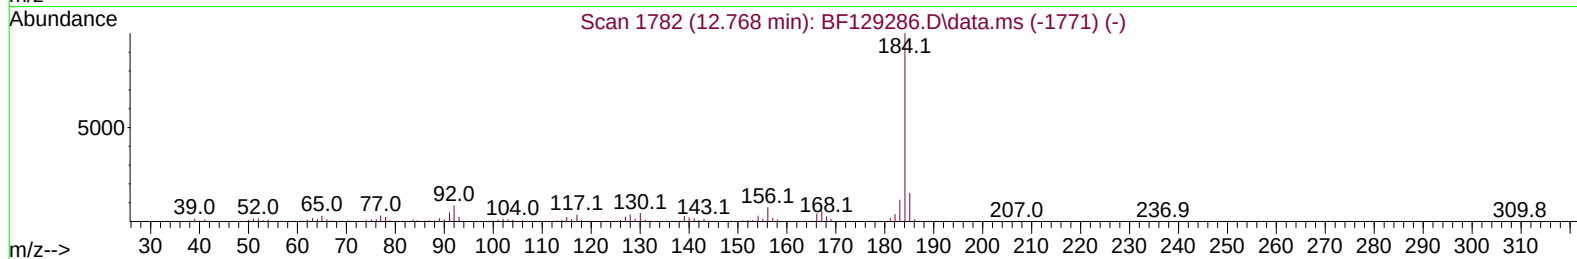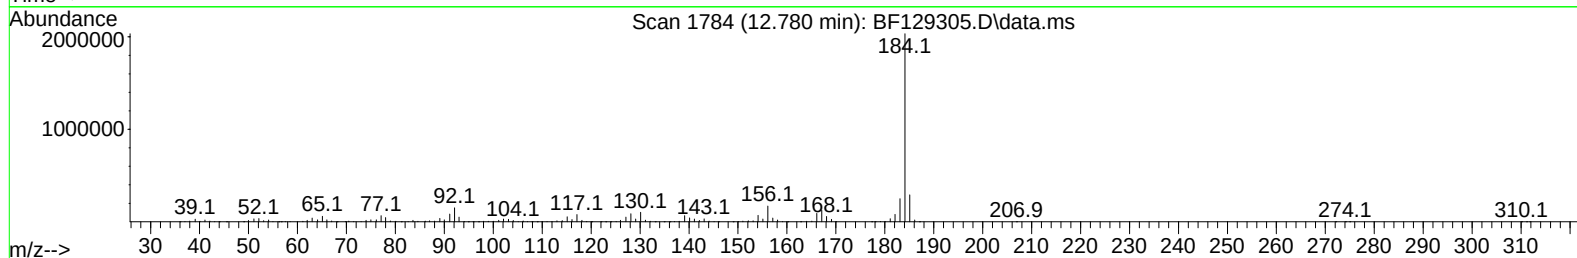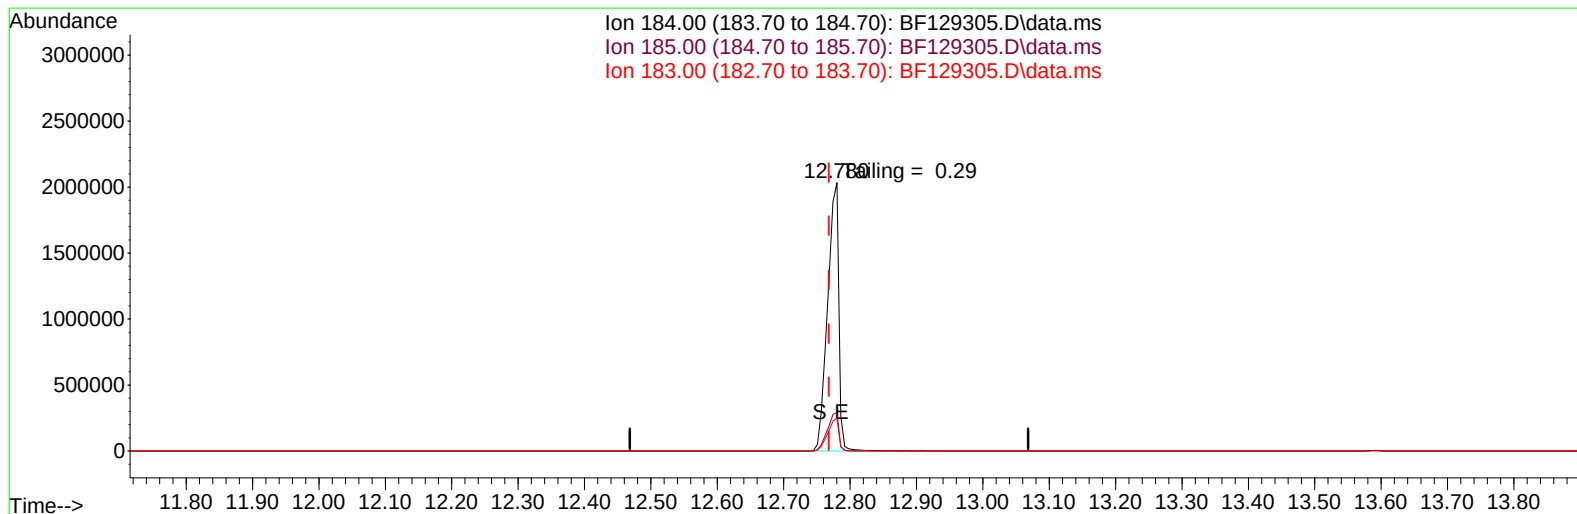

TIC: BF129305.D\data.ms

(77) Benzidine

12.780min (+ 0.012) 76143.97 ng

response 2379024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.31
183.00	11.60	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2022	BNA_F	<u>BF129305.D</u>
Compound Name	Response	Retention Time
DDT	1054514	13.59
DDD	6913	13.28
DDE	301	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7214	1061728	0.68

Instrument :
BNA_F
ClientSampleId :
DFTPP