


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129314.D
 Acq On : 22 Jul 2022 14:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 13:42:18 2022

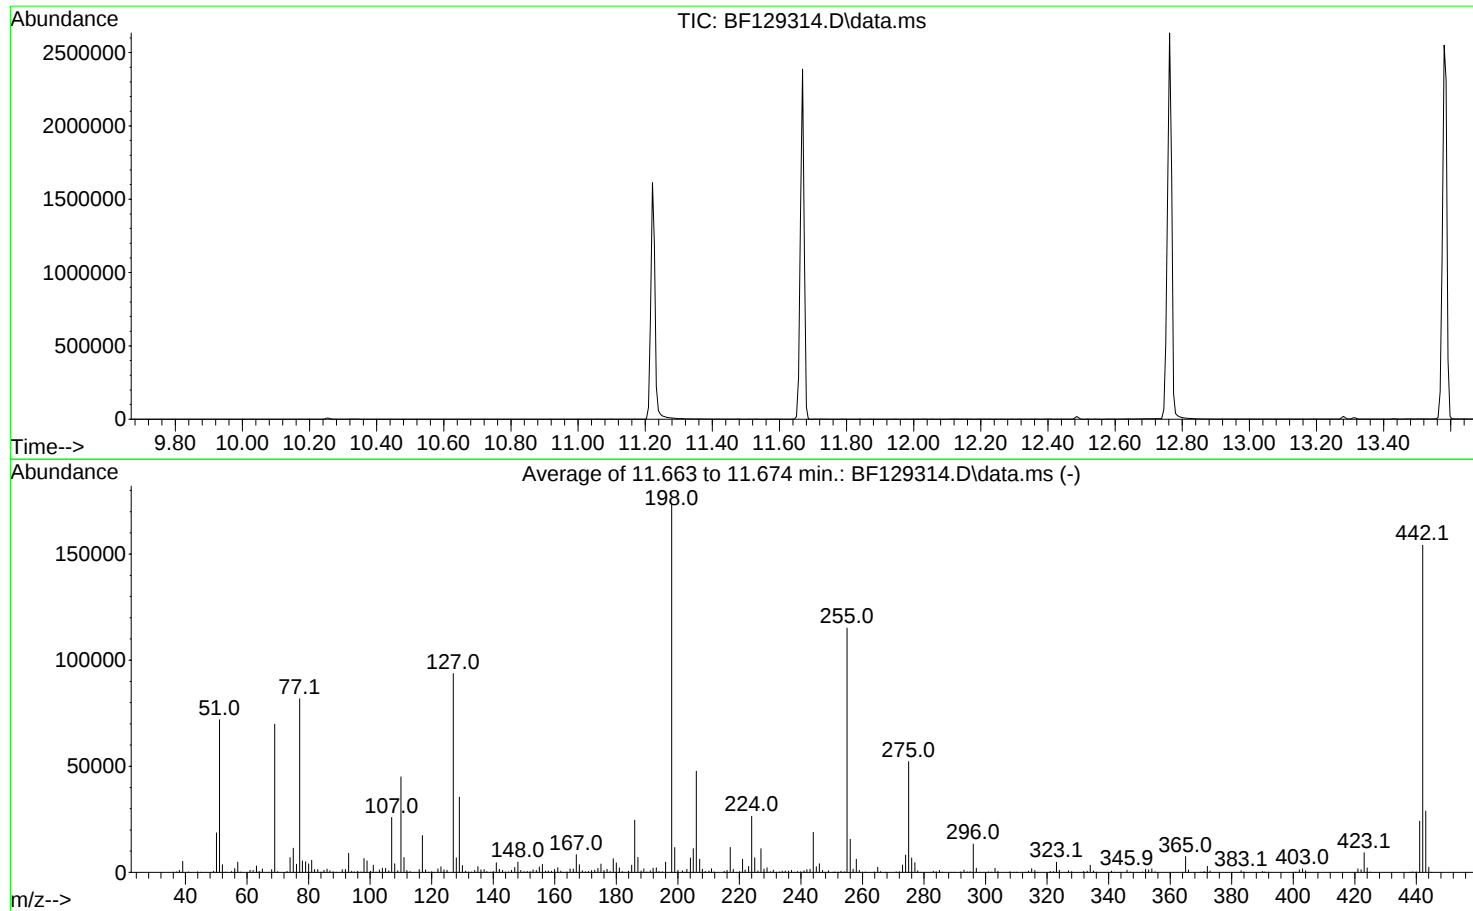




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	71947	PASS
68	69	0.00	2	1.8	1289	PASS
69	198	0.00	100	40.3	69877	PASS
70	69	0.00	2	0.5	331	PASS
127	198	10	80	54.1	93733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173392	PASS
199	198	5	9	6.8	11734	PASS
275	198	10	60	30.1	52163	PASS
365	198	1	100	4.3	7457	PASS
441	198	0.01	100	13.9	24145	PASS
442	442	50	100	100.0	154176	PASS
443	442	15	24	18.7	28877	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
 Data File : BF129314.D
 Acq On : 22 Jul 2022 14:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 16:59:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 13:42:18 2022
 Response via : Initial Calibration

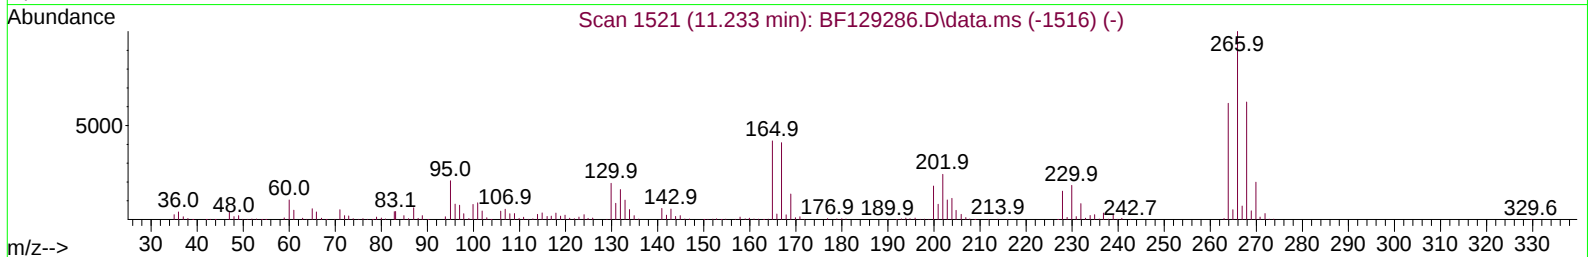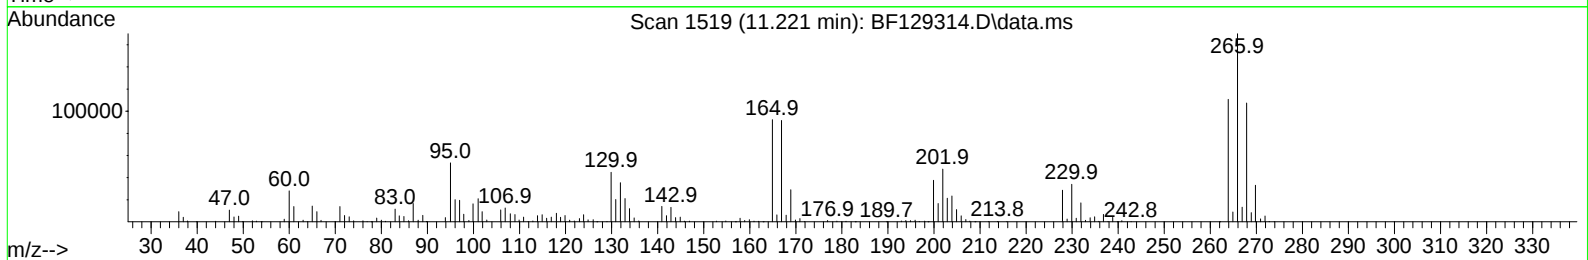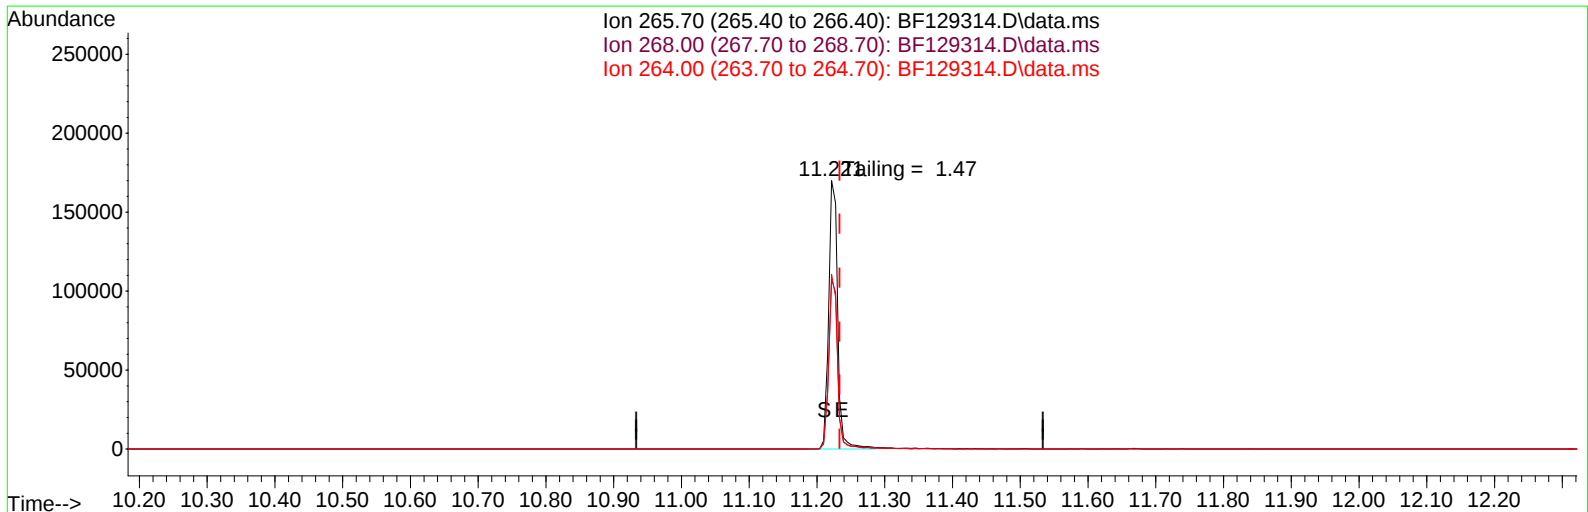

TIC: BF129314.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.012) 29181.90 ng




response 158880

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.15
264.00	61.80	65.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072222\
Data File : BF129314.D
Acq On : 22 Jul 2022 14:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 16:59:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 13:42:18 2022
Response via : Initial Calibration

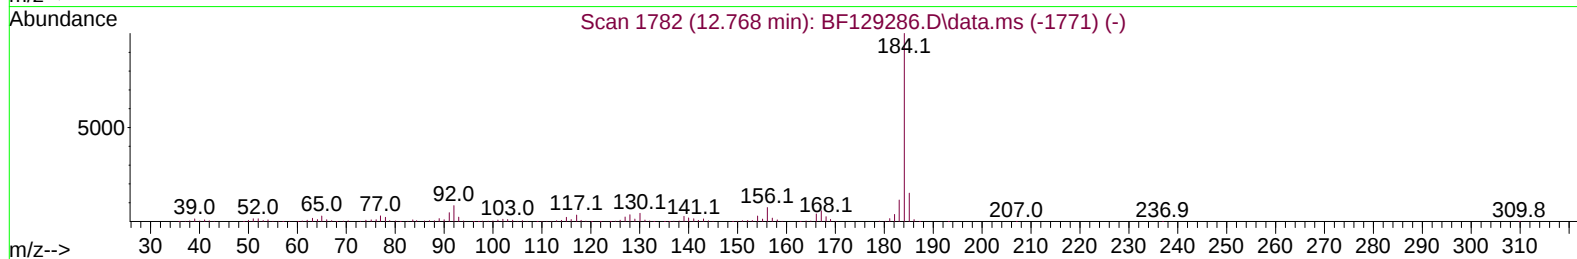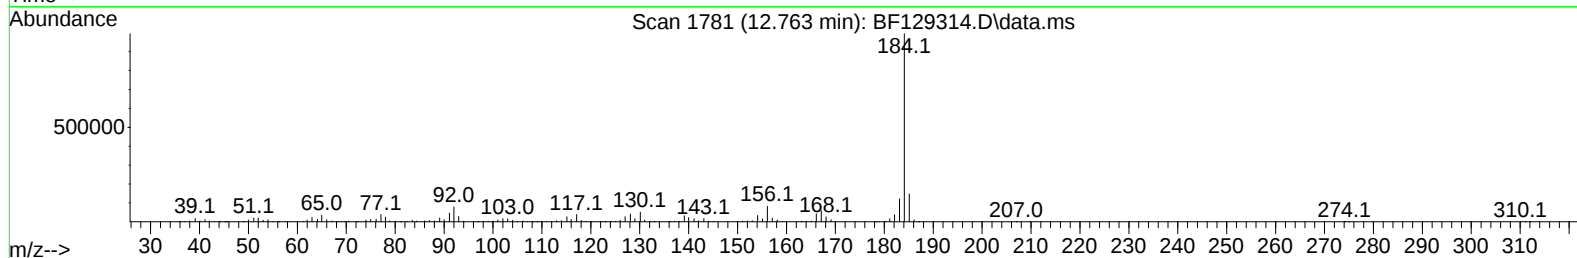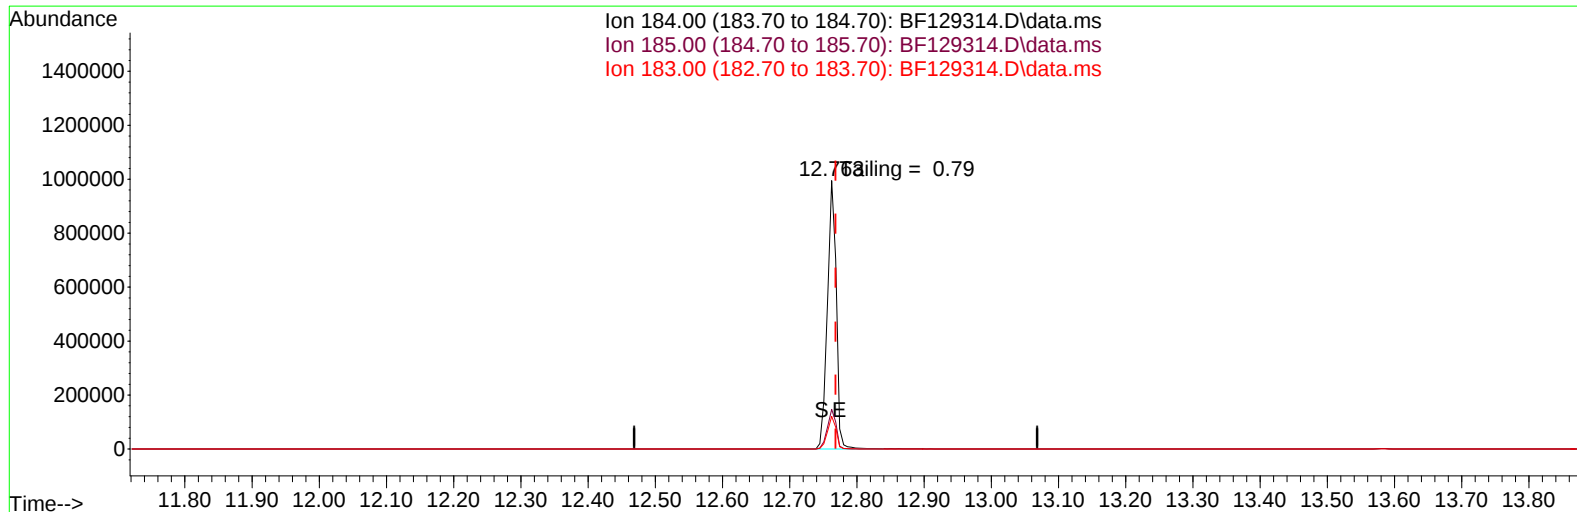

TIC: BF129314.D\data.ms

(77) Benzidine

12.763min (-0.006) 0.00 ng

response 917834

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.80
183.00	11.60	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2022	BNA_F	<u>BF129314.D</u>
Compound Name	Response	Retention Time
DDT	429911	13.58
DDD	3110	13.28
DDE	82	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3192	433103	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP