


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072224\
Data File : BF138600.D
Acq On : 22 Jul 2024 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

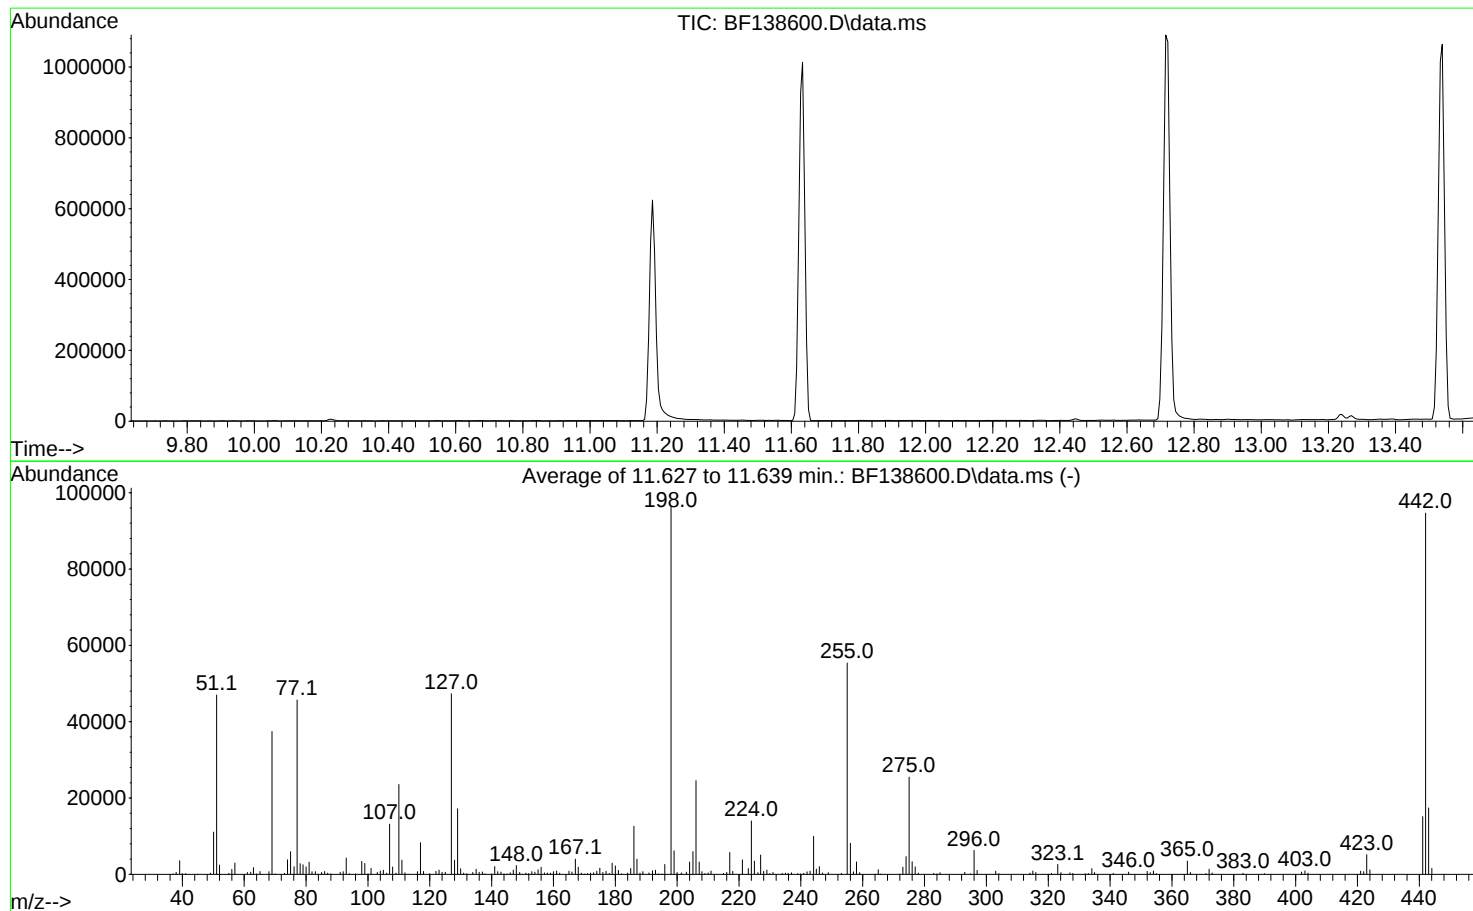




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	46989	PASS
68	69	0.00	2	1.9	696	PASS
69	198	0.00	100	38.9	37456	PASS
70	69	0.00	2	0.3	130	PASS
127	198	10	80	49.1	47320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96379	PASS
199	198	5	9	6.4	6182	PASS
275	198	10	60	26.4	25477	PASS
365	198	1	100	3.6	3493	PASS
441	198	0.01	100	15.7	15151	PASS
442	442	50	100	100.0	94645	PASS
443	442	15	24	18.4	17388	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072224\
Data File : BF138600.D
Acq On : 22 Jul 2024 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 12:06:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

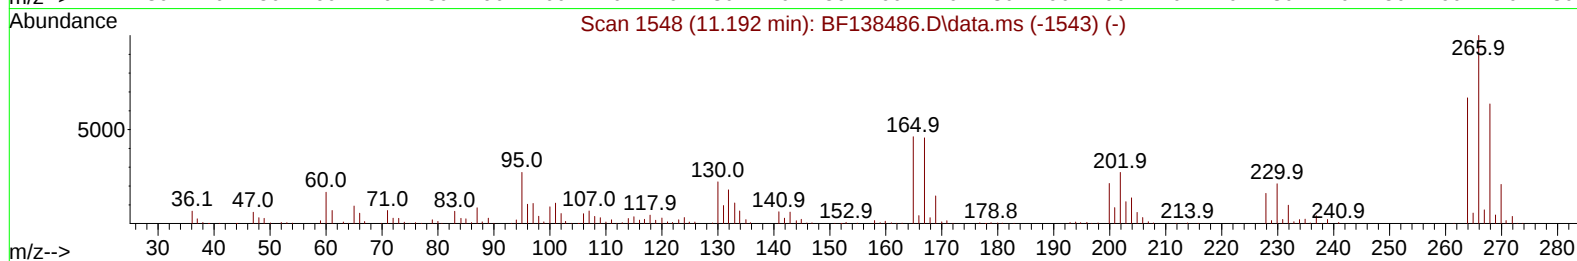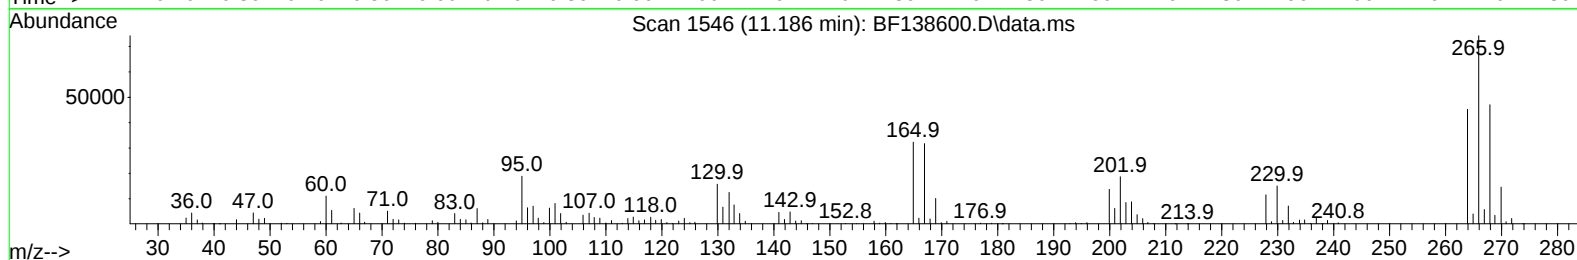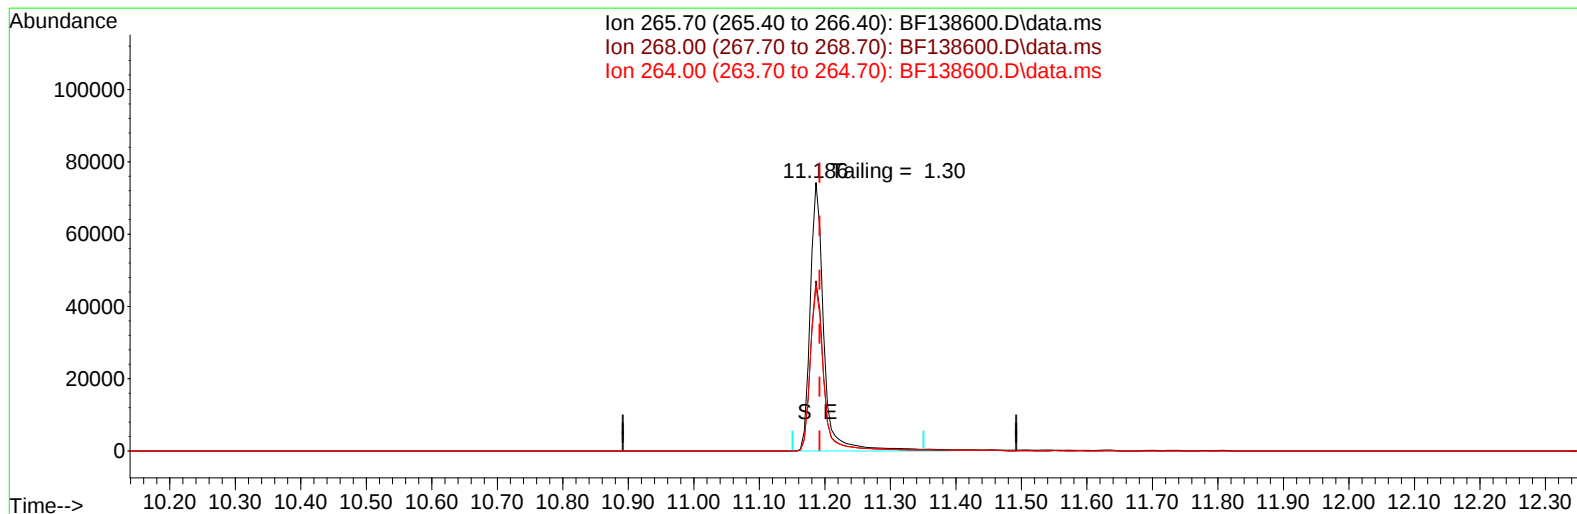

TIC: BF138600.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 36412.58 ng




response 106281

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.36
264.00	66.90	60.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072224\
Data File : BF138600.D
Acq On : 22 Jul 2024 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 12:06:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

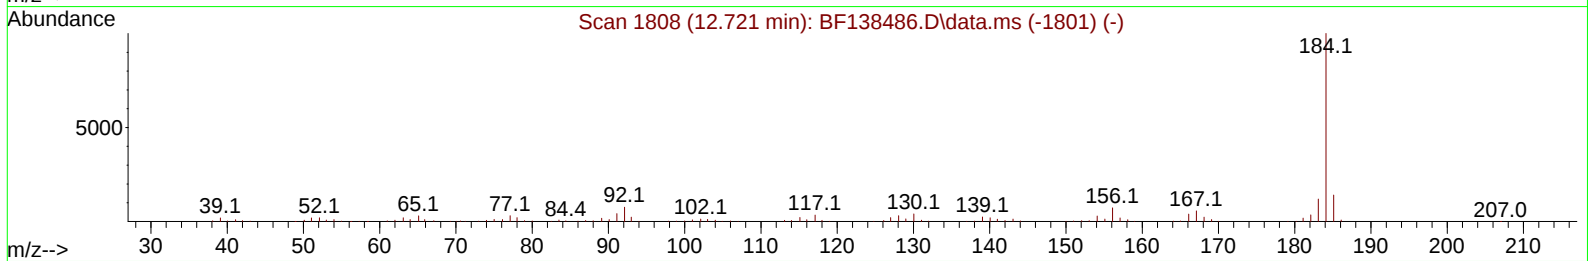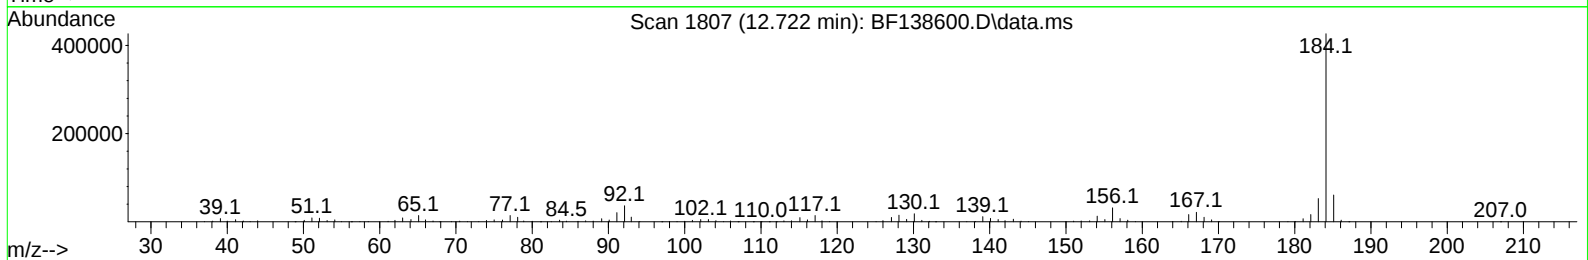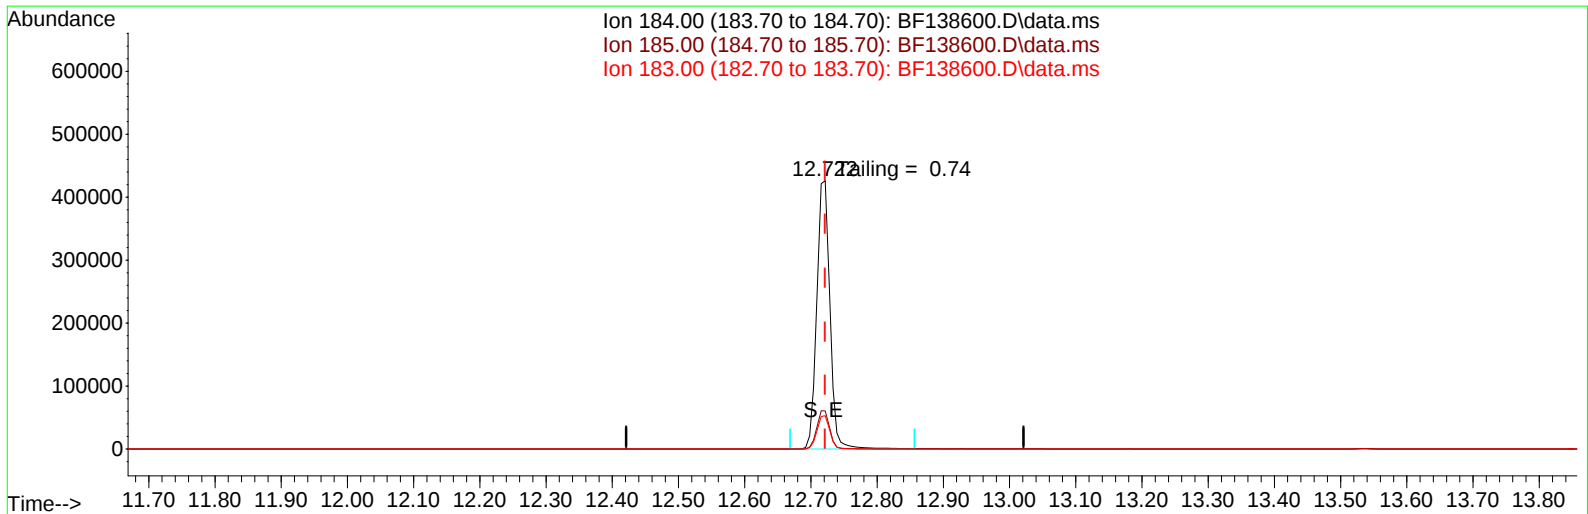

TIC: BF138600.D\data.ms

(77) Benzidine

12.722min (+ 0.001) 0.00 ng

response 586776

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.22
183.00	11.90	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2024	BNA_F	<u>BF138600.D</u>
Compound Name	Response	Retention Time
DDT	257304	13.539
DDD	7310	13.239
DDE	677	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7987	265291	3.01

Instrument :
BNA_F
ClientSampleId :
DFTPP