

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
 Data File : BF143182.D
 Acq On : 22 Jul 2025 11:25
 Operator : RC/JU
 Sample : Q2638-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-31-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	8	16	24	rVB	648231	1027116	39.75%	3.871%
2	5.192	503	510	518	rVB	190948	279385	10.81%	1.053%
3	5.587	571	577	583	rBV	1668419	2249473	87.05%	8.478%
4	6.581	740	746	751	rBV	1755938	2338569	90.50%	8.814%
5	6.963	806	811	816	rBV	632606	760629	29.44%	2.867%
6	7.516	899	905	910	rBV	1246979	1598255	61.85%	6.024%
7	8.245	1023	1029	1034	rBV	772905	996880	38.58%	3.757%
8	8.304	1034	1039	1050	rVB	183802	269161	10.42%	1.014%
9	8.804	1119	1124	1132	rBV2	16324	36355	1.41%	0.137%
10	9.316	1205	1211	1216	rBV	2072299	2583991	100.00%	9.739%
11	9.445	1229	1233	1246	rVB8	11656	32121	1.24%	0.121%
12	9.598	1255	1259	1263	rBV	25892	30636	1.19%	0.115%
13	9.663	1263	1270	1274	rBV2	19608	30193	1.17%	0.114%
14	9.998	1322	1327	1332	rBV	829919	1027043	39.75%	3.871%
15	10.404	1392	1396	1402	rVB	32894	44728	1.73%	0.169%
16	10.710	1443	1448	1455	rVB	271412	369086	14.28%	1.391%
17	10.786	1455	1461	1466	rBV	1049732	1385500	53.62%	5.222%
18	11.016	1489	1500	1505	rBV	64420	110510	4.28%	0.417%
19	11.139	1515	1521	1525	rBV4	26631	39816	1.54%	0.150%
20	11.357	1552	1558	1565	rVB7	20084	41929	1.62%	0.158%
21	11.421	1565	1569	1573	rBV	63364	95634	3.70%	0.360%
22	11.486	1574	1580	1586	rVV	673558	902780	34.94%	3.403%
23	11.539	1586	1589	1593	rVB2	25307	30549	1.18%	0.115%
24	11.704	1613	1617	1621	rBV2	18482	28247	1.09%	0.106%
25	11.933	1651	1656	1659	rBV	44843	72819	2.82%	0.274%
26	11.974	1659	1663	1665	rBV2	79094	119397	4.62%	0.450%
27	12.010	1665	1669	1673	rVV	521098	683752	26.46%	2.577%
28	12.186	1694	1699	1707	rBV4	134214	216311	8.37%	0.815%
29	12.627	1770	1774	1781	rBV4	30605	73802	2.86%	0.278%
30	12.698	1782	1786	1797	rBV3	90311	274643	10.63%	1.035%
31	12.792	1797	1802	1814	rVV	141536	236244	9.14%	0.890%
32	12.927	1821	1825	1834	rVB	49494	101399	3.92%	0.382%
33	13.068	1843	1849	1854	rBV	1333264	1717472	66.47%	6.473%
34	13.504	1920	1923	1928	rBV3	63411	92963	3.60%	0.350%
35	13.962	1996	2001	2008	rBV2	267475	404205	15.64%	1.523%
36	14.121	2023	2028	2035	rVB	632832	894867	34.63%	3.373%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143182.D
Acq On : 22 Jul 2025 11:25
Operator : RC/JU
Sample : Q2638-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-31-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.286	2053	2056	2063	rVB2	62377	82480	3.19%	0.311%
38	14.592	2104	2108	2114	rBV	316281	434294	16.81%	1.637%
39	15.262	2218	2222	2234	rVB	662242	1032105	39.94%	3.890%
40	15.627	2279	2284	2289	rBV	346139	578923	22.40%	2.182%
41	16.127	2364	2369	2375	rBV	447044	757776	29.33%	2.856%
42	17.815	2650	2656	2660	rBV2	239037	577883	22.36%	2.178%
43	18.309	2733	2740	2752	rBV	229055	687829	26.62%	2.592%
44	18.421	2755	2759	2771	rVB4	201121	562113	21.75%	2.119%
45	18.680	2795	2803	2807	rBV4	209781	621814	24.06%	2.344%


Sum of corrected areas: 26531677

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143182.D
Acq On : 22 Jul 2025 11:25
Operator : RC/JU
Sample : Q2638-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-31-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

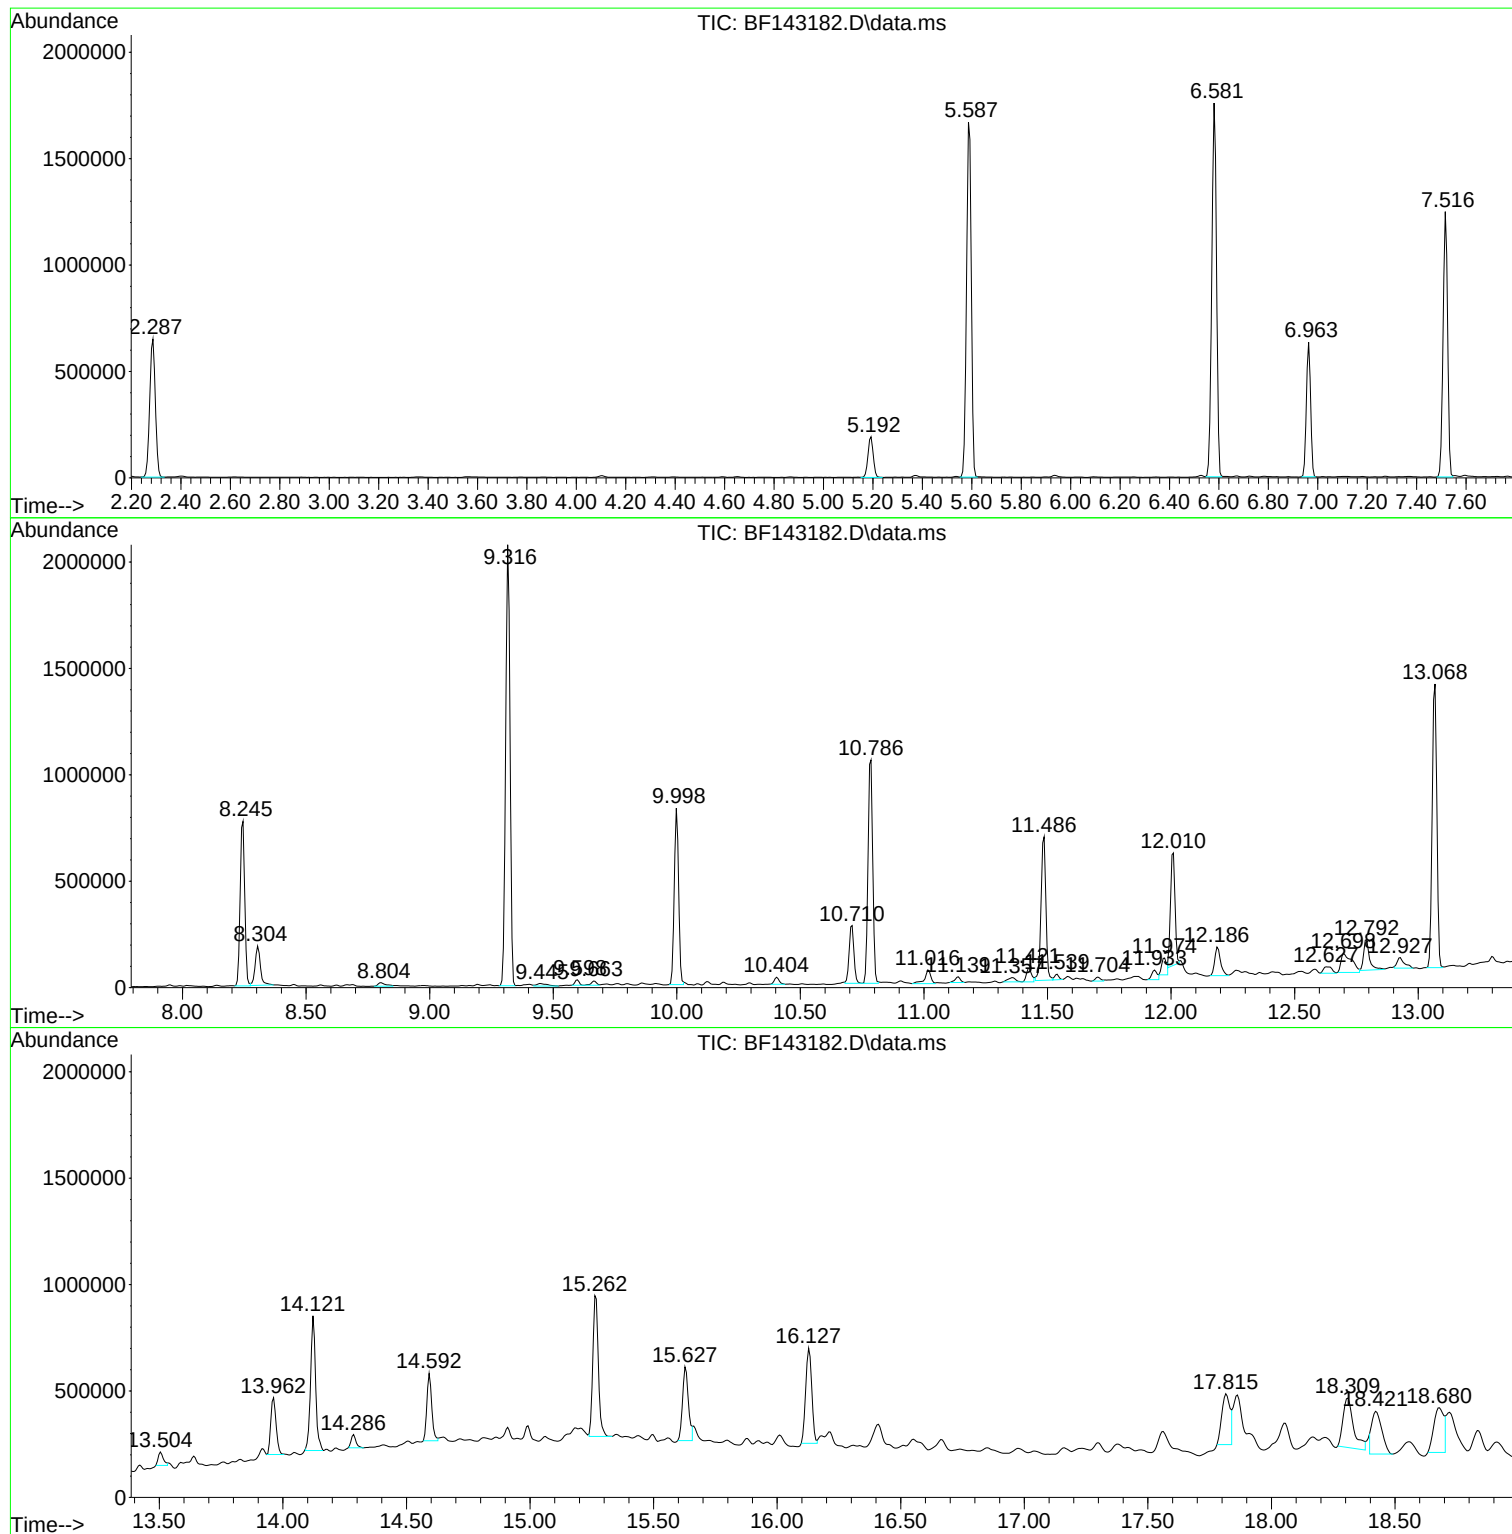

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143182.D
Acq On : 22 Jul 2025 11:25
Operator : RC/JU
Sample : Q2638-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-31-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143182.D
Acq On : 22 Jul 2025 11:25
Operator : RC/JU
Sample : Q2638-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-31-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------