

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
 Data File : BF143184.D
 Acq On : 22 Jul 2025 12:23
 Operator : RC/JU
 Sample : Q2638-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-33-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	9	17	27	rVB	763331	1214969	46.54%	4.863%
2	5.192	503	510	516	rVB	187739	271063	10.38%	1.085%
3	5.592	572	578	583	rVV	1687724	2283447	87.47%	9.139%
4	6.581	740	746	752	rVB	1734329	2358621	90.35%	9.440%
5	6.963	803	811	816	rVB	650583	793773	30.41%	3.177%
6	7.516	899	905	910	rBV	1246052	1595366	61.11%	6.385%
7	8.245	1023	1029	1034	rBV	826518	1036234	39.70%	4.147%
8	8.304	1034	1039	1050	rVB	122923	179026	6.86%	0.716%
9	8.798	1119	1123	1133	rBV2	13691	32366	1.24%	0.130%
10	9.316	1205	1211	1216	rBV	2088653	2610474	100.00%	10.448%
11	9.998	1322	1327	1332	rBV	882605	1086777	41.63%	4.349%
12	10.404	1392	1396	1402	rVB	27204	37405	1.43%	0.150%
13	10.710	1435	1448	1455	rBV2	138733	221865	8.50%	0.888%
14	10.786	1455	1461	1466	rBV	1135359	1451048	55.59%	5.807%
15	11.016	1497	1500	1505	rVB	28462	40119	1.54%	0.161%
16	11.139	1517	1521	1526	rVB	27960	36961	1.42%	0.148%
17	11.357	1552	1558	1565	rBV5	16970	38469	1.47%	0.154%
18	11.422	1565	1569	1574	rBV	48222	81143	3.11%	0.325%
19	11.486	1574	1580	1586	rVV	743166	972459	37.25%	3.892%
20	11.539	1586	1589	1593	rVB2	20717	26219	1.00%	0.105%
21	11.704	1613	1617	1624	rBV	56619	83169	3.19%	0.333%
22	11.933	1652	1656	1659	rBV	30681	48684	1.86%	0.195%
23	11.974	1659	1663	1664	rVV2	67266	88289	3.38%	0.353%
24	12.010	1664	1669	1681	rVB2	568741	891330	34.14%	3.567%
25	12.186	1694	1699	1707	rVB4	99976	161605	6.19%	0.647%
26	12.527	1753	1757	1761	rBV4	23699	36866	1.41%	0.148%
27	12.627	1770	1774	1775	rBV2	23097	30101	1.15%	0.120%
28	12.698	1782	1786	1797	rBV2	81647	237139	9.08%	0.949%
29	12.786	1797	1801	1814	rVV	123108	213185	8.17%	0.853%
30	12.927	1822	1825	1834	rVB	48722	75638	2.90%	0.303%
31	13.068	1843	1849	1854	rBV	1411398	1790818	68.60%	7.167%
32	13.504	1920	1923	1928	rBV3	45911	64431	2.47%	0.258%
33	13.963	1996	2001	2010	rBV2	218298	323570	12.40%	1.295%
34	14.121	2024	2028	2040	rVB	746136	1206783	46.23%	4.830%
35	14.592	2104	2108	2114	rBV	240062	328703	12.59%	1.316%
36	15.262	2218	2222	2233	rVB	517995	797492	30.55%	3.192%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143184.D
Acq On : 22 Jul 2025 12:23
Operator : RC/JU
Sample : Q2638-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-33-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.633	2280	2285	2300	rVB	313351	583674	22.36%	2.336%
38	16.127	2364	2369	2374	rBV	319402	533515	20.44%	2.135%
39	17.815	2650	2656	2660	rBV2	172278	418940	16.05%	1.677%
40	18.303	2734	2739	2747	rBV2	133442	297624	11.40%	1.191%
41	18.674	2796	2802	2807	rBV3	152614	407092	15.59%	1.629%




Sum of corrected areas: 24986452

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143184.D
Acq On : 22 Jul 2025 12:23
Operator : RC/JU
Sample : Q2638-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-33-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

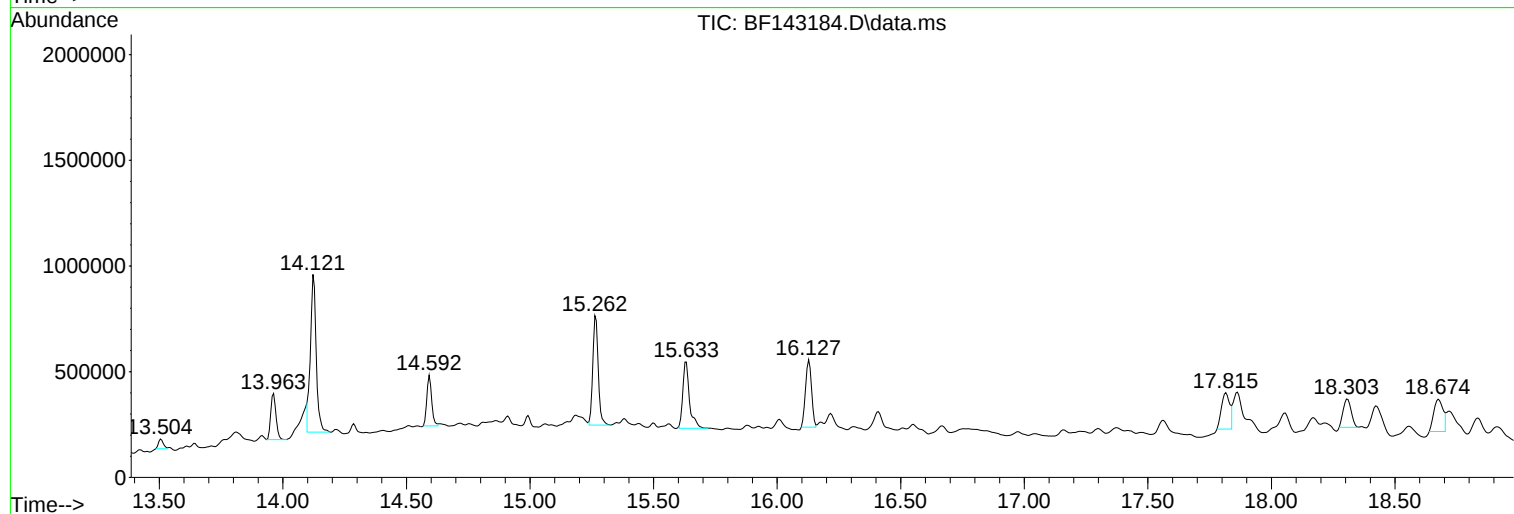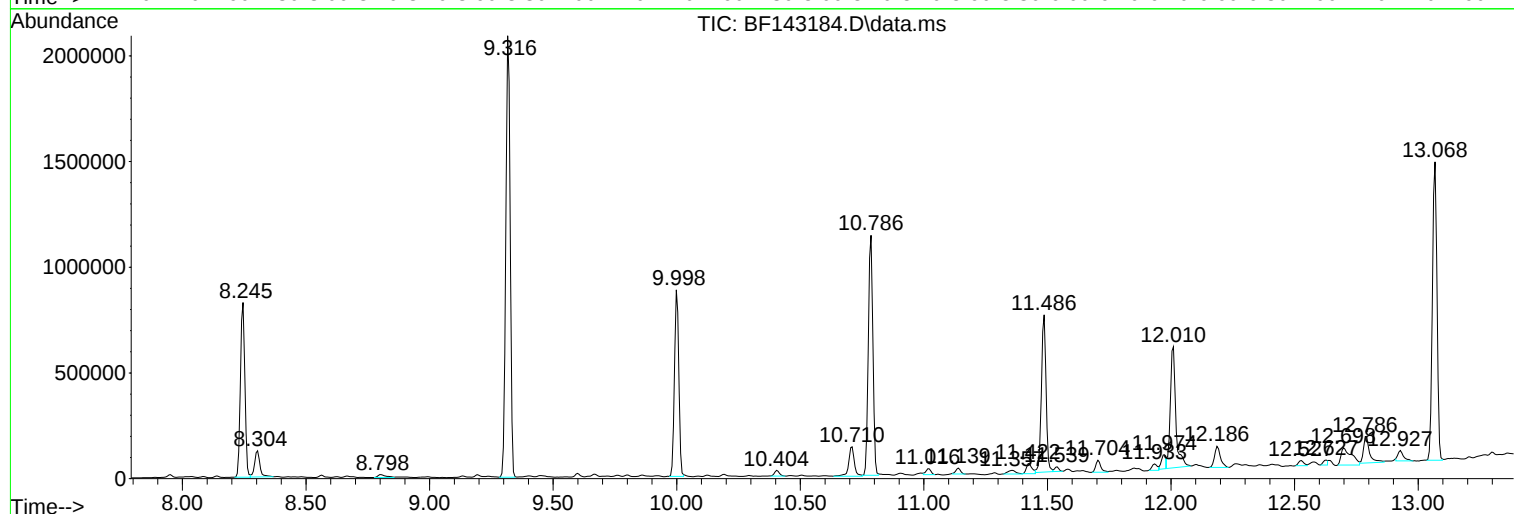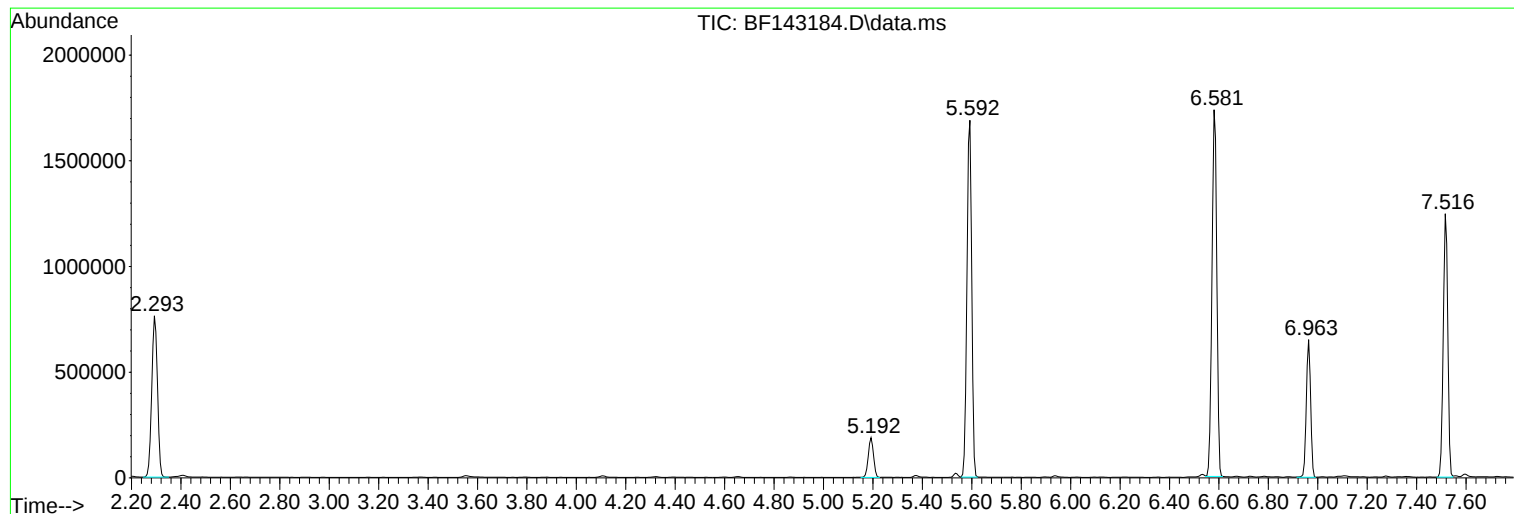

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143184.D
Acq On : 22 Jul 2025 12:23
Operator : RC/JU
Sample : Q2638-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-33-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143184.D
Acq On : 22 Jul 2025 12:23
Operator : RC/JU
Sample : Q2638-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-33-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------