

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072315\
 Data File : BF080601.D
 Acq On : 23 Jul 2015 19:44
 Operator : TP/UM
 Sample : PB84614BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84614BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.464	206	208	211	rVB	10520	13711	1.35%	0.160%
2	5.104	262	264	267	rBV	323479	320161	31.49%	3.744%
3	5.527	298	301	303	rBV	754418	880500	86.60%	10.297%
4	5.950	336	338	340	rBV	24373	23671	2.33%	0.277%
5	6.556	389	391	393	rBV	1047494	931612	91.63%	10.895%
6	6.704	402	404	406	rBV	1157866	933380	91.81%	10.915%
7	6.945	423	425	427	rVB	353698	276044	27.15%	3.228%
8	7.105	436	439	441	rBV	787803	723422	71.15%	8.460%
9	7.505	472	474	476	rBV	727876	564378	55.51%	6.600%
10	8.236	536	538	540	rBV	401274	330856	32.54%	3.869%
11	9.310	630	632	634	rBV	1316062	1016689	100.00%	11.890%
12	9.996	689	692	694	rVB	324983	331496	32.61%	3.877%
13	10.773	758	760	763	rBV	587525	532209	52.35%	6.224%
14	11.482	819	822	824	rBV	310518	322053	31.68%	3.766%
15	13.082	960	962	965	rBV	1038094	906115	89.12%	10.597%
16	14.225	1059	1062	1064	rBV	191717	258387	25.41%	3.022%
17	15.837	1201	1203	1206	rBV	158311	186296	18.32%	2.179%


Sum of corrected areas: 8550980

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072315\
Data File : BF080601.D
Acq On : 23 Jul 2015 19:44
Operator : TP/UM
Sample : PB84614BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84614BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

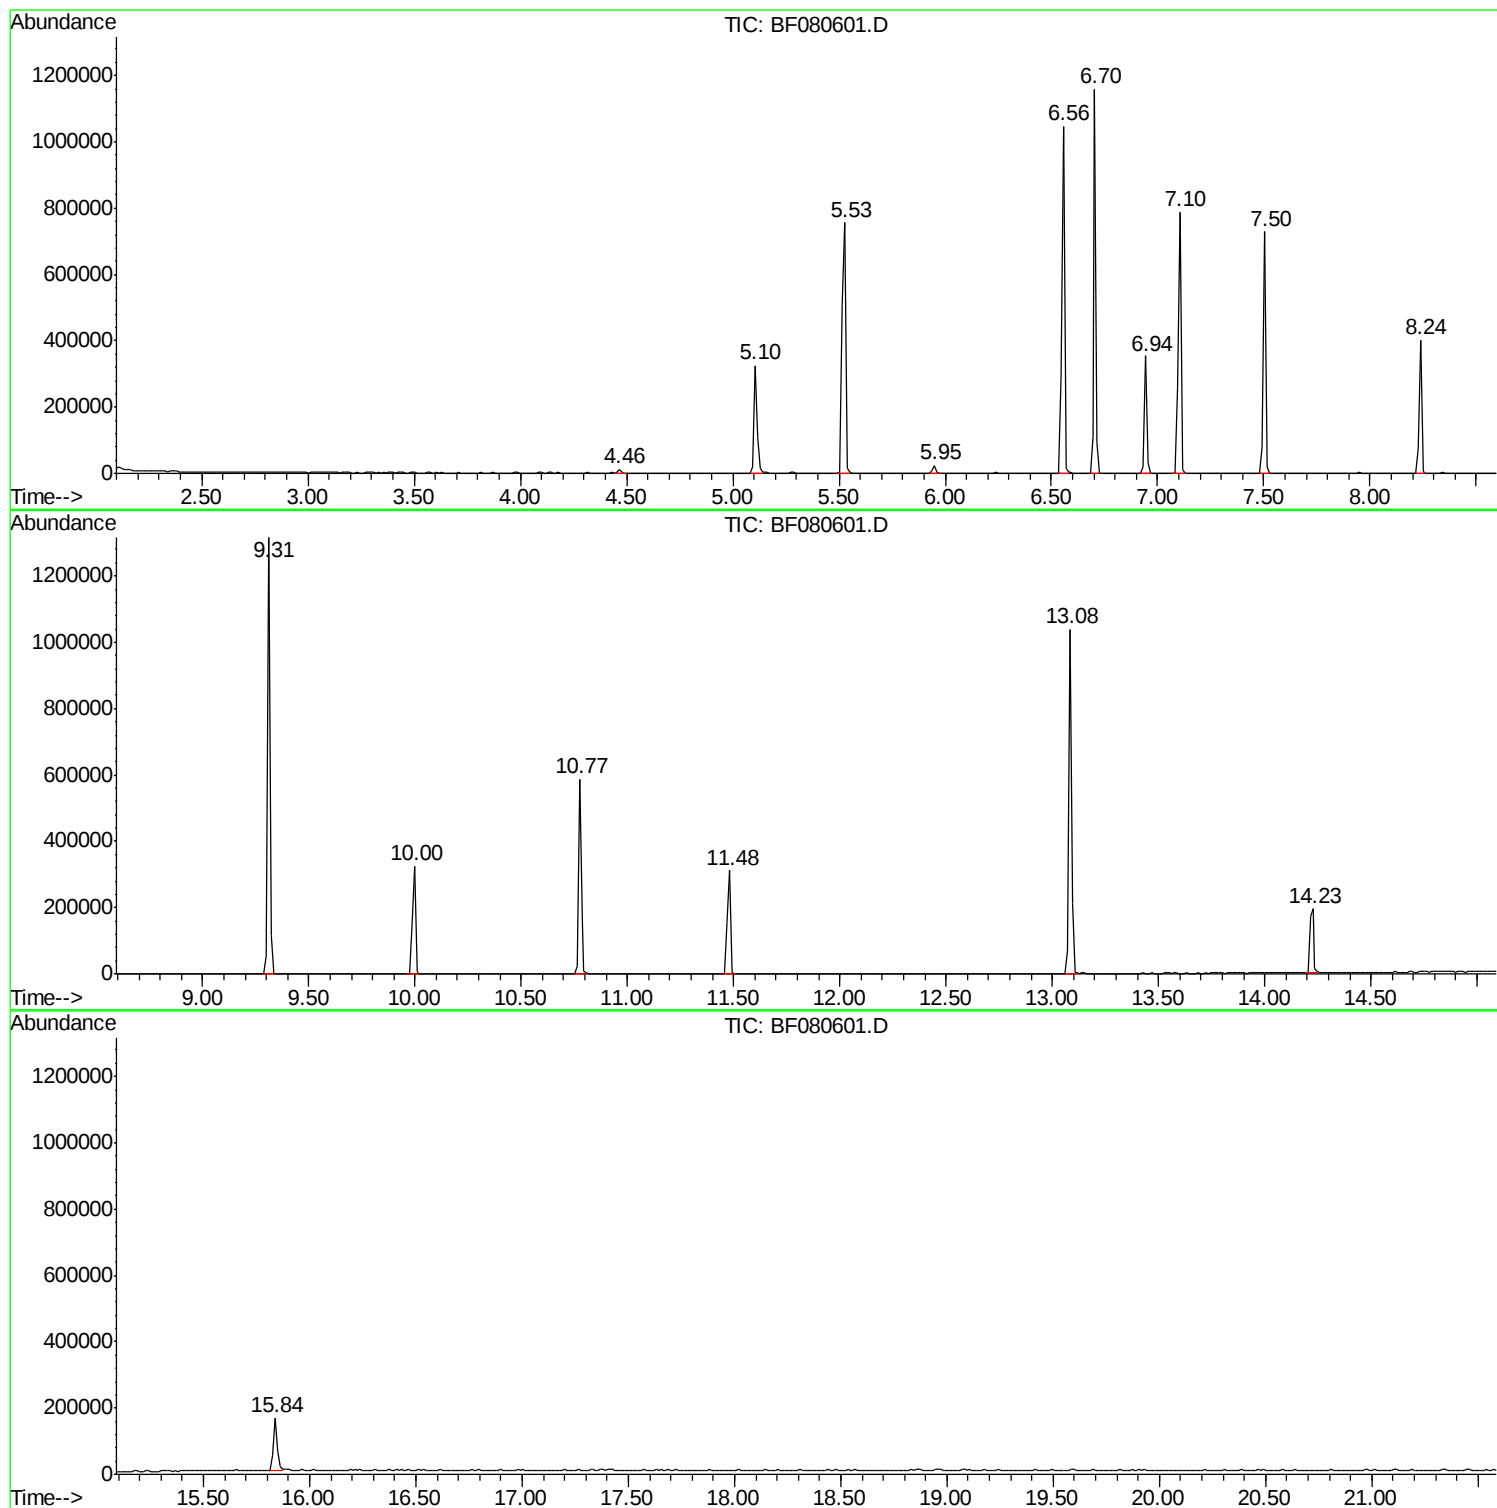

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072315\
Data File : BF080601.D
Acq On : 23 Jul 2015 19:44
Operator : TP/UM
Sample : PB84614BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84614BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.10	23.20 ng	320161	1,4-Dichlorobenzene-d4	6.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
3		Diacetamide	101	C4H7NO2	000625-77-4	9
4		Butane	58	C4H10	000106-97-8	9
5		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

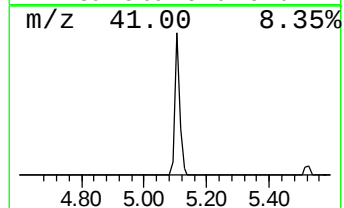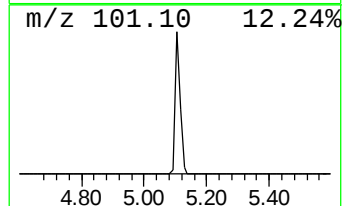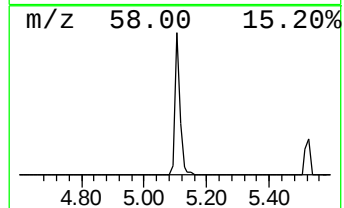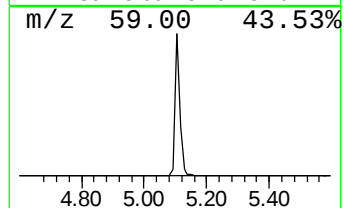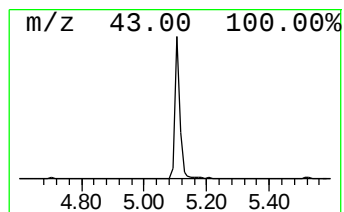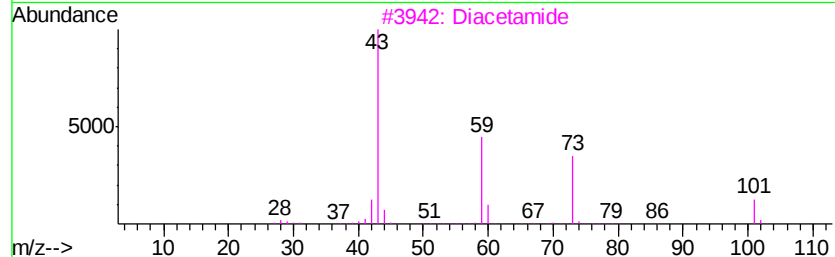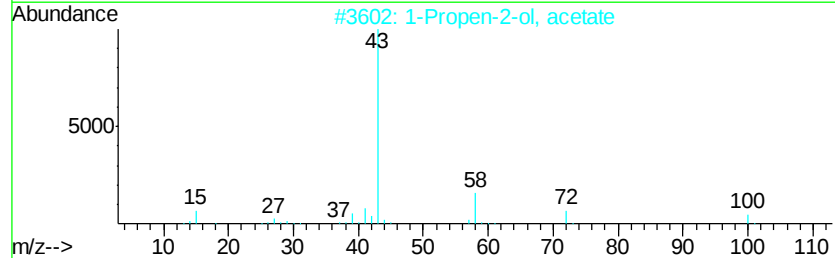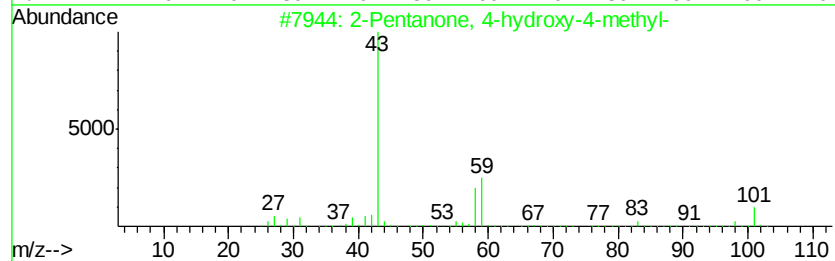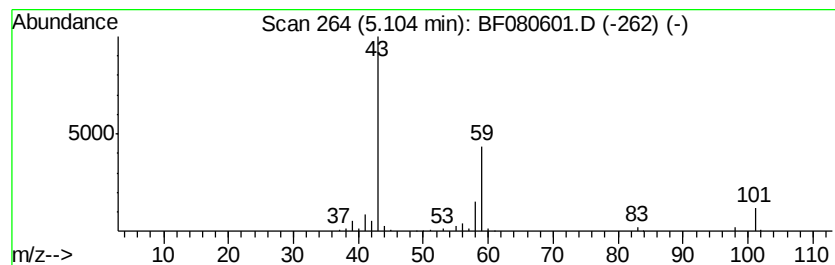

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072315\
Data File : BF080601.D
Acq On : 23 Jul 2015 19:44
Operator : TP/UM
Sample : PB84614BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84614BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.70 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.70	67.63 ng	933380	1,4-Dichlorobenzene-d4	6.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	25
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	14

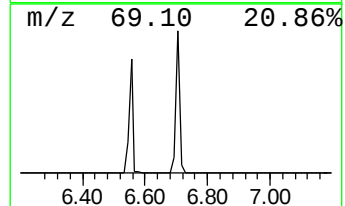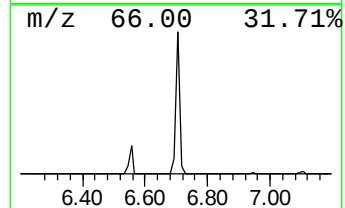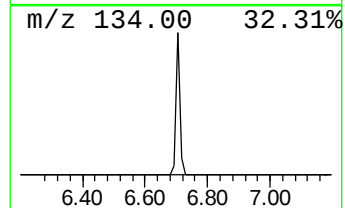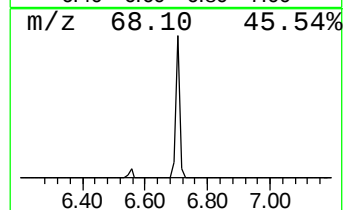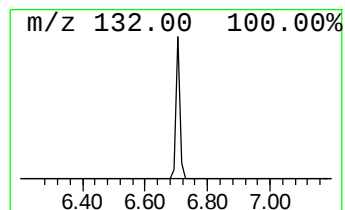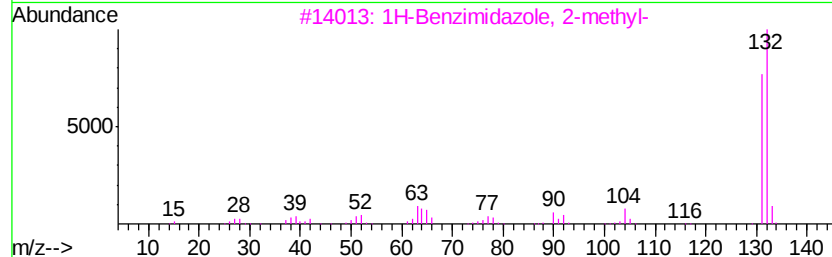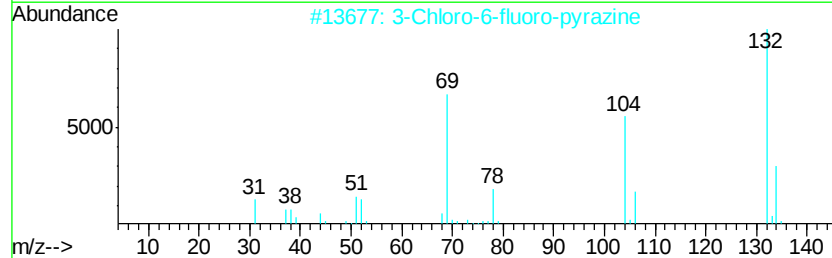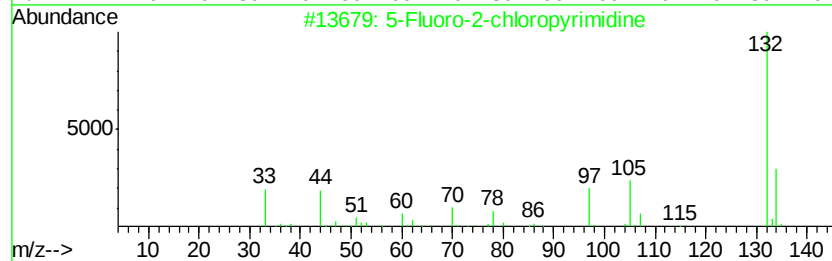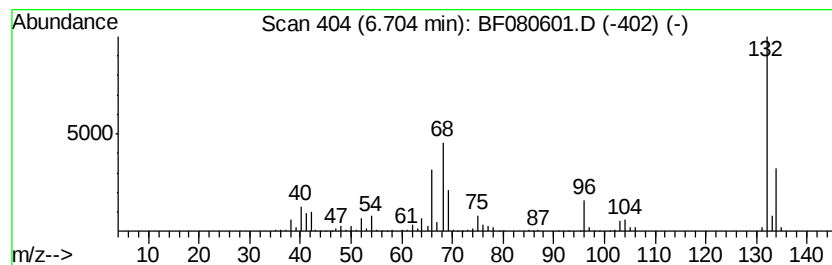

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072315\
Data File : BF080601.D
Acq On : 23 Jul 2015 19:44
Operator : TP/UM
Sample : PB84614BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84614BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.10	23.2	ng	320161	1	6.94	276044	20.0
unknown6.70	6.70	67.6	ng	933380	1	6.94	276044	20.0