


Data Path : Z:\HPCHEM1\BNA_F\Data\BF072315\
Data File : BF080604.D
Acq On : 23 Jul 2015 21:40
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 23 19:10:33 2015

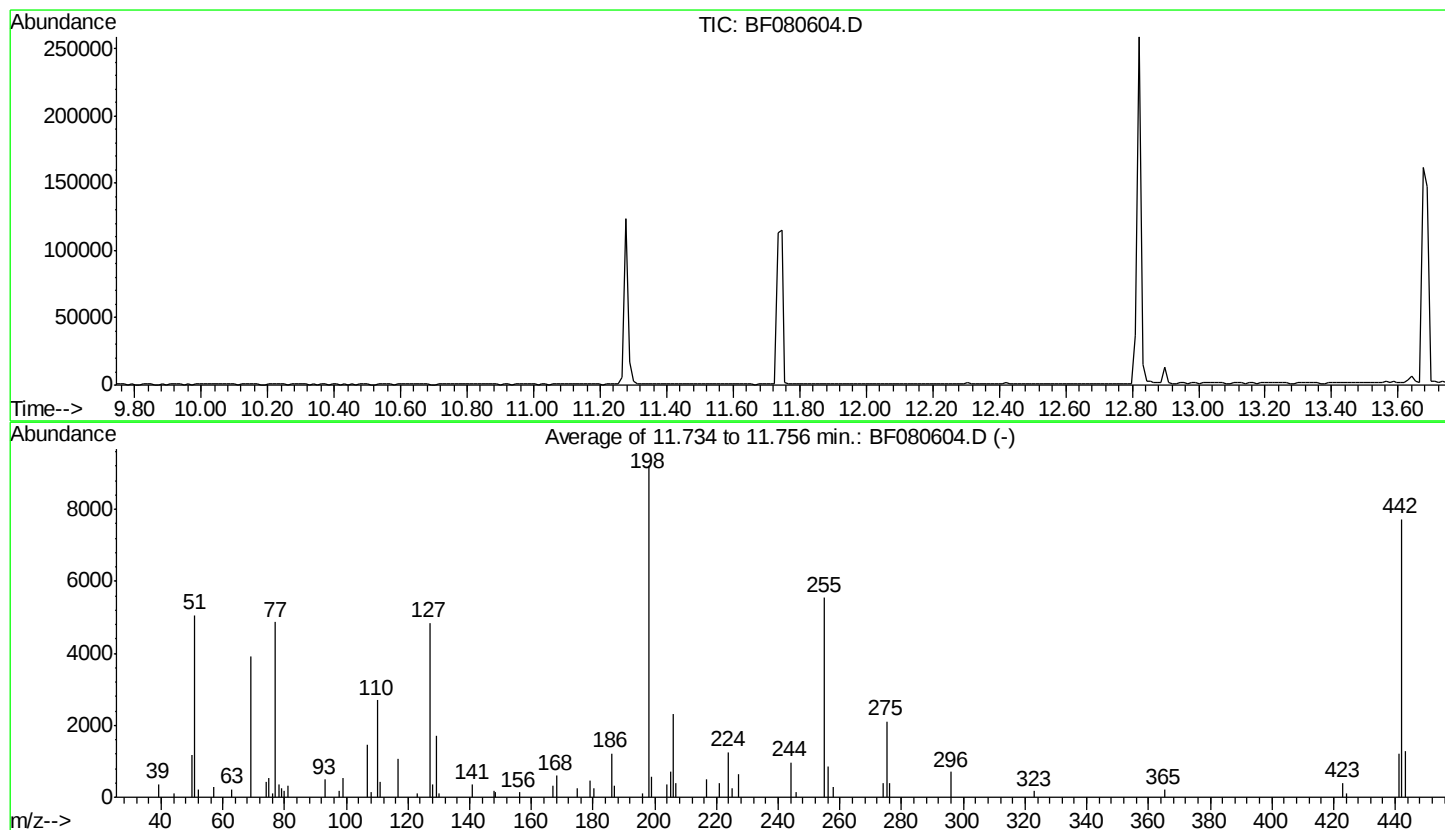

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	5069	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.6	3921	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	4854	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9213	PASS
199	198	5	9	6.1	563	PASS
275	198	10	60	22.8	2105	PASS
365	198	1	100	2.3	213	PASS
441	442	0.01	24	15.6	1205	PASS
442	198	50	100	84.0	7736	PASS
443	442	15	24	16.5	1280	PASS