

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089223.D
 Acq On : 23 Jul 2016 7:52
 Operator : UM/SJ
 Sample : H4129-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Quant Time: Jul 25 01:05:12 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 19:03:15 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	45045	20.00	ng	-0.02
21) Naphthalene-d8	7.86	136	198230	20.00	ng	-0.02
38) Acenaphthene-d10	9.61	164	95188	20.00	ng	-0.02
63) Phenanthrene-d10	11.08	188	185377	20.00	ng	-0.02
75) Chrysene-d12	13.70	240	143289	20.00	ng	-0.02
86) Perylene-d12	15.05	264	103401	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	152268	51.41	ng	-0.03
7) Phenol-d6	6.23	99	128595	33.67	ng	-0.05
23) Nitrobenzene-d5	7.15	82	360276	96.57	ng	-0.02
41) 2,4,6-Tribromophenol	10.40	330	118462	138.23	ng	-0.02
44) 2-Fluorobiphenyl	8.95	172	676206	97.88	ng	-0.02
78) Terphenyl-d14	12.67	244	597148	90.39	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.34	77	7235	2.61	ng	# 71
19) n-Nitroso-di-n-propylamine	7.15	70	47262	18.92	ng	# 78
25) Isophorone	7.15	82	274766	39.96	ng	# 66
50) 2,6-Dinitrotoluene	9.61	165	11571	7.02	ng	# 28
56) 2,4-Dinitrotoluene	9.61	165	11571	5.45	ng	# 10
66) 4-Bromophenyl-phenylether	10.40	248	9379	5.11	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089223.D
Acq On : 23 Jul 2016 7:52
Operator : UM/SJ
Sample : H4129-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELD BLANK

Quant Time: Jul 25 01:05:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

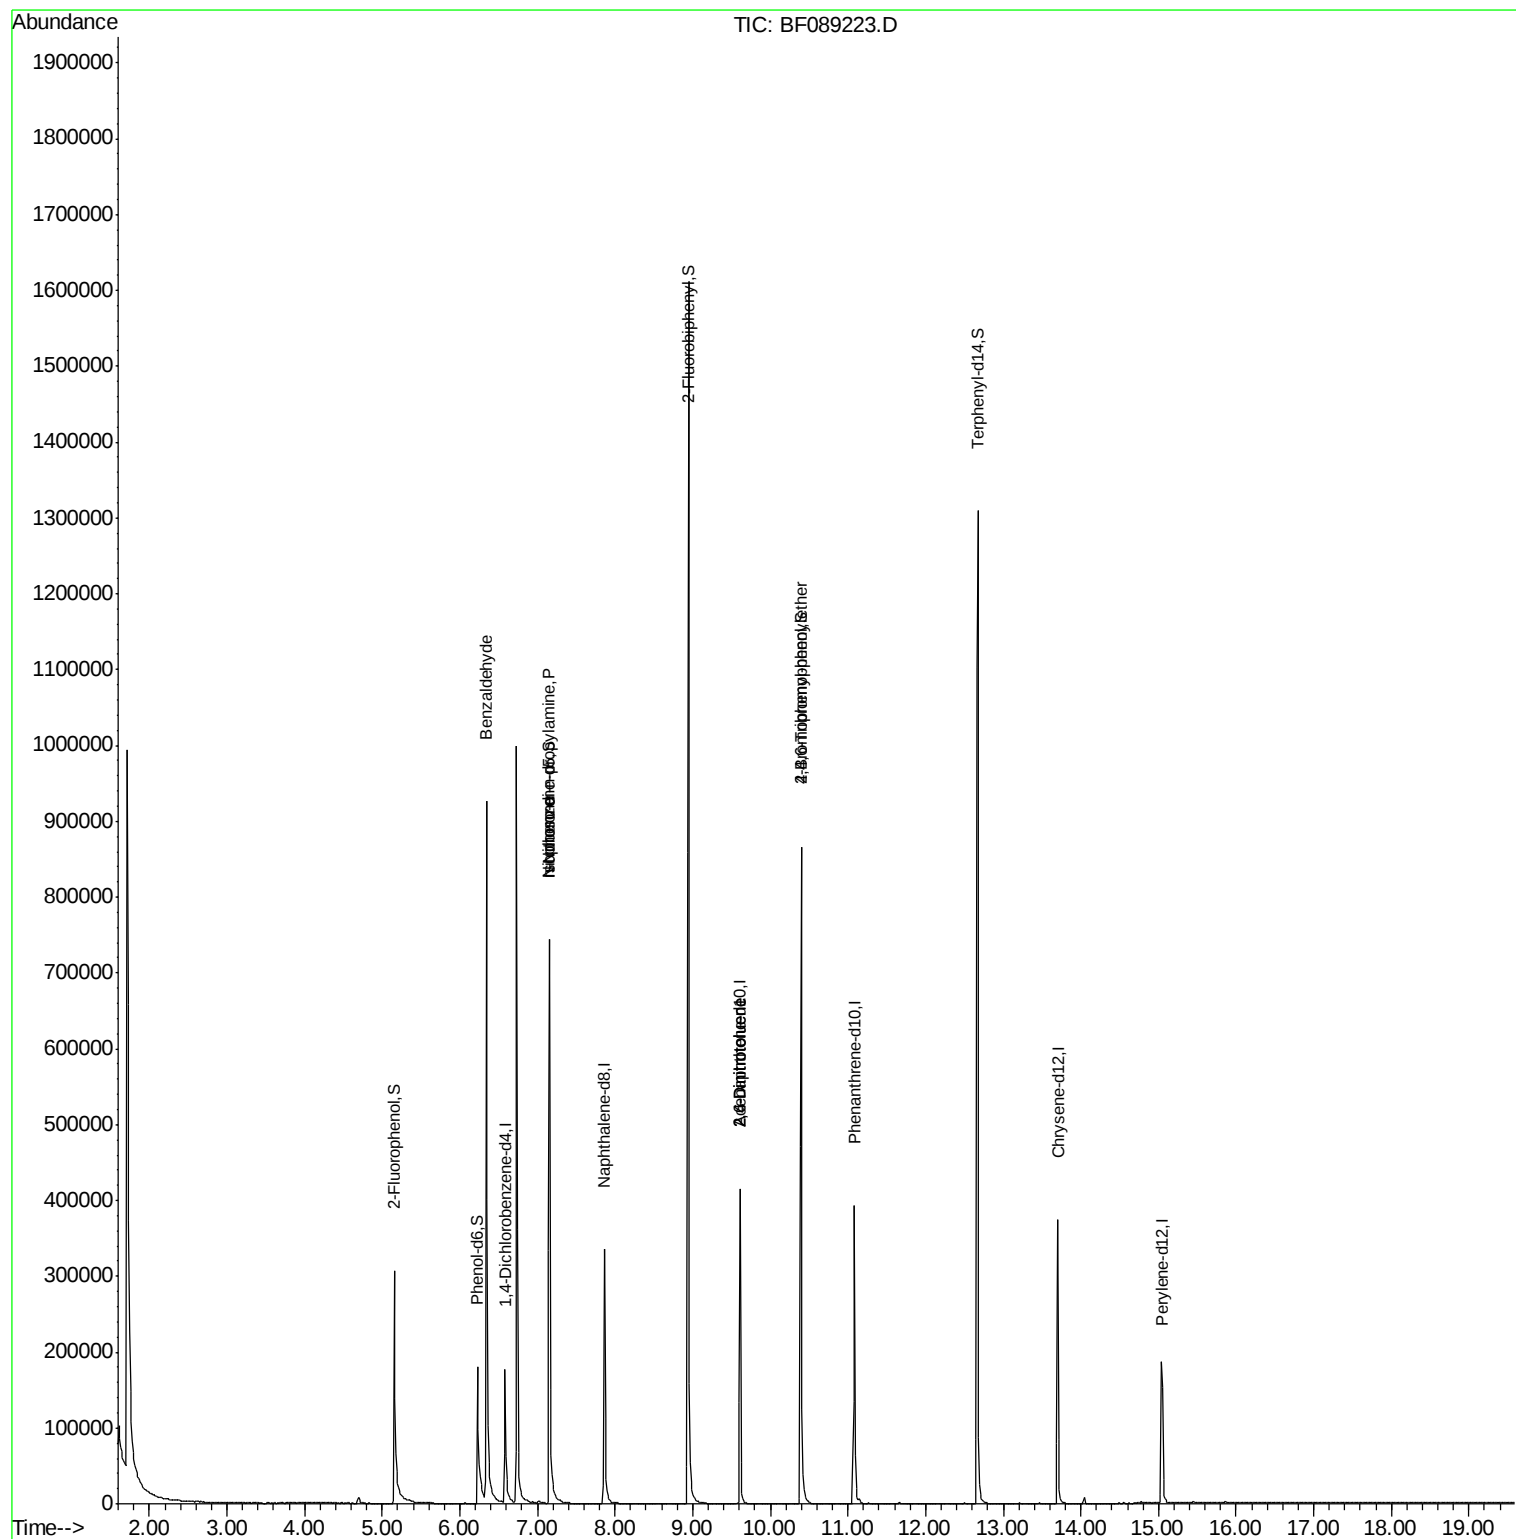

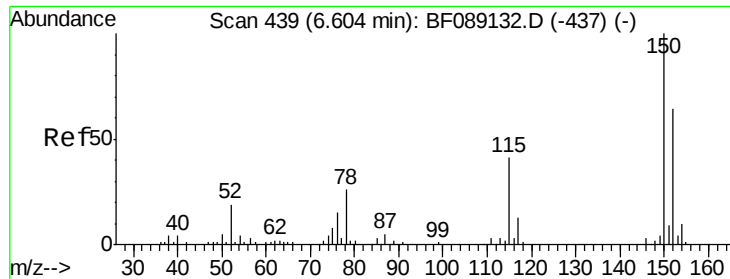

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 437

Delta R.T. -0.02 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK


Tgt Ion:152 Resp: 45045

Ion Ratio Lower Upper

152 100

150 155.1 125.1 187.7




115 62.2 51.1 76.7

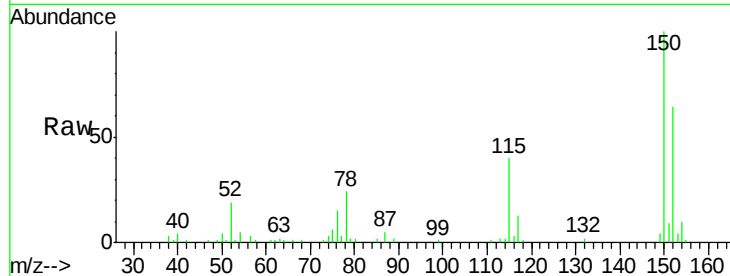

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

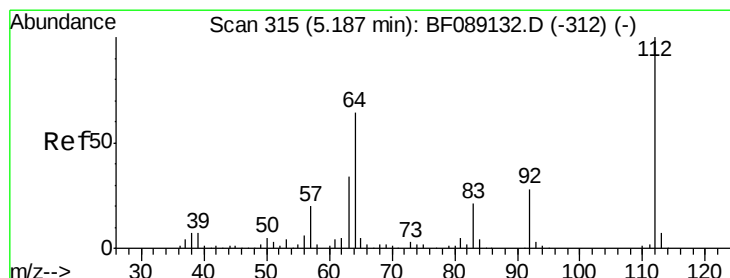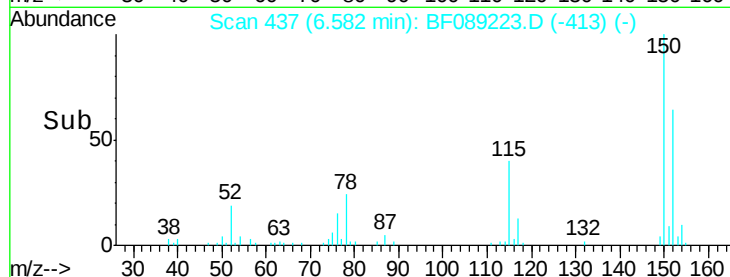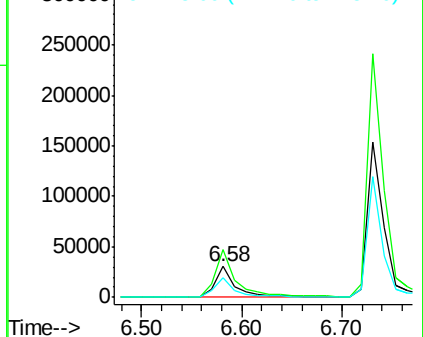

#5

2-Fluorophenol

Concen: 51.41 ng

RT: 5.15 min Scan# 312

Delta R.T. -0.03 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52


Tgt Ion:112 Resp: 152268

Ion Ratio Lower Upper

112 100

64 59.0 51.0 76.4



63 31.5 27.3 40.9

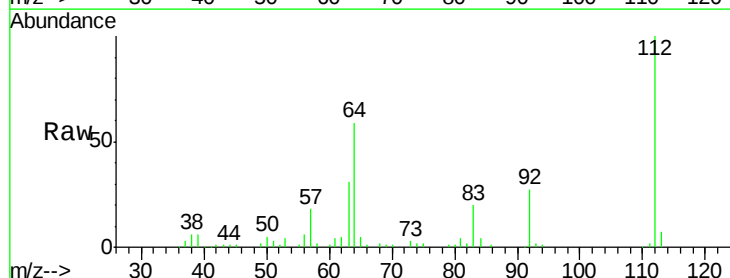


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

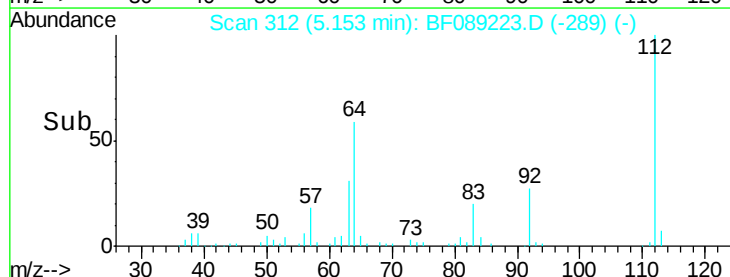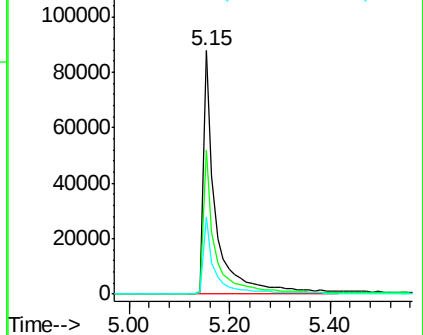



#7

Phenol-d6

Concen: 33.67 ng

RT: 6.23 min Scan# 406

Delta R.T. -0.05 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK





Tgt Ion: 99 Resp: 128595

Ion Ratio Lower Upper

99 100

42 18.3 13.5 20.3

71 38.1 28.9 43.3

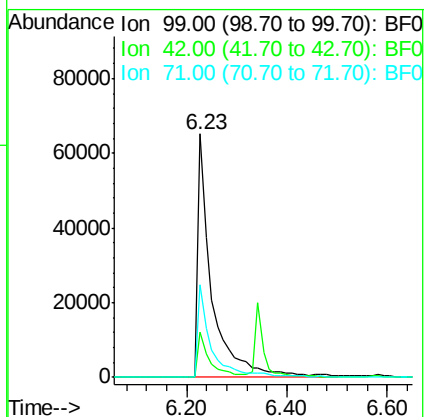

#9

Benzaldehyde

Concen: 2.61 ng

RT: 6.34 min Scan# 416

Delta R.T. 0.19 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52




Tgt Ion: 77 Resp: 7235




Ion Ratio Lower Upper

77 100

105 75.7 86.2 126.2#

106 69.0 76.3 116.3#

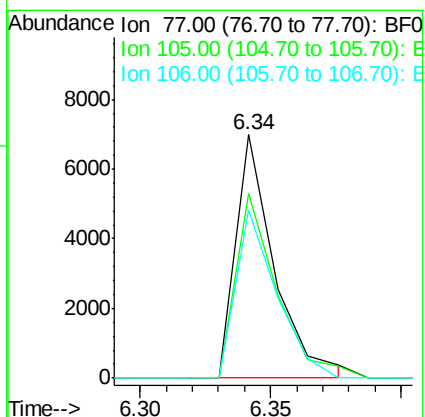

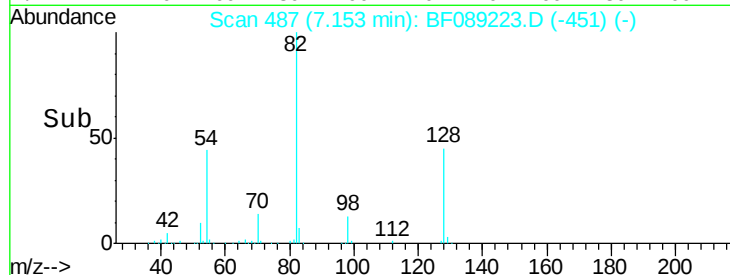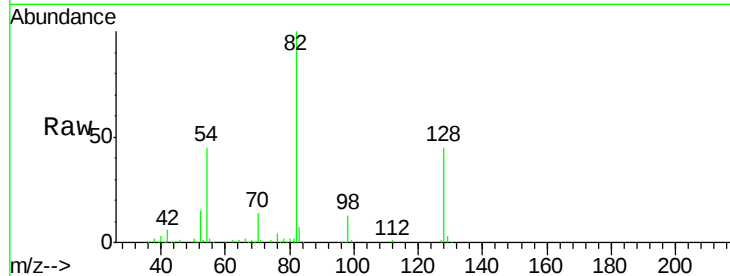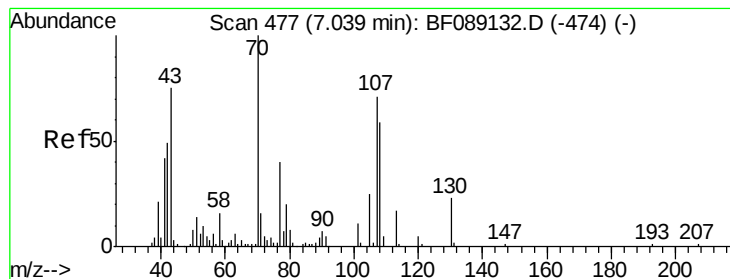

#19

n-Nitroso-di-n-propylamine

Concen: 18.92 ng

RT: 7.15 min Scan# 487

Delta R.T. 0.11 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52

Instrument :

BNA_F

ClientSampled :

FIELDBLANK

Tgt Ion: 70 Resp: 47262





Ion Ratio Lower Upper

70 100

42 41.1 39.2 58.8

101 0.0 8.5 12.7#

130 2.2 18.4 27.6#

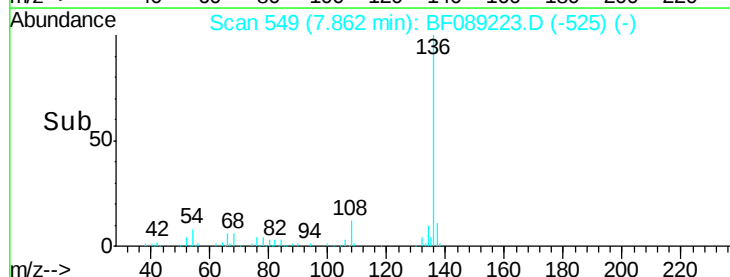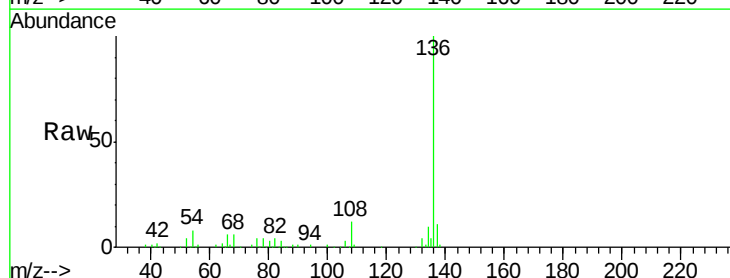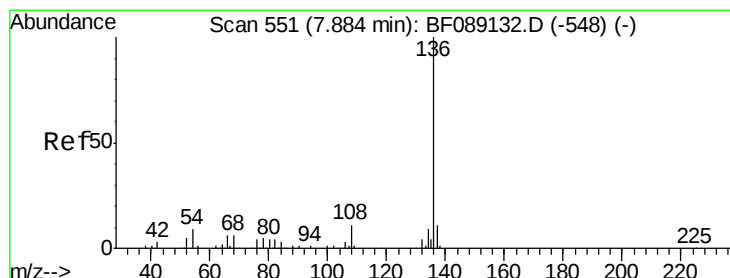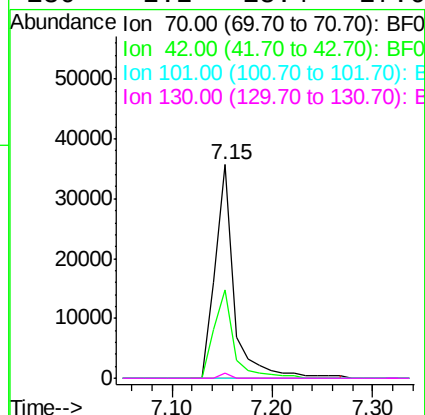

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.02 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52

Tgt Ion: 136 Resp: 198230


Ion Ratio Lower Upper


136 100

137 11.0 8.8 13.2

54 7.7 7.0 10.4

68 5.8 5.0 7.6




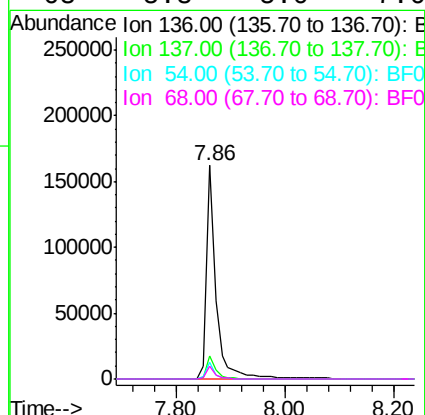


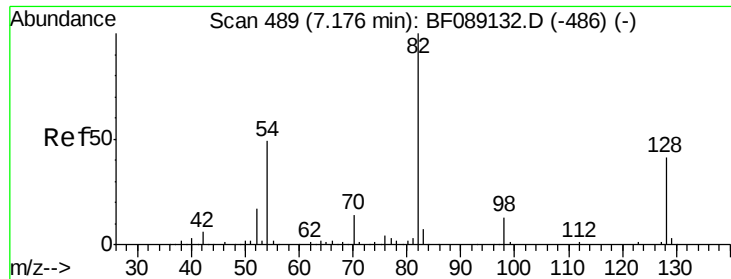

#23
Nitrobenzene-d5
Concen: 96.57 ng
RT: 7.15 min Scan# 487
Delta R.T. -0.02 min
Lab File: BF089223.D
Acq: 23 Jul 2016 7:52




Instrument :
BNA_F
ClientSampleId :
FIELDBLANK


Tgt Ion: 82 Resp: 360276
Ion Ratio Lower Upper
82 100
128 45.3 33.0 49.6
54 45.5 39.0 58.4

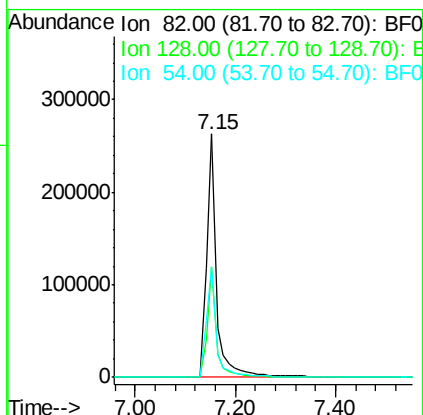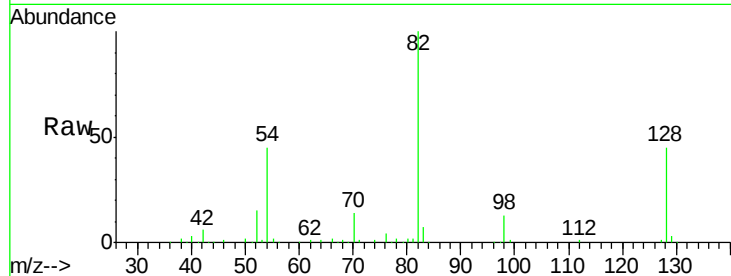

#25
Isophorone
Concen: 39.96 ng
RT: 7.15 min Scan# 487
Delta R.T. -0.29 min
Lab File: BF089223.D
Acq: 23 Jul 2016 7:52

Tgt Ion: 82 Resp: 274766
Ion Ratio Lower Upper
82 100
95 0.0 6.1 9.1#
138 0.0 13.6 20.4#

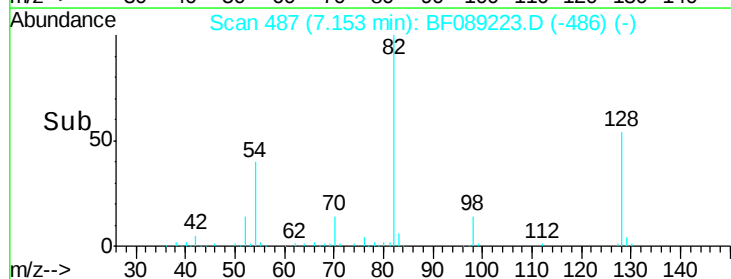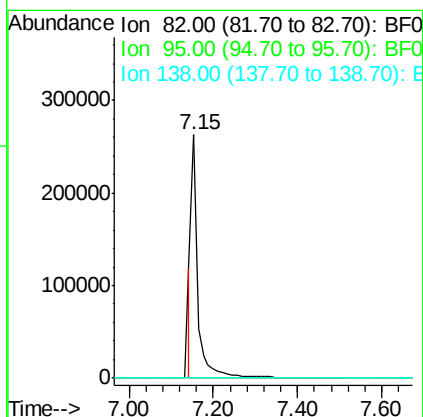



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.02 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK


Tgt Ion:164 Resp: 95188

Ion Ratio Lower Upper

164 100

162 107.6 84.1 126.1




160 48.0 37.1 55.7

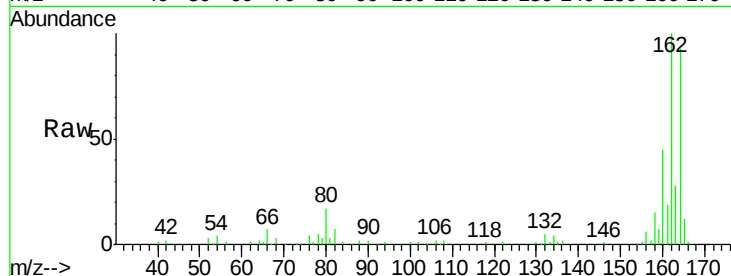

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

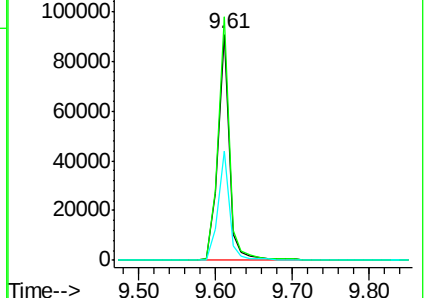

#41

2,4,6-Tribromophenol

Concen: 138.23 ng

RT: 10.40 min Scan# 771

Delta R.T. -0.02 min

Lab File: BF089223.D

Acq: 23 Jul 2016 7:52


Tgt Ion:330 Resp: 118462

Ion Ratio Lower Upper

330 100

332 96.3 77.2 115.8



141 48.1 42.2 63.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



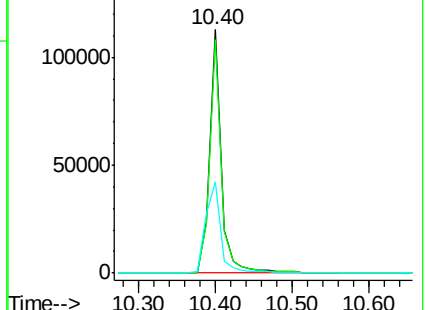



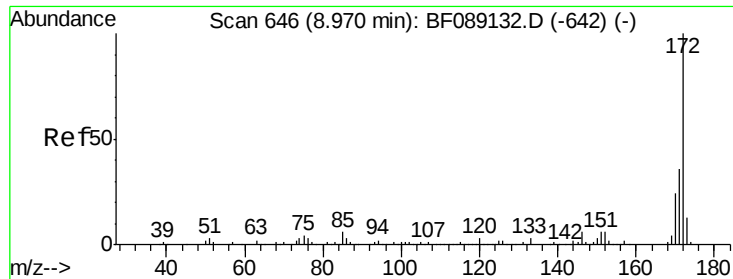

#44
 2-Fluorobiphenyl
 Concen: 97.88 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.02 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52




Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK


Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.2	43.8
170	23.7	19.1	28.7

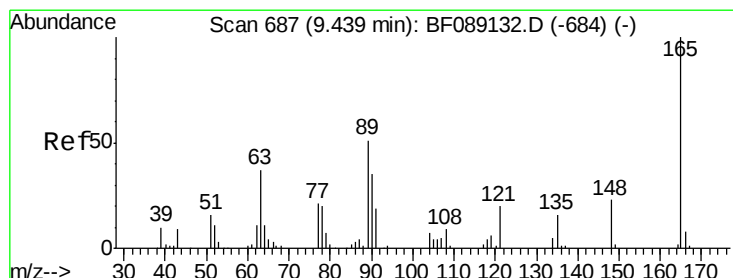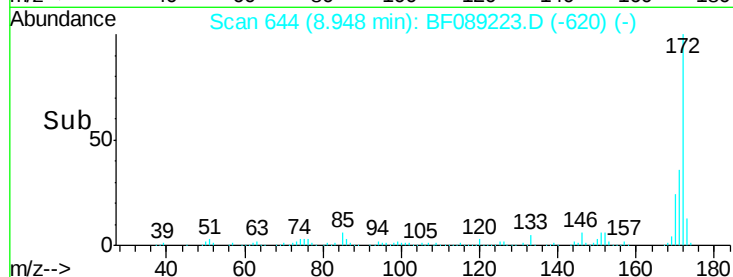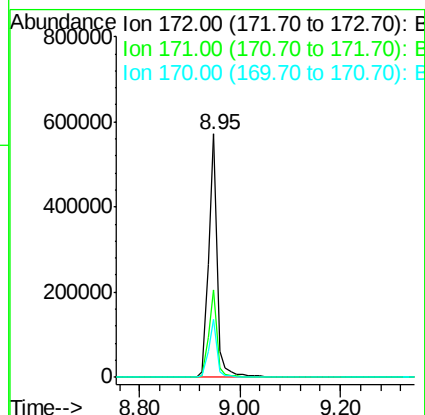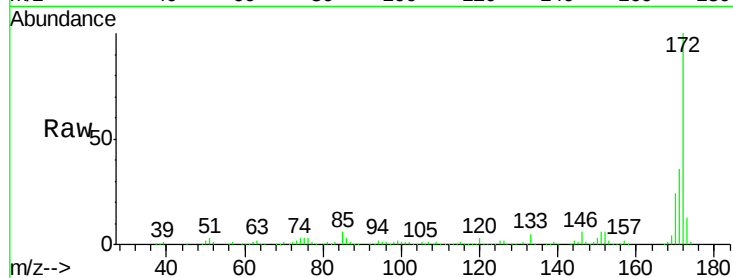

#50
 2,6-Dinitrotoluene
 Concen: 7.02 ng
 RT: 9.61 min Scan# 702
 Delta R.T. 0.17 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	37.0	55.4#
89	0.0	40.9	61.3#

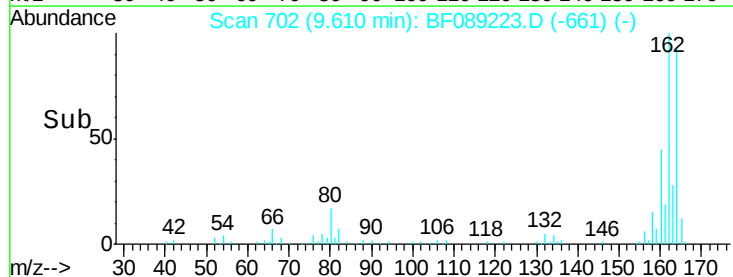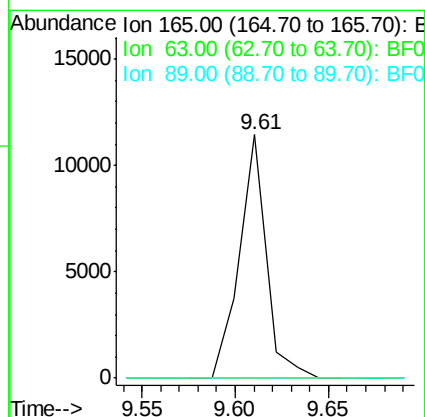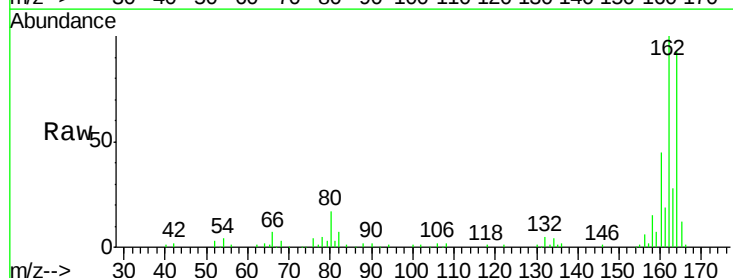


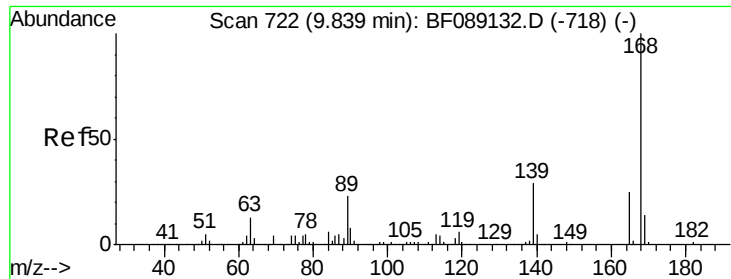




#56
 2,4-Dinitrotoluene
 Concen: 5.45 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.23 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Tgt Ion:165 Resp: 11571
 Ion Ratio Lower Upper
 165 100
 63 0.0 55.4 83.2#
 89 0.0 74.3 111.5#
 182 0.0 2.0 3.0#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

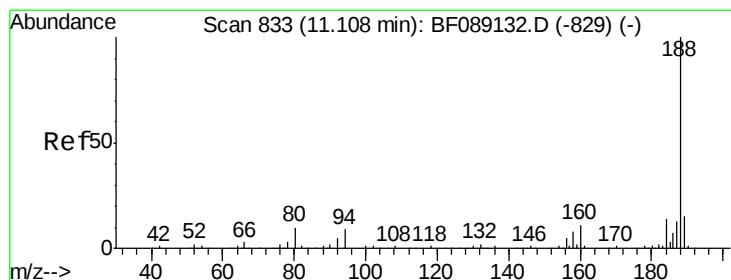
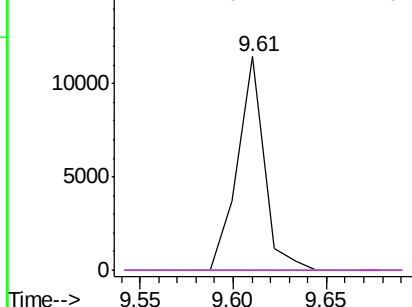



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.08 min Scan# 831
 Delta R.T. -0.02 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Tgt Ion:188 Resp: 185377
 Ion Ratio Lower Upper
 188 100
 94 7.6 7.0 10.4
 80 8.8 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

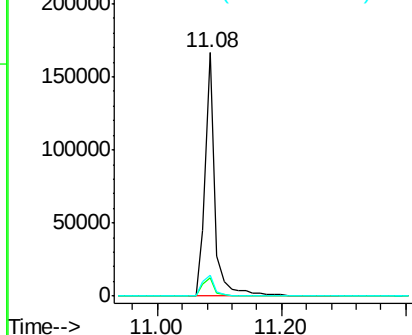


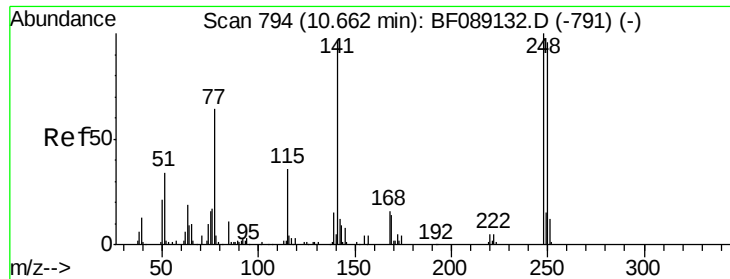




#66
 4-Bromophenyl-phenylether
 Concen: 5.11 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.26 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Tgt Ion:248 Resp: 9379
 Ion Ratio Lower Upper
 248 100
 250 191.4 76.9 115.3#
 141 469.9 77.4 116.2#

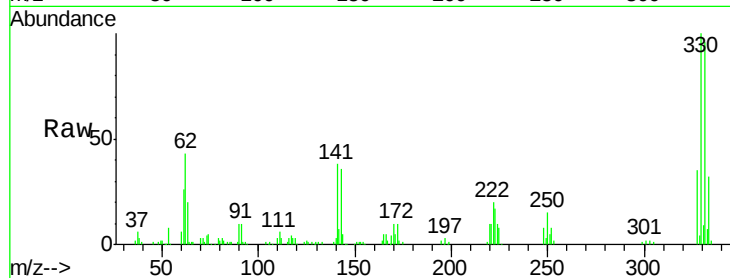


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

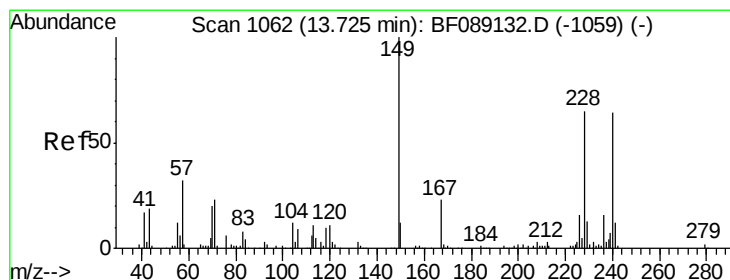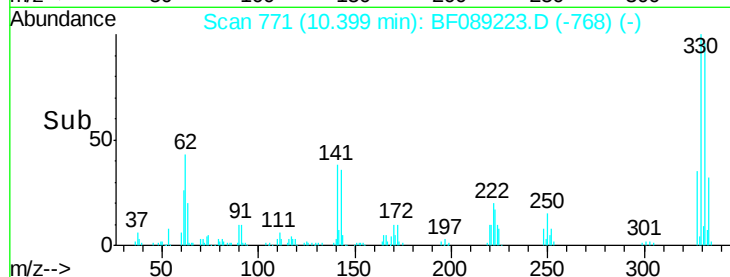
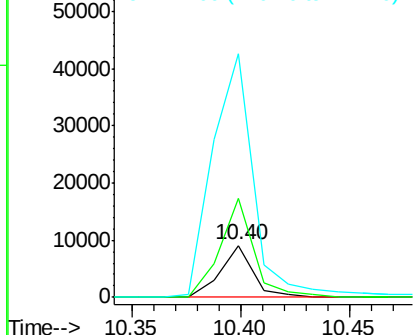



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.70 min Scan# 1060
 Delta R.T. -0.02 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Tgt Ion:240 Resp: 143289
 Ion Ratio Lower Upper
 240 100
 120 11.2 13.6 20.4#
 236 25.0 20.5 30.7

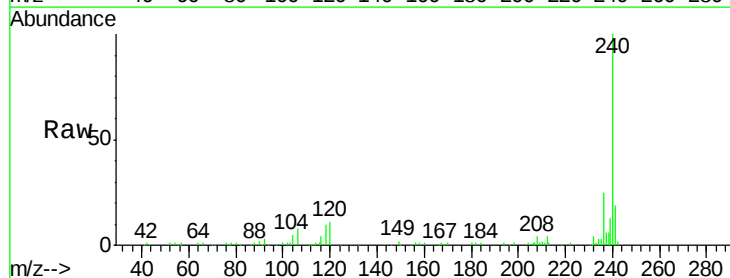

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



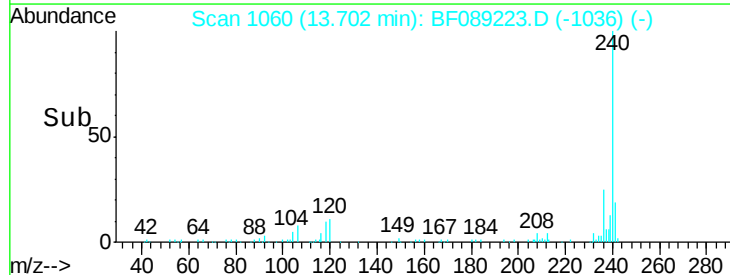
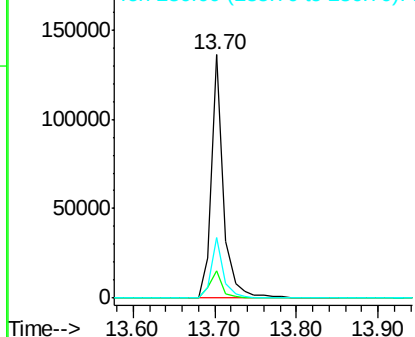




#78
 Terphenyl-d14
 Concen: 90.39 ng
 RT: 12.67 min Scan# 970
 Delta R.T. -0.01 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	7.0	10.4
122	8.4	13.8	20.8#

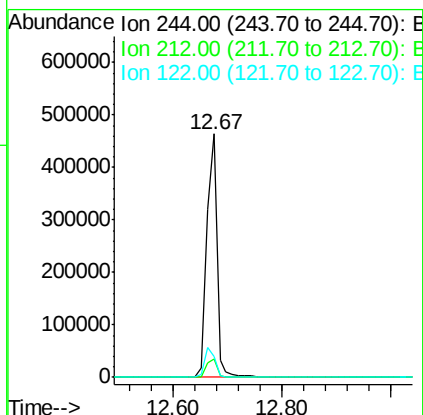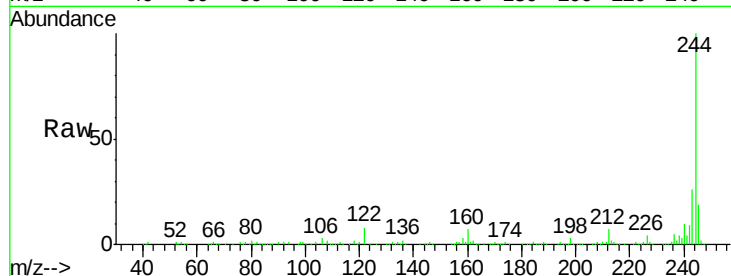

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.05 min Scan# 1178
 Delta R.T. -0.02 min
 Lab File: BF089223.D
 Acq: 23 Jul 2016 7:52

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.0	18.5	27.7
265	21.5	17.3	25.9

