

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089232.D
 Acq On : 23 Jul 2016 12:28
 Operator : UM/SJ
 Sample : H4120-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUP-01

Quant Time: Jul 25 01:07:17 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 19:03:15 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	45460	20.00	ng	-0.02
21) Naphthalene-d8	7.86	136	191716	20.00	ng	-0.02
38) Acenaphthene-d10	9.61	164	97504	20.00	ng	-0.02
63) Phenanthrene-d10	11.08	188	182100	20.00	ng	-0.02
75) Chrysene-d12	13.70	240	133086	20.00	ng	-0.02
86) Perylene-d12	15.04	264	93722	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	199983	66.90	ng	-0.03
7) Phenol-d6	6.23	99	181178	47.00	ng	-0.05
23) Nitrobenzene-d5	7.15	82	361809	100.27	ng	-0.02
41) 2,4,6-Tribromophenol	10.40	330	103518	117.92	ng	-0.02
44) 2-Fluorobiphenyl	8.95	172	615570	86.99	ng	-0.02
78) Terphenyl-d14	12.67	244	518976	84.58	ng	-0.01
Target Compounds						Qvalue
15) Benzyl Alcohol	6.73	79	6337	2.24	ng	# 51
18) Hexachloroethane	7.15	117	4006	2.89	ng	# 16
25) Isophorone	7.50	82	17875	2.69	ng	# 33
35) Caprolactam	8.31	113	11140	13.31	ng	# 1
49) Dimethylphthalate	9.35	163	24306	3.25	ng	# 93
53) 2,4-Dinitrophenol	9.83	184	256	8.80	ng	# 1
66) 4-Bromophenyl-phenylether	10.40	248	8190	4.54	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089232.D
Acq On : 23 Jul 2016 12:28
Operator : UM/SJ
Sample : H4120-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP-01

Quant Time: Jul 25 01:07:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration




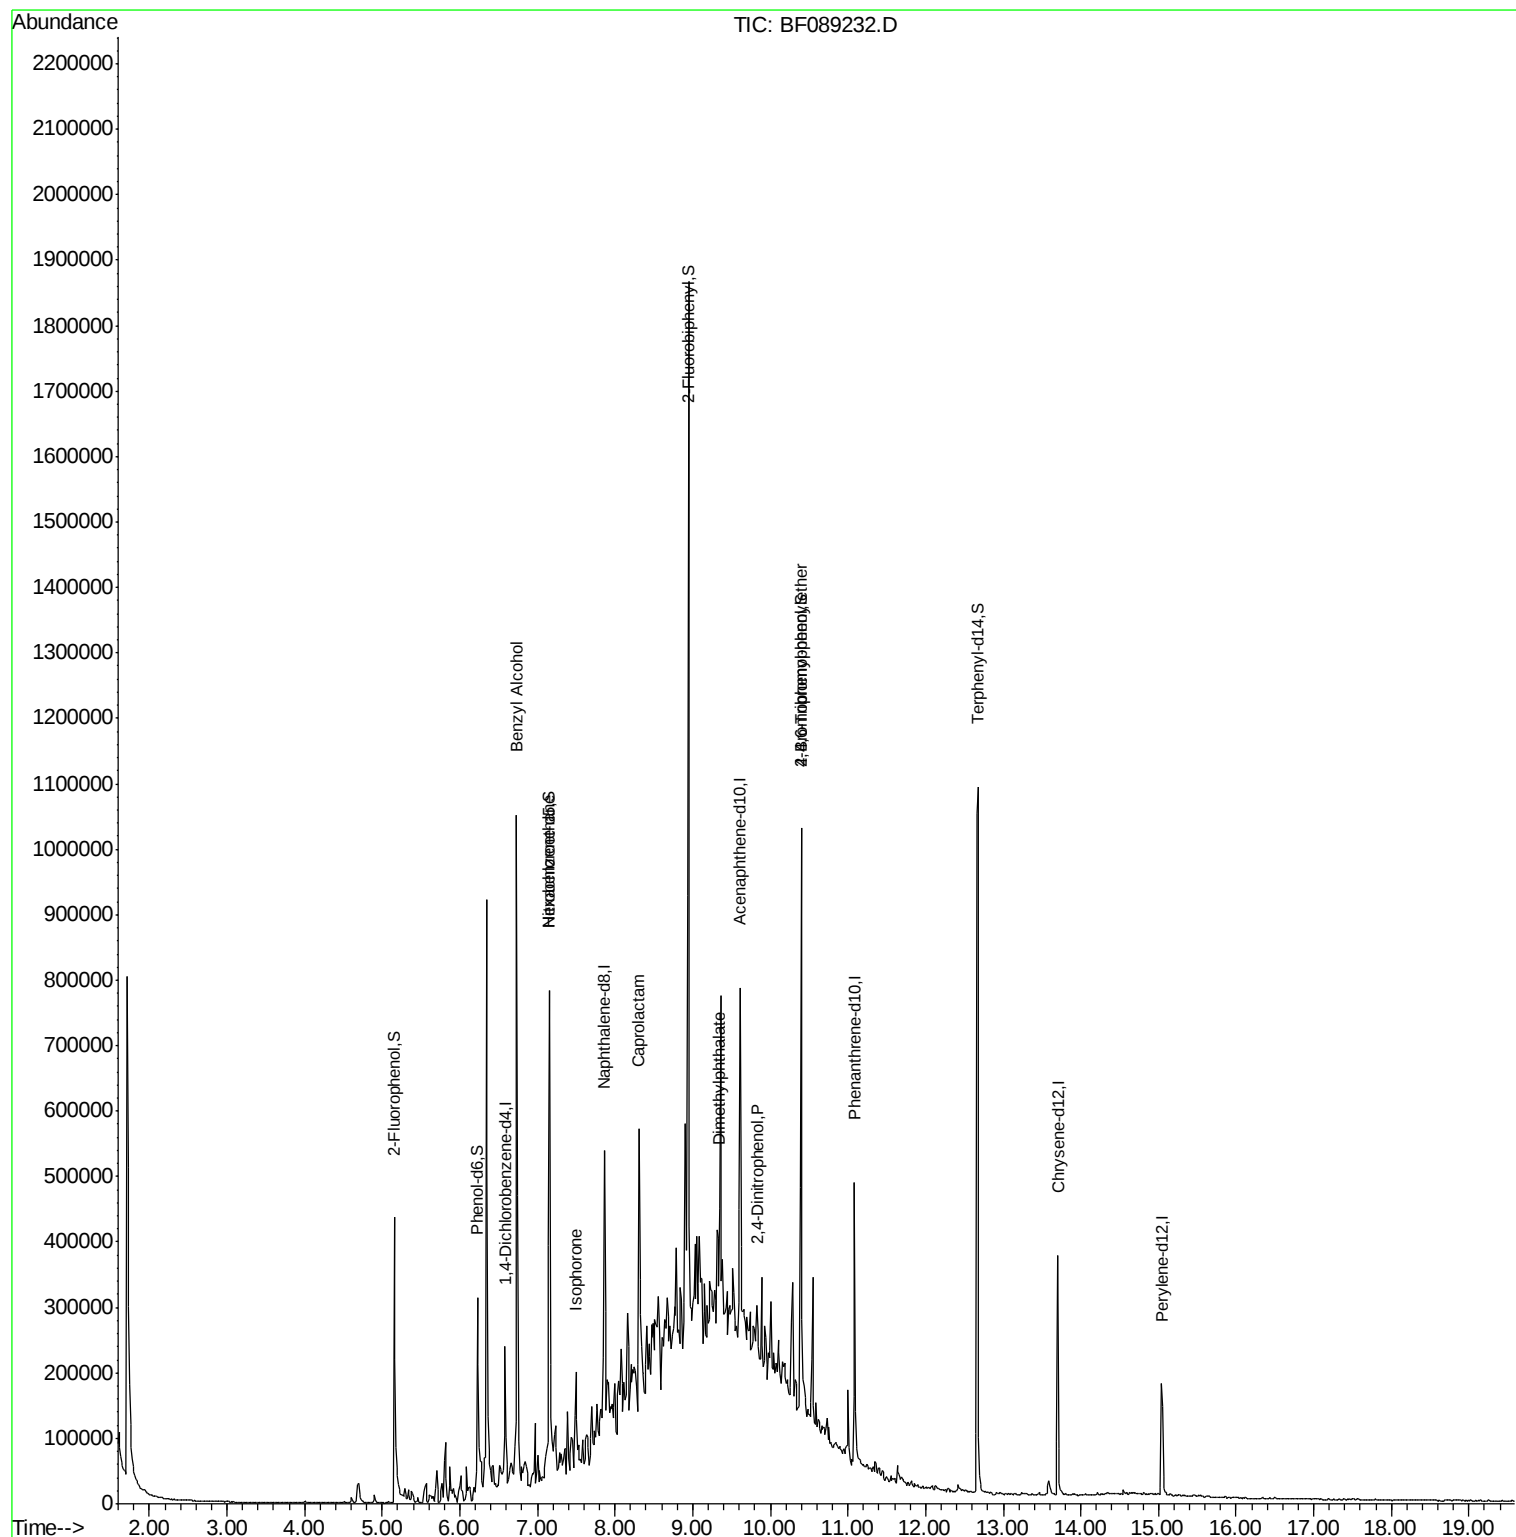


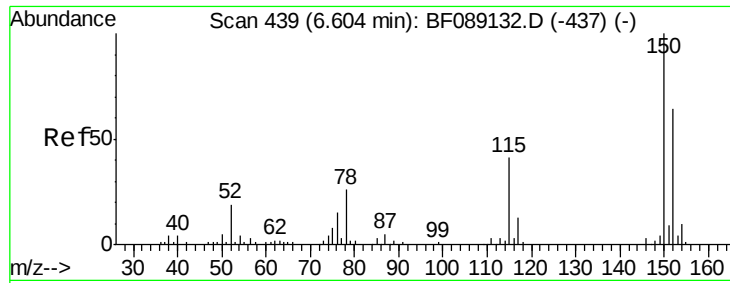

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.58 min Scan# 437
 Delta R.T. -0.02 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28




Instrument :
 BNA_F
 ClientSampleId :
 DUP-01


Tgt Ion:152 Resp: 45460
 Ion Ratio Lower Upper
 152 100
 150 159.7 125.1 187.7
 115 63.8 51.1 76.7

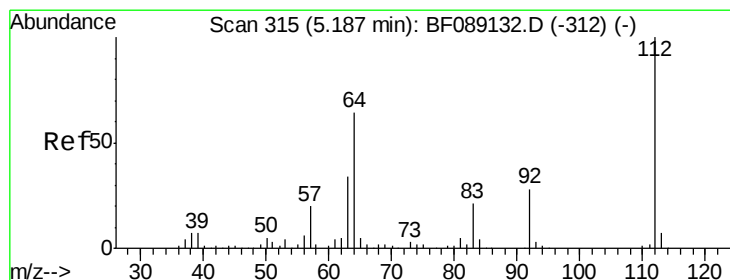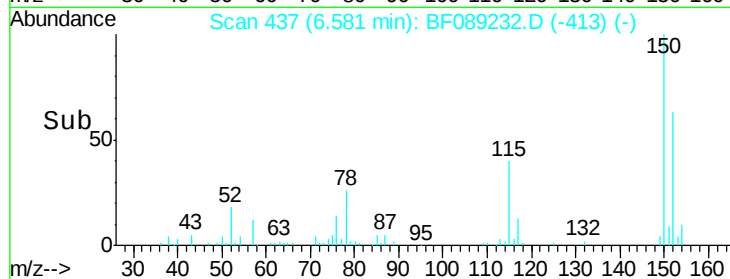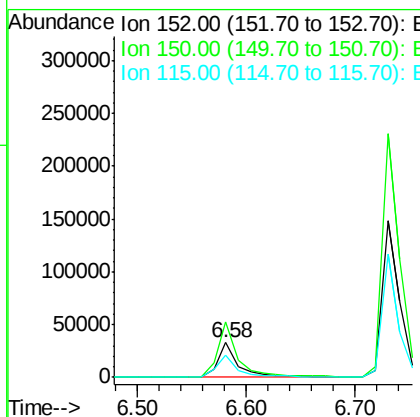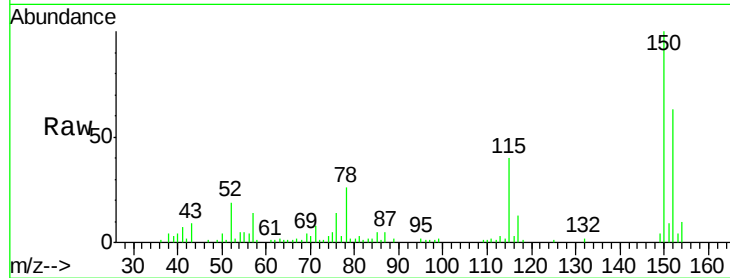

#5
 2-Fluorophenol
 Concen: 66.90 ng
 RT: 5.15 min Scan# 312
 Delta R.T. -0.03 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Tgt Ion:112 Resp: 199983
 Ion Ratio Lower Upper
 112 100
 64 62.3 51.0 76.4
 63 33.7 27.3 40.9

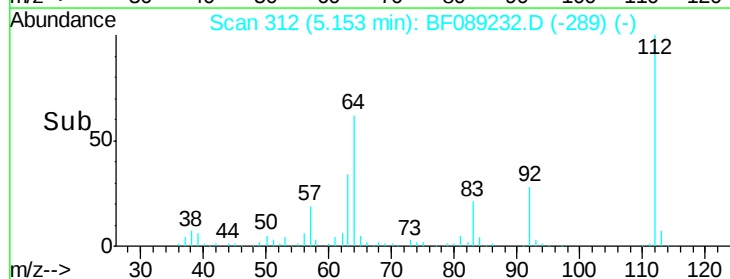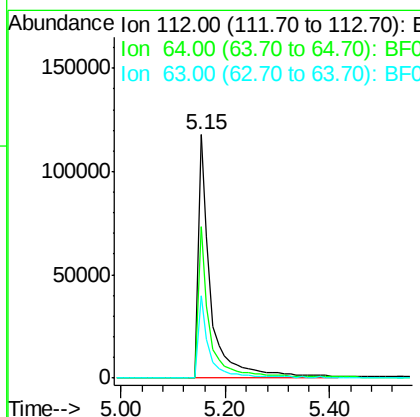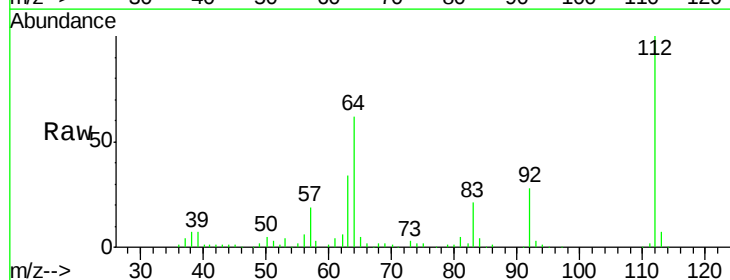

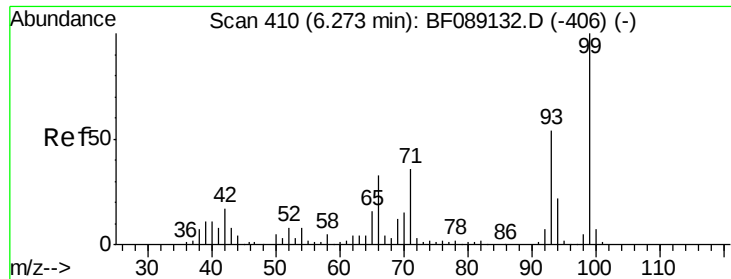

#7

Phenol-d6

Concen: 47.00 ng

RT: 6.23 min Scan# 406

Delta R.T. -0.05 min

Lab File: BF089232.D

Acq: 23 Jul 2016 12:28

Instrument :

BNA_F

ClientSampled :

DUP-01


Tgt Ion: 99 Resp: 181178

Ion Ratio Lower Upper

99 100

42 19.9 13.5 20.3




71 40.1 28.9 43.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

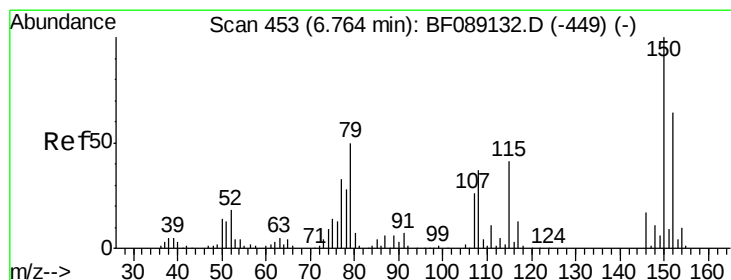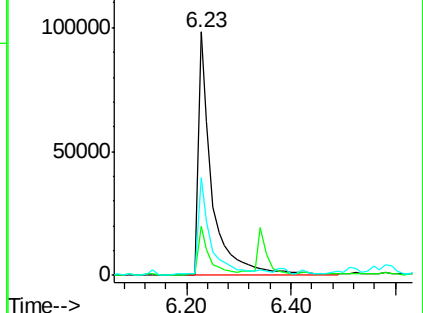

#15

Benzyl Alcohol

Concen: 2.24 ng

RT: 6.73 min Scan# 450

Delta R.T. -0.03 min

Lab File: BF089232.D

Acq: 23 Jul 2016 12:28


Tgt Ion: 79 Resp: 6337

Ion Ratio Lower Upper

79 100

108 24.9 58.2 87.4#



77 96.7 52.2 78.4#

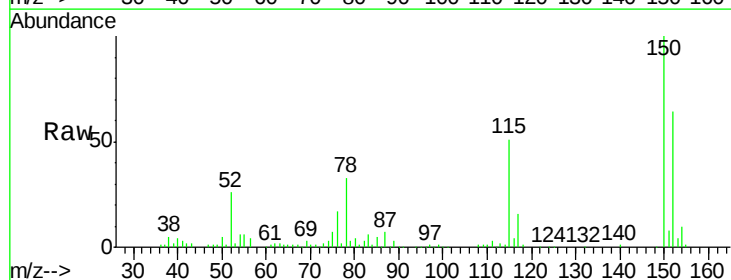


Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0



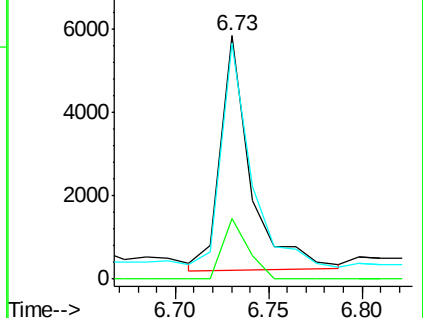
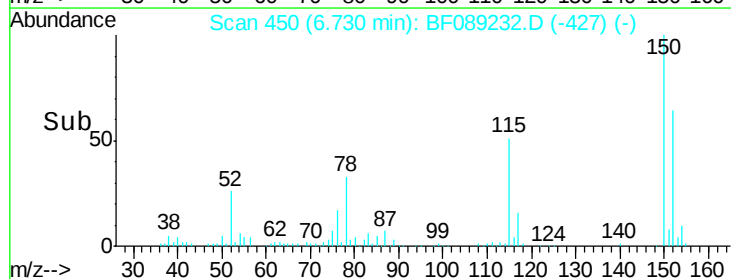




#18
Hexachloroethane
Concen: 2.89 ng
RT: 7.15 min Scan# 487
Delta R.T. 0.05 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28




Instrument :
BNA_F
ClientSampleId :
DUP-01


Tgt Ion:117 Resp: 4006
Ion Ratio Lower Upper
117 100
119 10.6 74.5 111.7#
201 0.0 51.8 77.6#

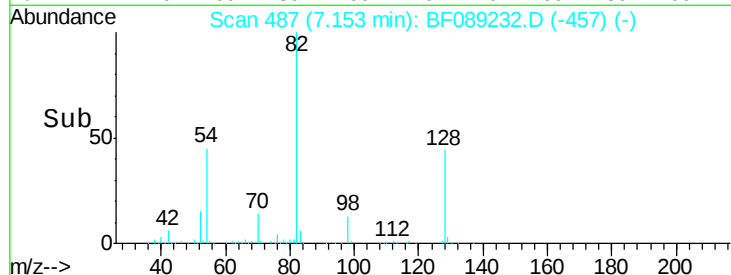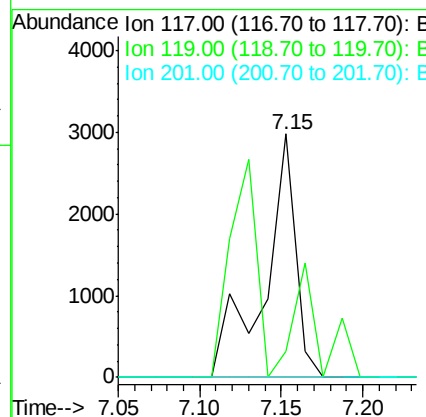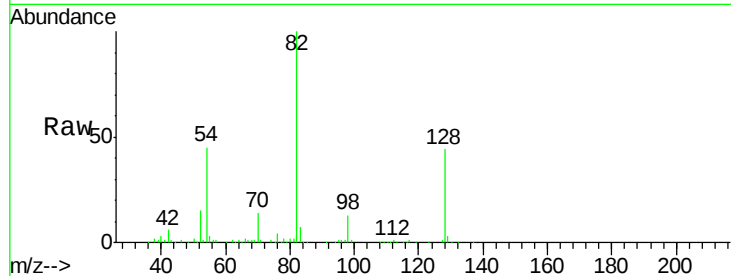

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.86 min Scan# 549
Delta R.T. -0.02 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28

Tgt Ion:136 Resp: 191716
Ion Ratio Lower Upper
136 100
137 11.3 8.8 13.2
54 9.1 7.0 10.4
68 7.8 5.0 7.6#

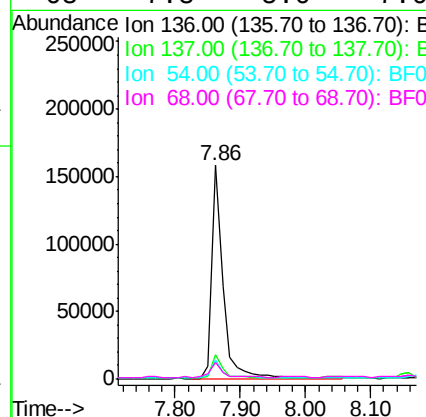


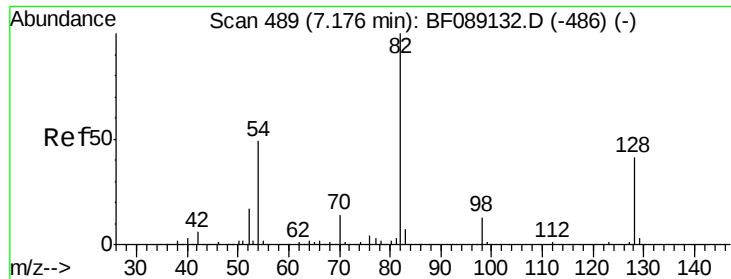




#23
 Nitrobenzene-d5
 Concen: 100.27 ng
 RT: 7.15 min Scan# 487
 Delta R.T. -0.02 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Instrument :
 BNA_F
 ClientSampleId :
 DUP-01

Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.0	33.0	49.6
54	45.1	39.0	58.4

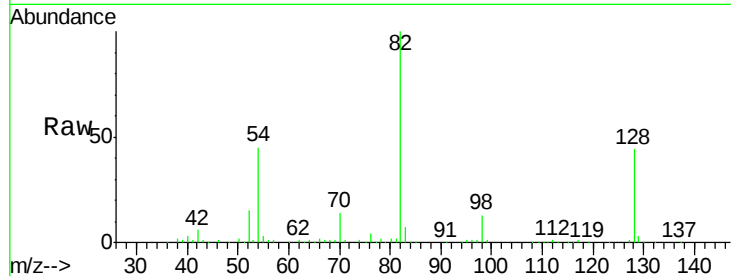


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

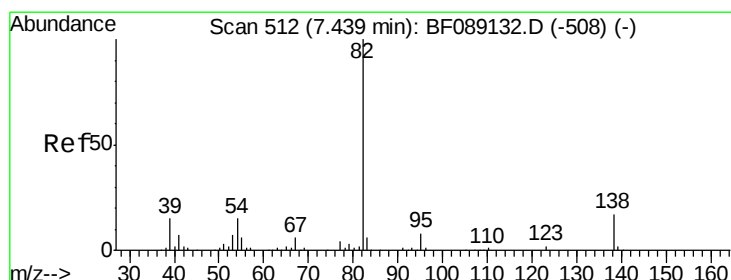
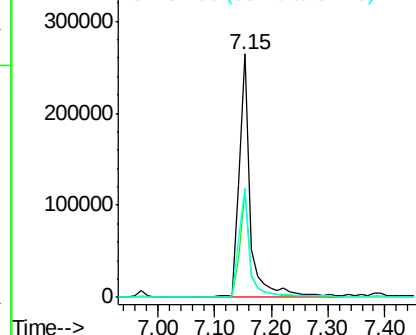



#25
 Isophorone
 Concen: 2.69 ng
 RT: 7.50 min Scan# 517
 Delta R.T. 0.06 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Tgt Ion	Ratio	Lower	Upper
82	100		
95	57.2	6.1	9.1#
138	2.5	13.6	20.4#

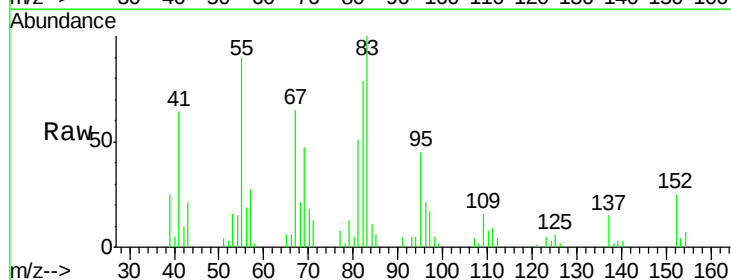

Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0




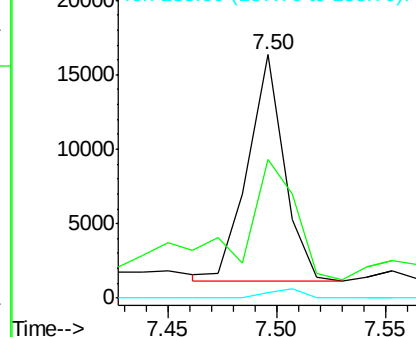




#35
 Caprolactam
 Concen: 13.31 ng
 RT: 8.31 min Scan# 588
 Delta R.T. -0.05 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28




Instrument :
 BNA_F
 ClientSampleId :
 DUP-01


Tgt Ion:113 Resp: 11140
 Ion Ratio Lower Upper
 113 100
 55 327.5 145.3 185.3#
 56 237.1 104.3 144.3#

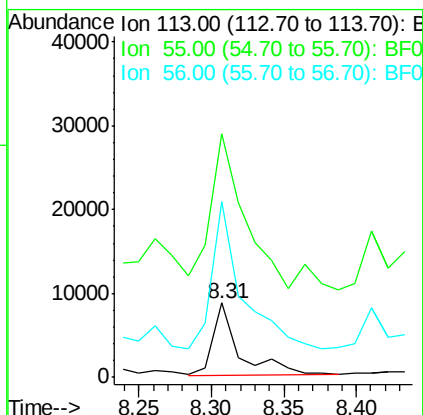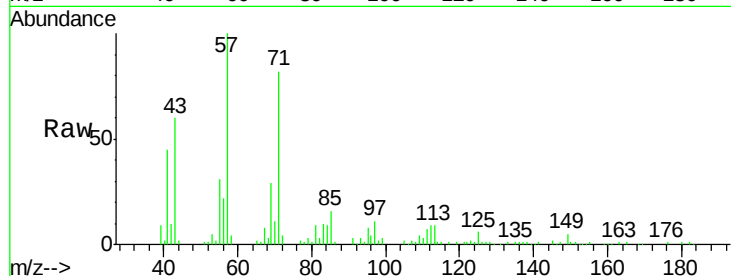

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.02 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Tgt Ion:164 Resp: 97504
 Ion Ratio Lower Upper
 164 100
 162 106.0 84.1 126.1
 160 46.9 37.1 55.7

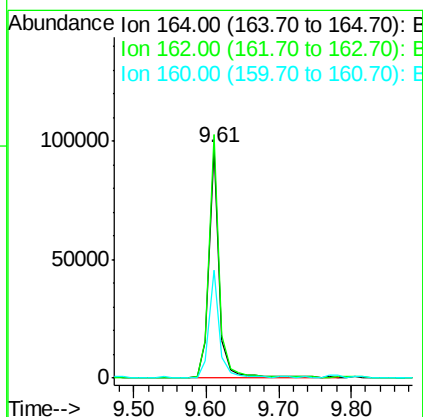


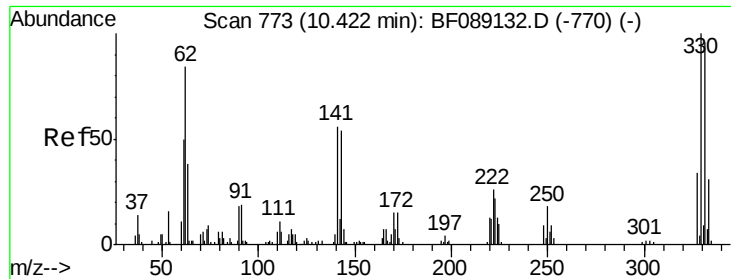




#41
 2,4,6-Tribromophenol
 Concen: 117.92 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.02 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Instrument :
 BNA_F
 ClientSampleId :
 DUP-01

Tgt Ion:330 Resp: 103518
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.2 115.8
 141 50.7 42.2 63.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

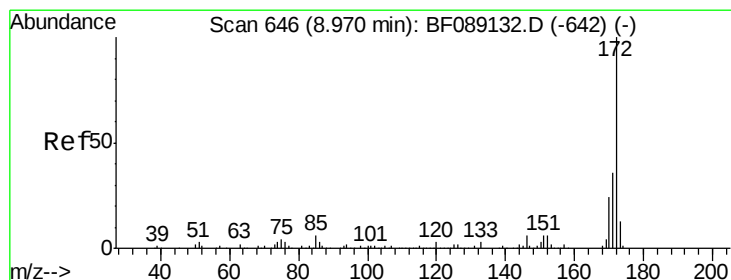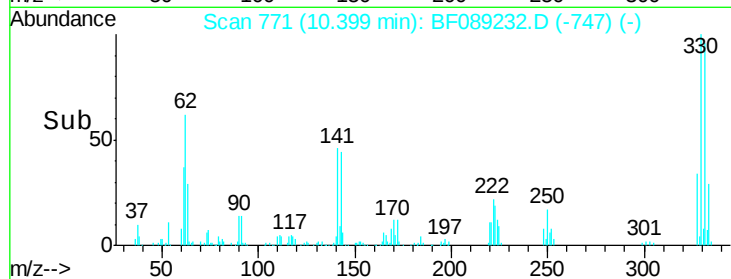
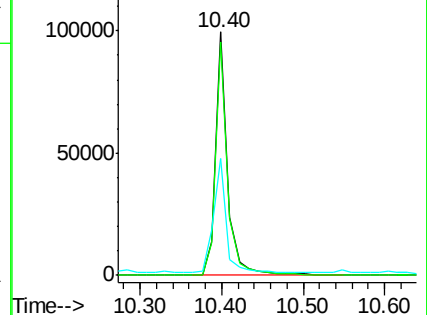



#44
 2-Fluorobiphenyl
 Concen: 86.99 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.02 min
 Lab File: BF089232.D
 Acq: 23 Jul 2016 12:28

Tgt Ion:172 Resp: 615570
 Ion Ratio Lower Upper
 172 100
 171 36.5 29.2 43.8
 170 23.8 19.1 28.7

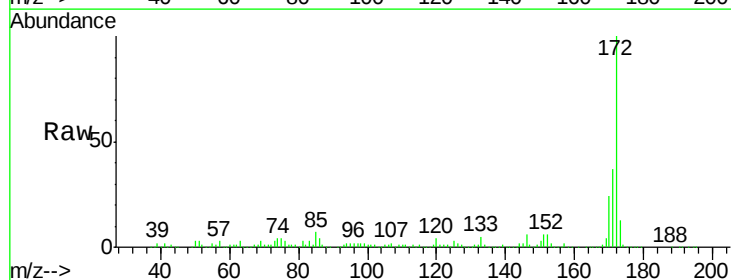

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

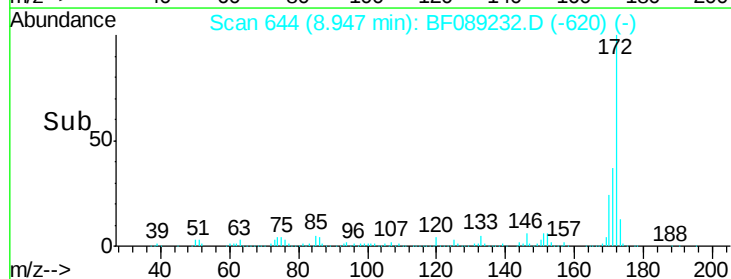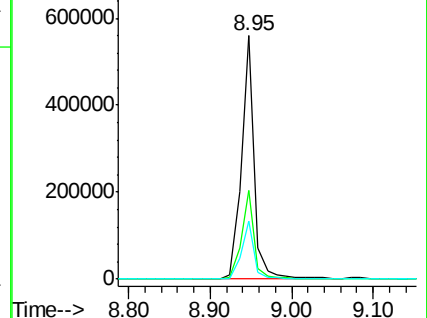


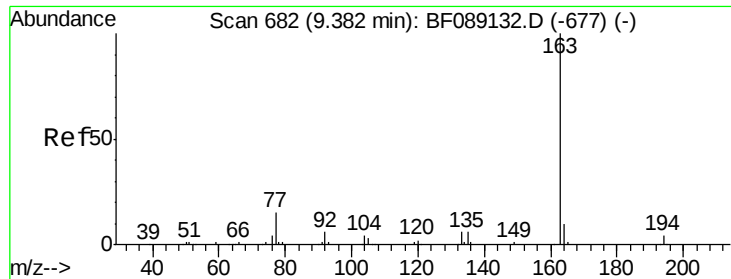




#49
Dimethylphthalate
Concen: 3.25 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.03 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28

Instrument :
BNA_F
ClientSampled :
DUP-01

Tgt Ion:163 Resp: 24306
Ion Ratio Lower Upper
163 100
194 6.0 2.9 4.3#
164 11.9 7.6 11.4#




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E


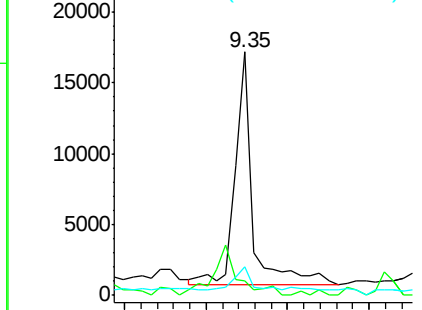



#53
2,4-Dinitrophenol
Concen: 8.80 ng
RT: 9.83 min Scan# 721
Delta R.T. 0.11 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28

Tgt Ion:184 Resp: 256
Ion Ratio Lower Upper
184 100
63 114.7 60.3 90.5#
154 290.9 60.7 91.1#



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 154.00 (153.70 to 154.70): E




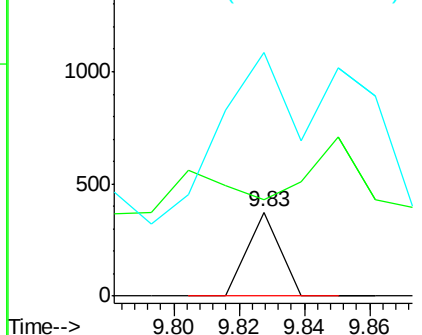


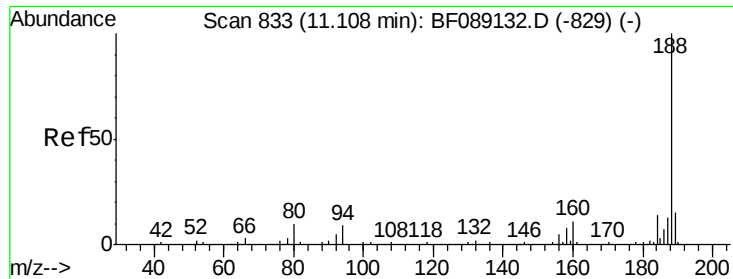

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.08 min Scan# 831
Delta R.T. -0.02 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28




Instrument :
BNA_F
ClientSampleId :
DUP-01


Tgt Ion:188 Resp: 182100
Ion Ratio Lower Upper
188 100
94 8.2 7.0 10.4
80 9.1 7.7 11.5

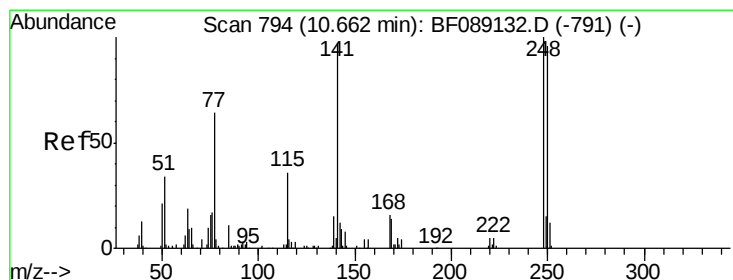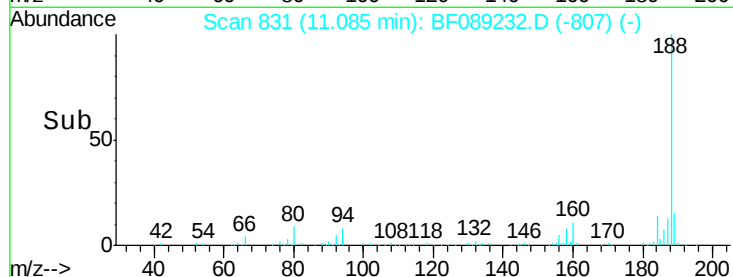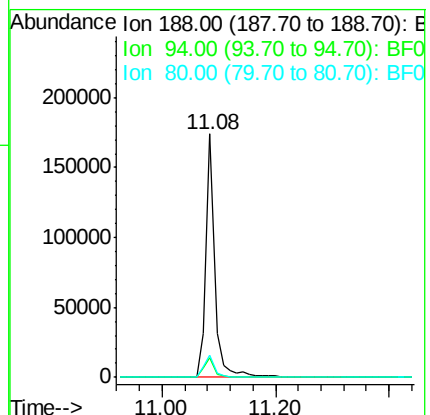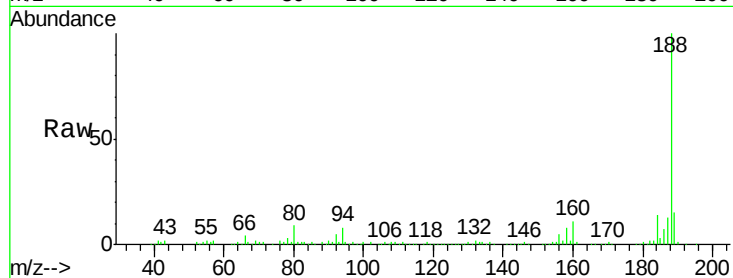

#66
4-Bromophenyl-phenylether
Concen: 4.54 ng
RT: 10.40 min Scan# 771
Delta R.T. -0.26 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28

Tgt Ion:248 Resp: 8190
Ion Ratio Lower Upper
248 100
250 200.4 76.9 115.3#
141 575.6 77.4 116.2#

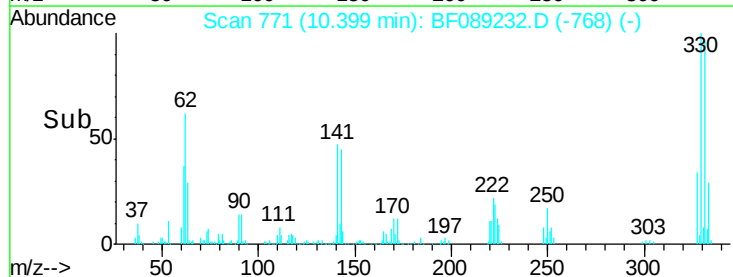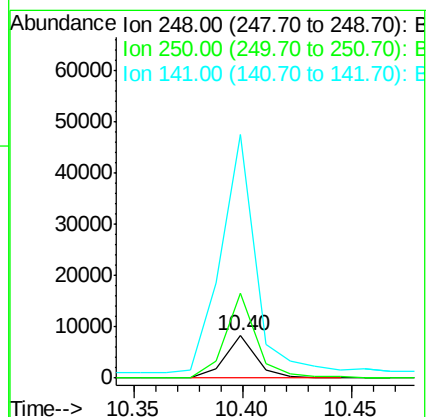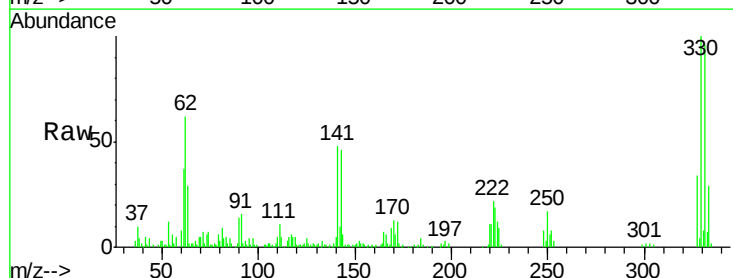

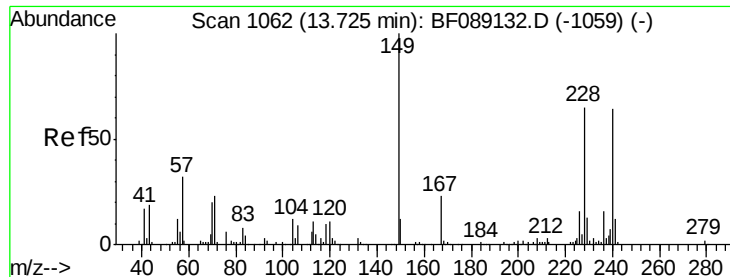

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.70 min Scan# 1060

Delta R.T. -0.02 min

Lab File: BF089232.D

Acq: 23 Jul 2016 12:28

Instrument :

BNA_F

ClientSampleId :

DUP-01


Tgt Ion:240 Resp: 133086

Ion Ratio Lower Upper

240 100

120 10.8 13.6 20.4#




236 25.8 20.5 30.7

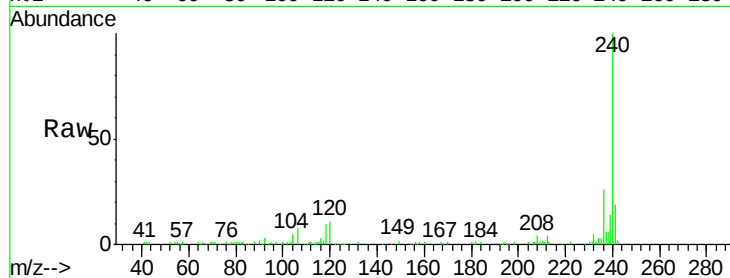

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

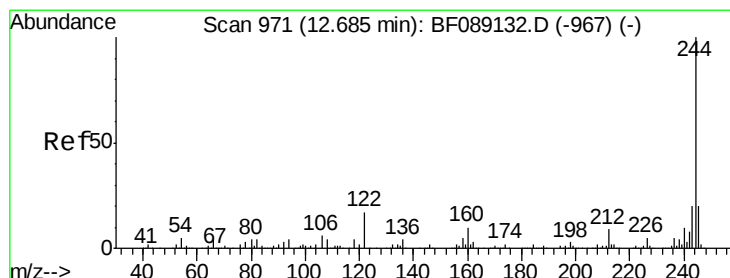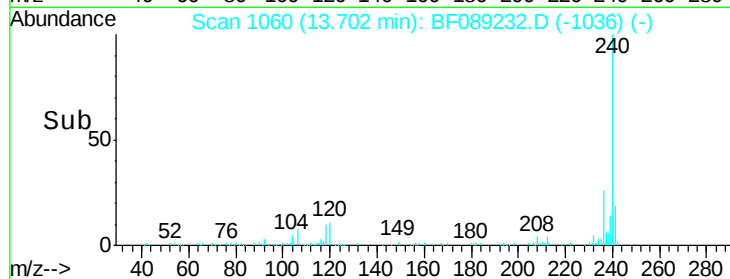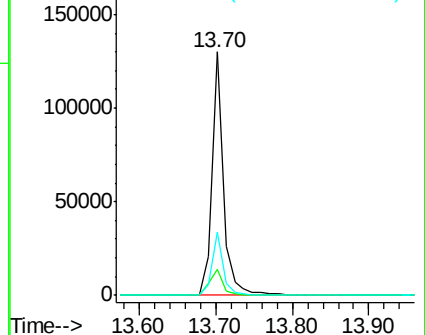

#78

Terphenyl-d14

Concen: 84.58 ng

RT: 12.67 min Scan# 970

Delta R.T. -0.01 min

Lab File: BF089232.D

Acq: 23 Jul 2016 12:28


Tgt Ion:244 Resp: 518976

Ion Ratio Lower Upper

244 100

212 7.3 7.0 10.4



122 7.6 13.8 20.8#

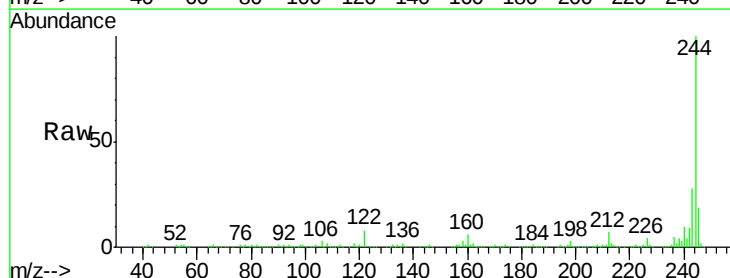


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

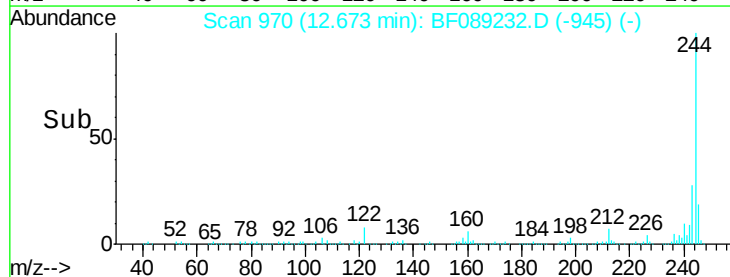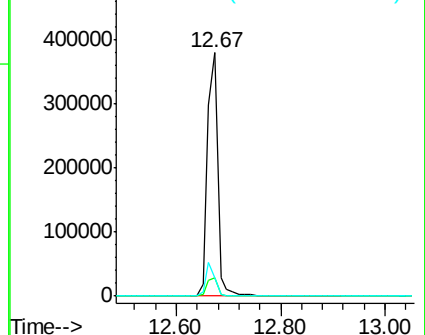


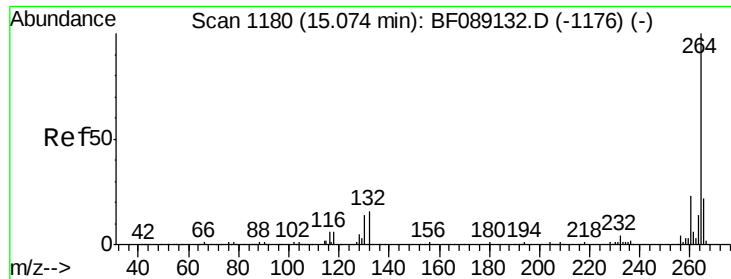

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.04 min Scan# 1177
Delta R.T. -0.03 min
Lab File: BF089232.D
Acq: 23 Jul 2016 12:28

Instrument :
BNA_F
ClientSampleId :
DUP-01

Tgt Ion: 264 Resp: 93722
Ion Ratio Lower Upper
264 100
260 23.7 18.5 27.7
265 21.8 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

