

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089250.D
 Acq On : 23 Jul 2016 23:59
 Operator : UM/SJ
 Sample : H4129-12
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Quant Time: Jul 25 01:13:12 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 19:03:15 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	45362	20.00	ng	-0.02
21) Naphthalene-d8	7.86	136	200886	20.00	ng	-0.02
38) Acenaphthene-d10	9.61	164	89629	20.00	ng	-0.02
63) Phenanthrene-d10	11.08	188	151110	20.00	ng	-0.02
75) Chrysene-d12	13.70	240	90198	20.00	ng	-0.02
86) Perylene-d12	15.05	264	86227	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	432059	144.86	ng	-0.02
7) Phenol-d6	6.24	99	558281	145.15	ng	-0.03
23) Nitrobenzene-d5	7.15	82	388857	102.85	ng	-0.02
41) 2,4,6-Tribromophenol	10.40	330	108278	134.18	ng	-0.02
44) 2-Fluorobiphenyl	8.95	172	603522	92.78	ng	-0.02
78) Terphenyl-d14	12.66	244	326472	78.51	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.24	77	755	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.15	70	52549	20.89 ng	#	79
25) Isophorone	7.15	82	290338	41.67 ng	#	66
49) Dimethylphthalate	9.35	163	259789	37.77 ng		99
56) 2,4-Dinitrotoluene	9.61	165	11346	5.67 ng	#	10
66) 4-Bromophenyl-phenylether	10.40	248	8296	5.55 ng	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089250.D
Acq On : 23 Jul 2016 23:59
Operator : UM/SJ
Sample : H4129-12
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0

Quant Time: Jul 25 01:13:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

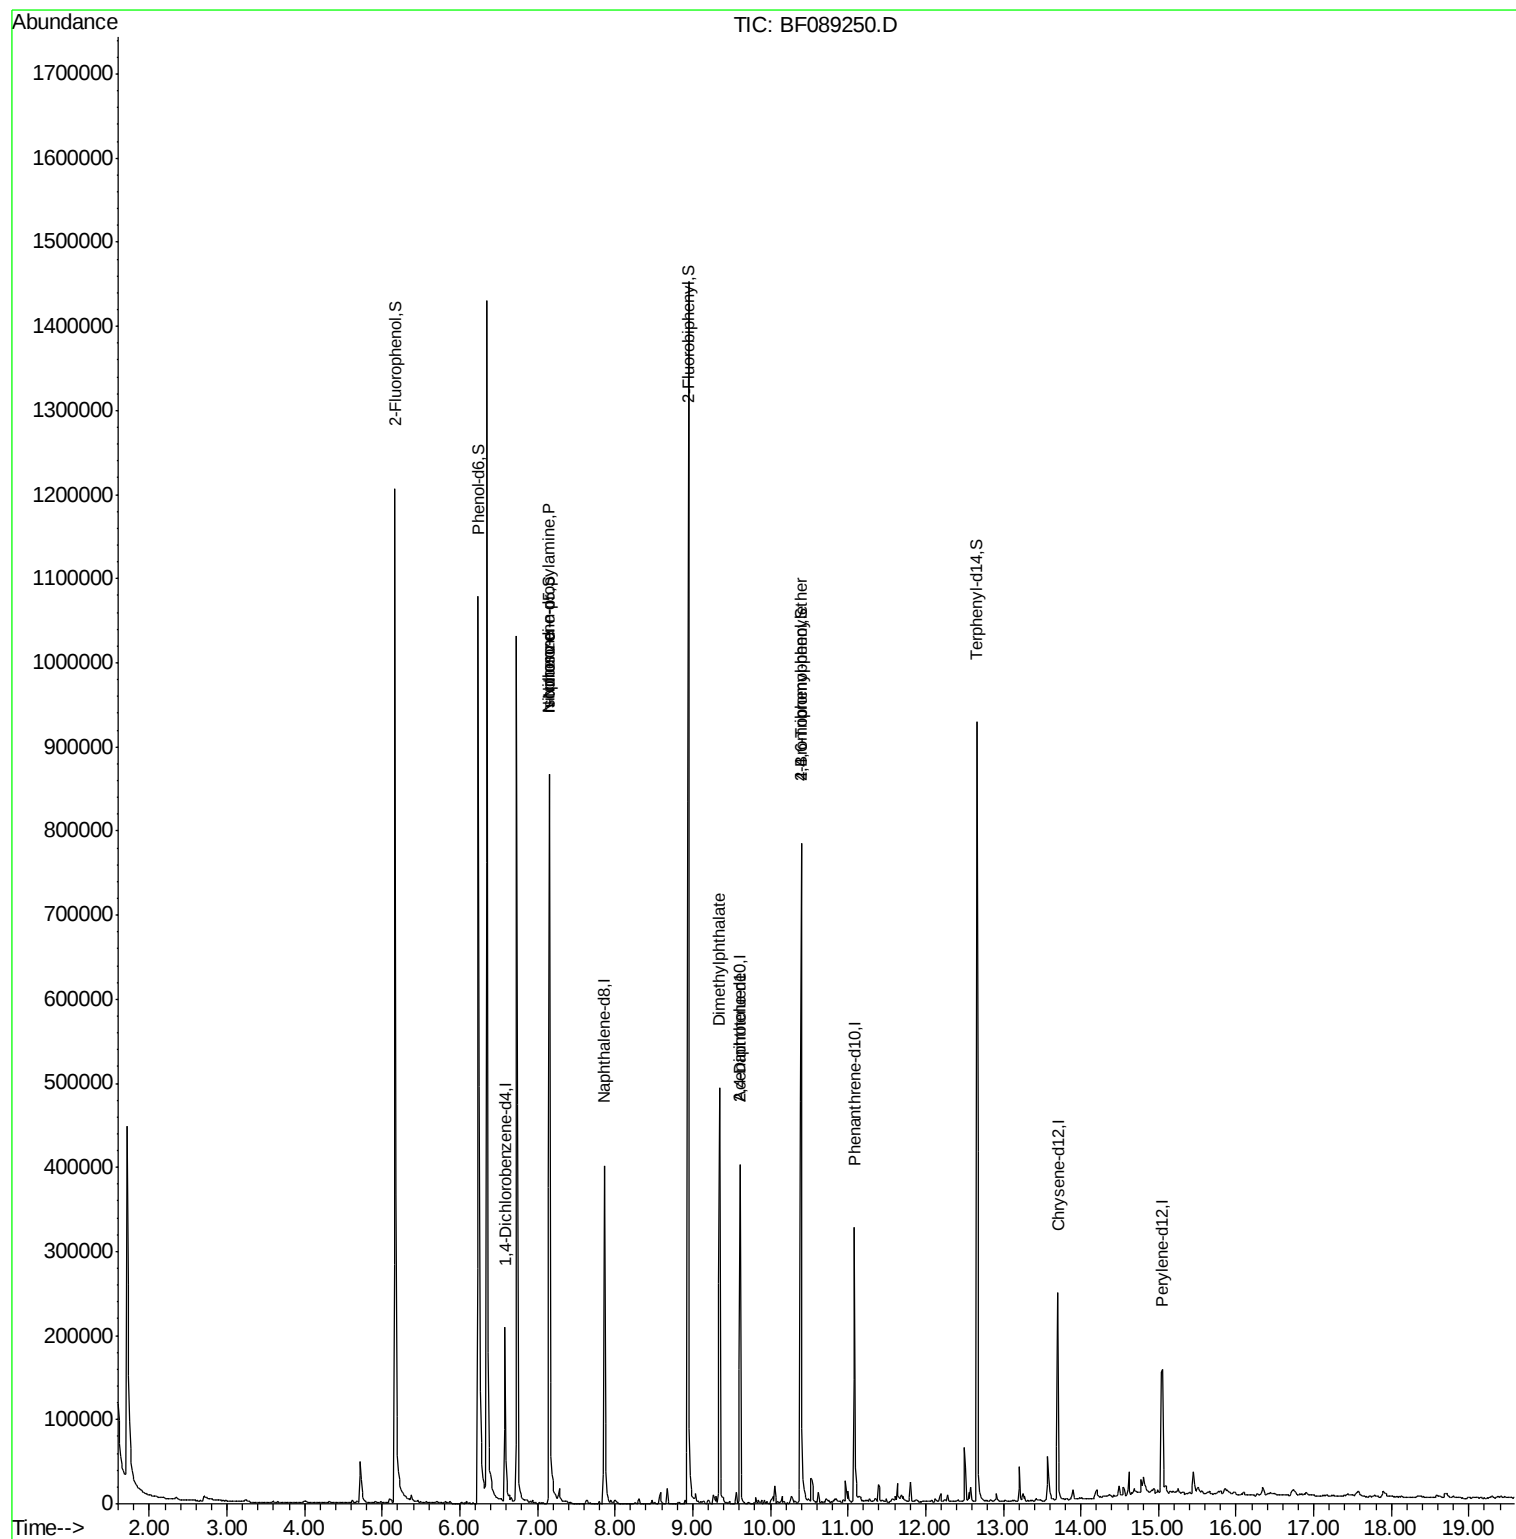




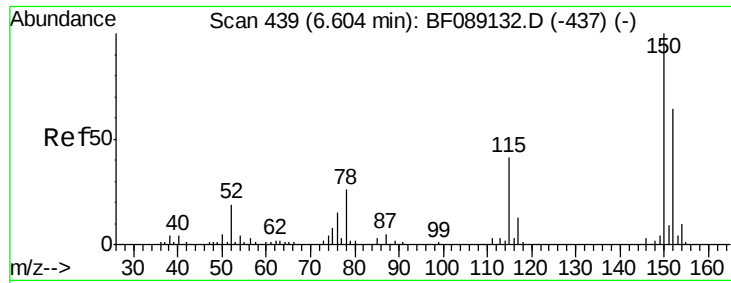


#1

1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.58 min Scan# 437
 Delta R.T. -0.02 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0




Tgt Ion:152 Resp: 45362
 Ion Ratio Lower Upper
 152 100
 150 153.9 125.1 187.7
 115 60.8 51.1 76.7

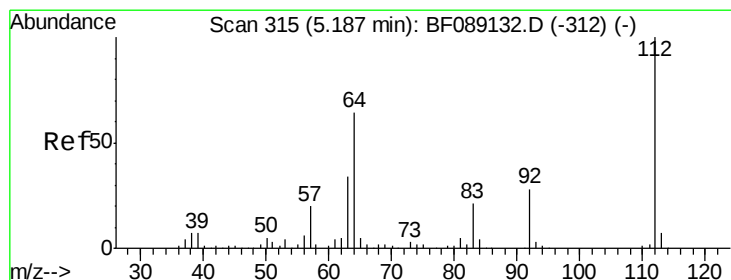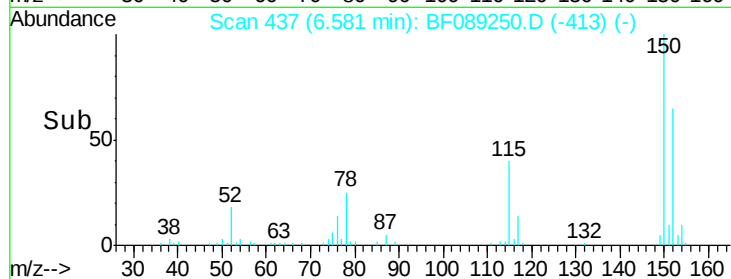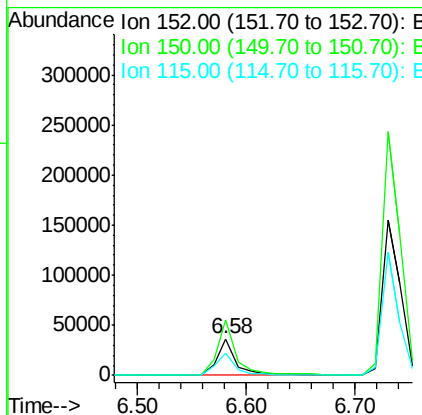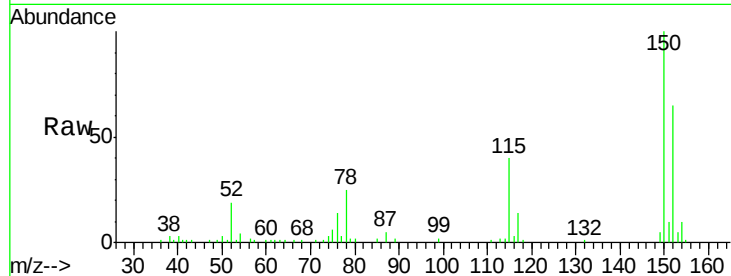


#5

2-Fluorophenol
 Concen: 144.86 ng
 RT: 5.16 min Scan# 313
 Delta R.T. -0.02 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Tgt Ion:112 Resp: 432059
 Ion Ratio Lower Upper
 112 100
 64 60.2 51.0 76.4
 63 32.5 27.3 40.9

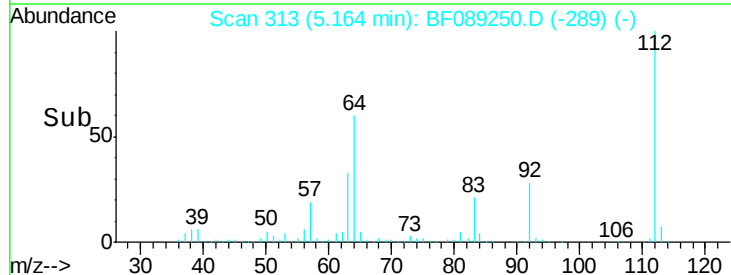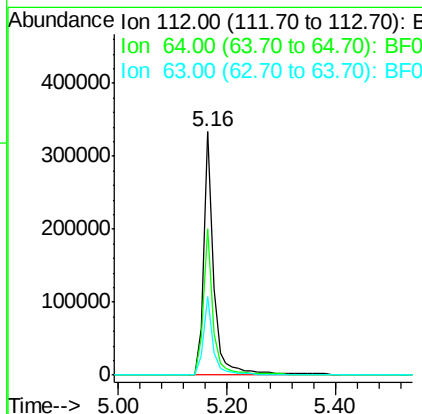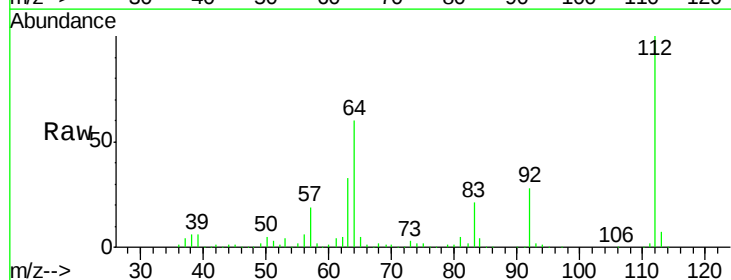

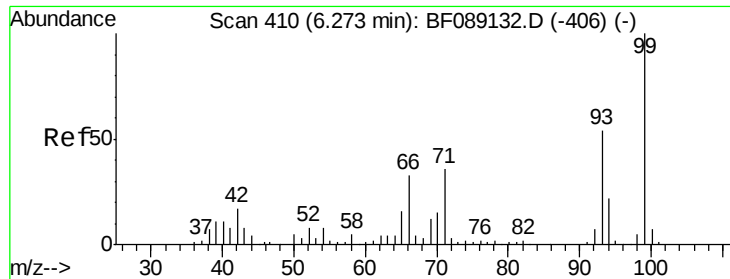

#7

Phenol-d6

Concen: 145.15 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.03 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0


Tgt Ion: 99 Resp: 558281

Ion Ratio Lower Upper

99 100

42 18.8 13.5 20.3




71 38.8 28.9 43.3

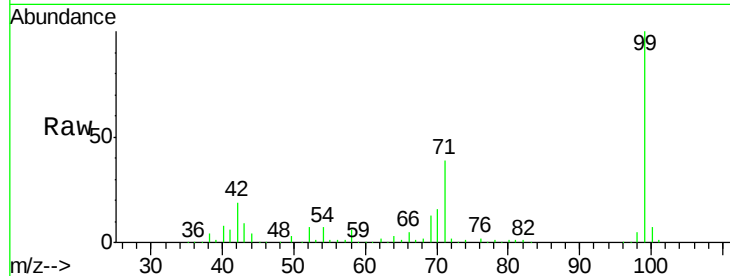

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

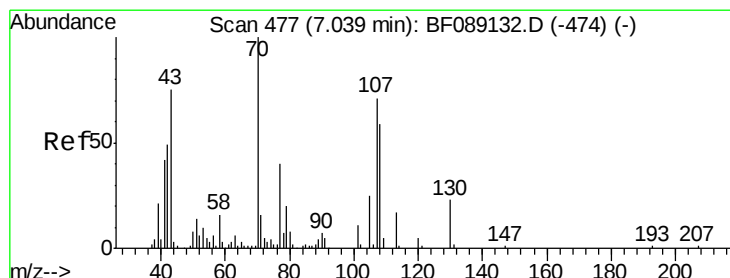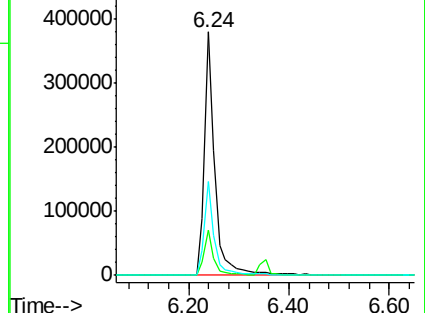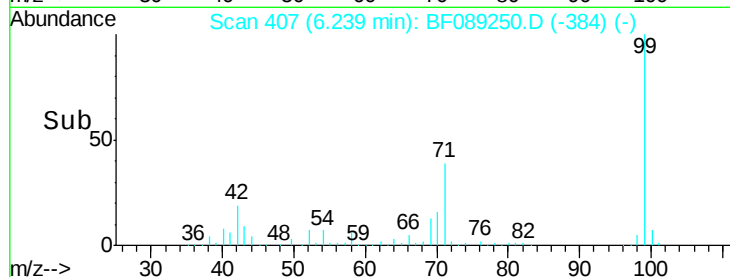

#19

n-Nitroso-di-n-propylamine

Concen: 20.89 ng

RT: 7.15 min Scan# 487

Delta R.T. 0.11 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59

Tgt Ion: 70 Resp: 52549


Ion Ratio Lower Upper

70 100

42 43.5 39.2 58.8

101 0.0 8.5 12.7#

130 1.8 18.4 27.6#


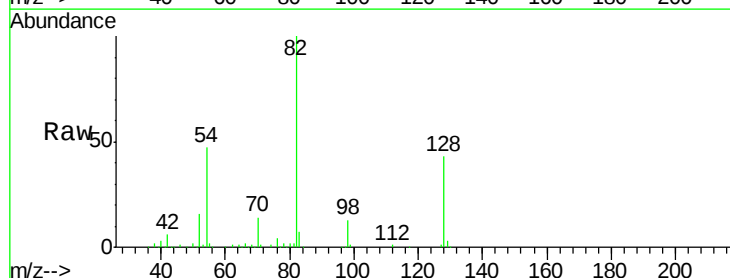



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

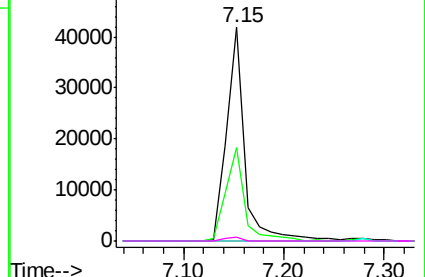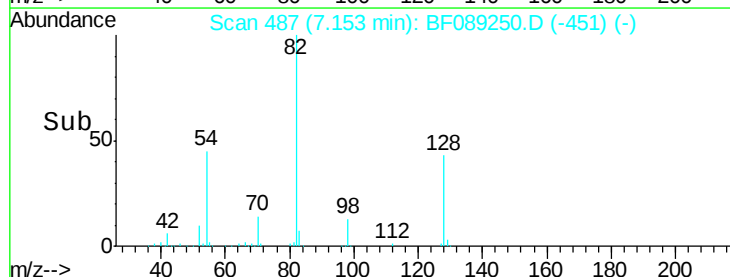



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.02 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0

Tgt Ion:136 Resp: 200886


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 7.7 7.0 10.4

68 5.7 5.0 7.6



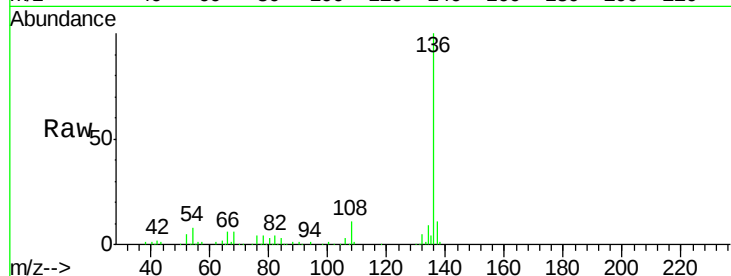


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

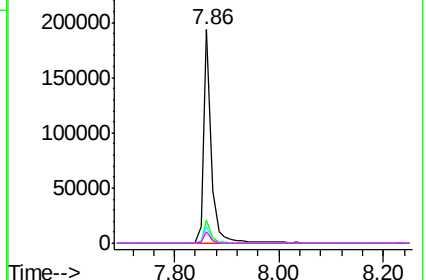

#23

Nitrobenzene-d5

Concen: 102.85 ng

RT: 7.15 min Scan# 487

Delta R.T. -0.02 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59


Tgt Ion: 82 Resp: 388857

Ion Ratio Lower Upper

82 100

128 43.4 33.0 49.6



54 46.7 39.0 58.4




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

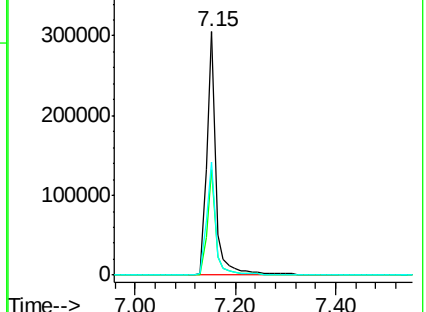



#25

Isophorone

Concen: 41.67 ng

RT: 7.15 min Scan# 487

Delta R.T. -0.29 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0


Tgt Ion: 82 Resp: 290338

Ion Ratio Lower Upper

82 100

95 0.0 6.1 9.1#




138 0.0 13.6 20.4#

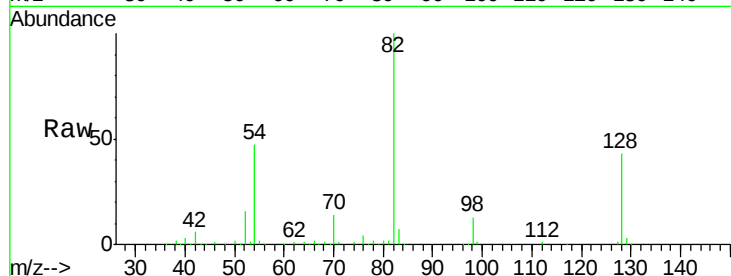

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

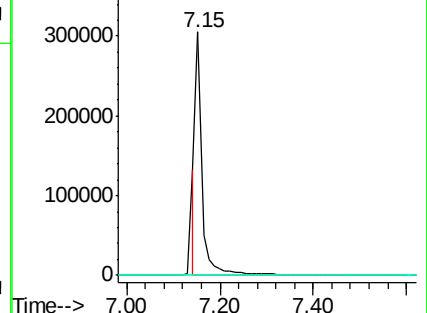

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.02 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59


Tgt Ion: 164 Resp: 89629

Ion Ratio Lower Upper

164 100

162 106.5 84.1 126.1



160 47.8 37.1 55.7




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

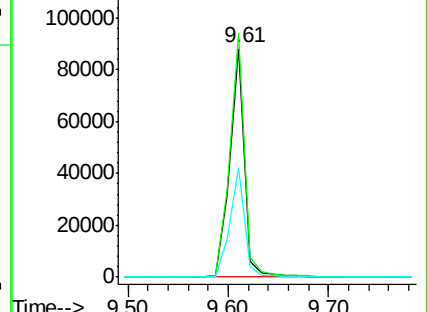


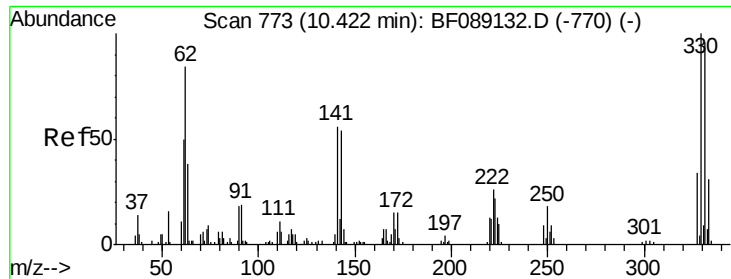




#41
 2,4,6-Tribromophenol
 Concen: 134.18 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.02 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Tgt Ion:330 Resp: 108278
 Ion Ratio Lower Upper
 330 100
 332 96.9 77.2 115.8
 141 46.2 42.2 63.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


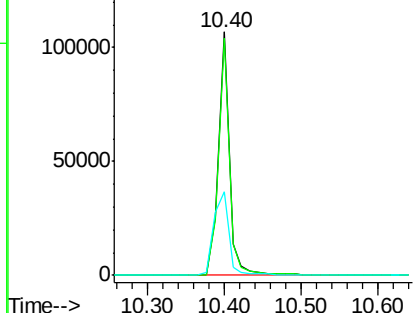



#44
 2-Fluorobiphenyl
 Concen: 92.78 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.02 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Tgt Ion:172 Resp: 603522
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.2 43.8
 170 23.8 19.1 28.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




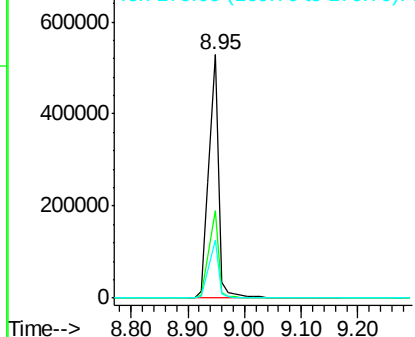


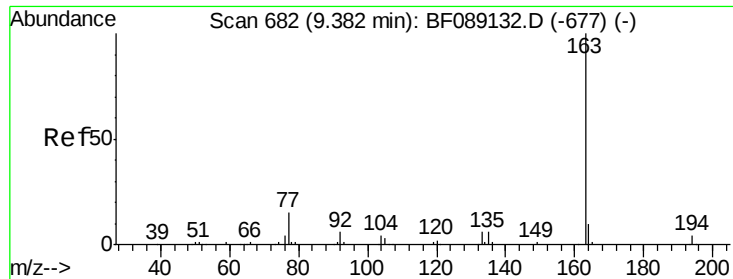

#49
Dimethylphthalate
Concen: 37.77 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.03 min
Lab File: BF089250.D
Acq: 23 Jul 2016 23:59




Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0


Tgt Ion:163 Resp: 259789
Ion Ratio Lower Upper
163 100
194 3.5 2.9 4.3
164 9.7 7.6 11.4

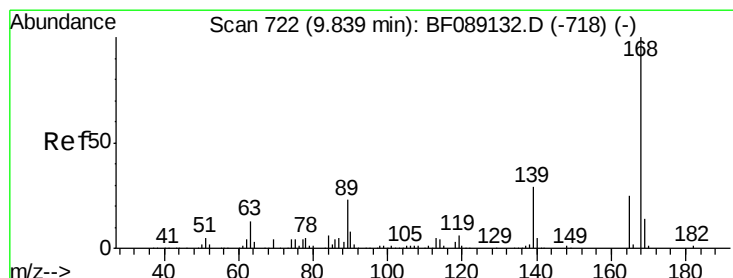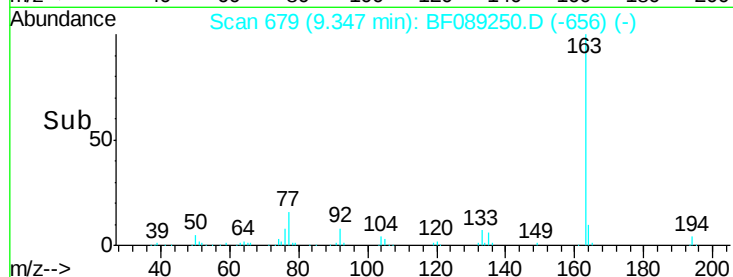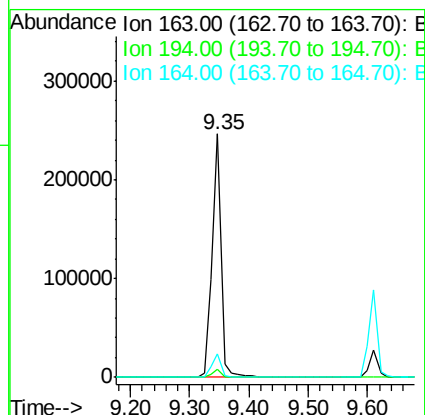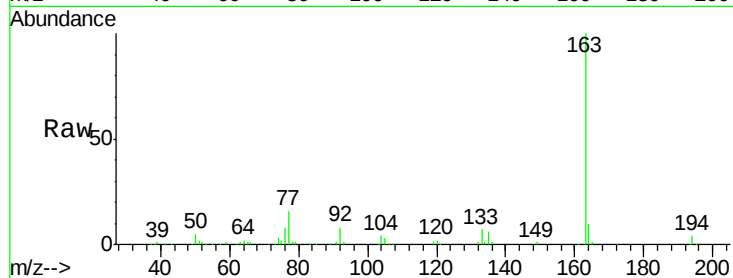

#56
2,4-Dinitrotoluene
Concen: 5.67 ng
RT: 9.61 min Scan# 702
Delta R.T. -0.23 min
Lab File: BF089250.D
Acq: 23 Jul 2016 23:59

Tgt Ion:165 Resp: 11346
Ion Ratio Lower Upper
165 100
63 0.0 55.4 83.2#
89 0.0 74.3 111.5#
182 0.0 2.0 3.0#

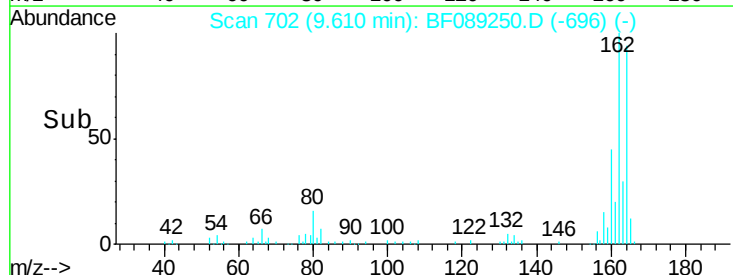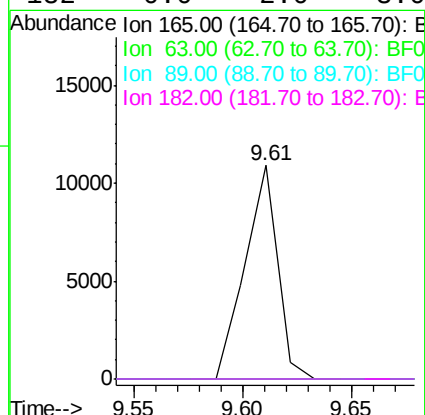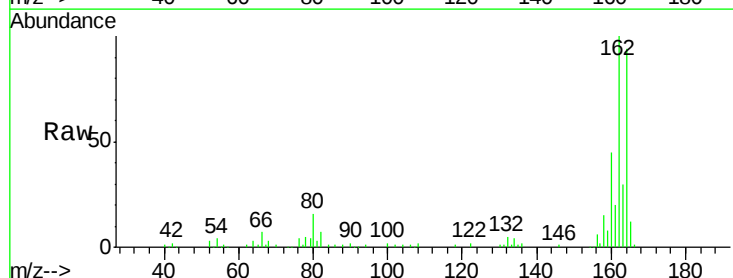


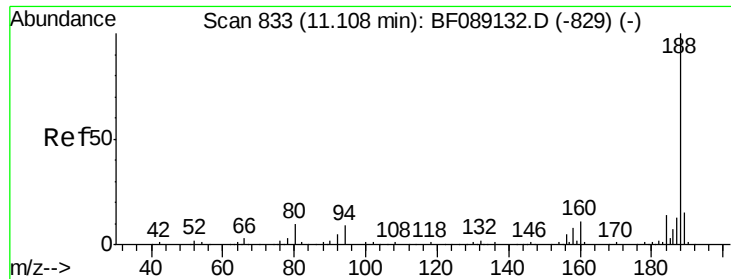




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.08 min Scan# 831
 Delta R.T. -0.02 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Tgt Ion:188 Resp: 151110
 Ion Ratio Lower Upper
 188 100
 94 7.5 7.0 10.4
 80 7.8 7.7 11.5

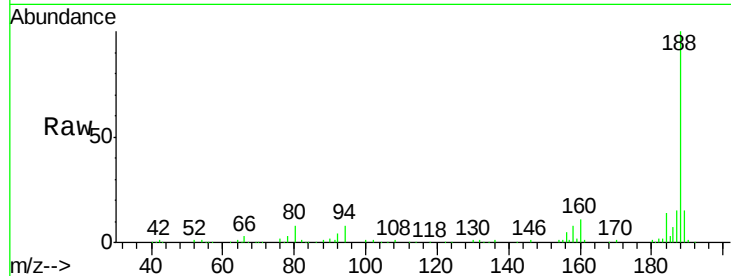


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0


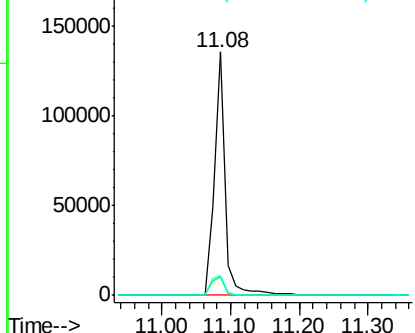



#66
 4-Bromophenyl-phenylether
 Concen: 5.55 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.26 min
 Lab File: BF089250.D
 Acq: 23 Jul 2016 23:59

Tgt Ion:248 Resp: 8296
 Ion Ratio Lower Upper
 248 100
 250 187.6 76.9 115.3#
 141 434.6 77.4 116.2#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

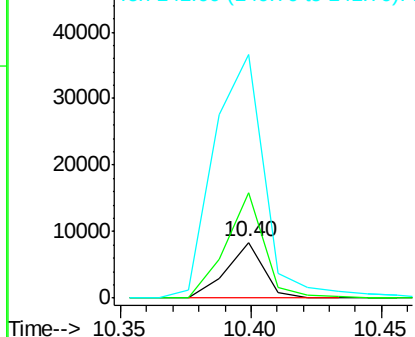

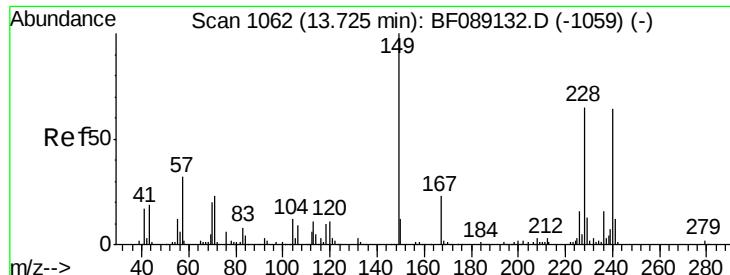

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.70 min Scan# 1060

Delta R.T. -0.02 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0


Tgt Ion:240 Resp: 90198

Ion Ratio Lower Upper

240 100

120 11.1 13.6 20.4#




236 24.7 20.5 30.7

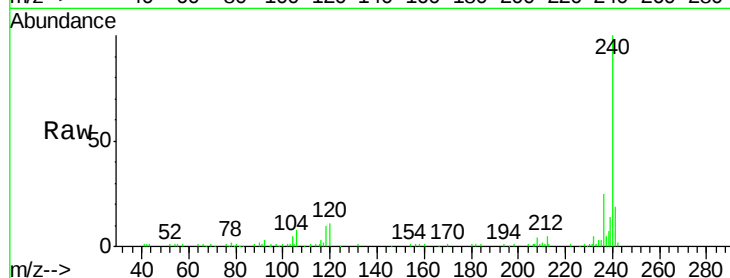

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

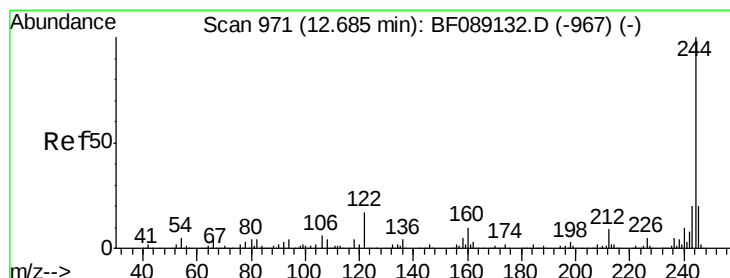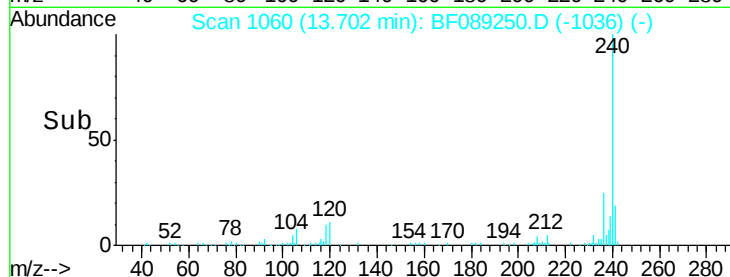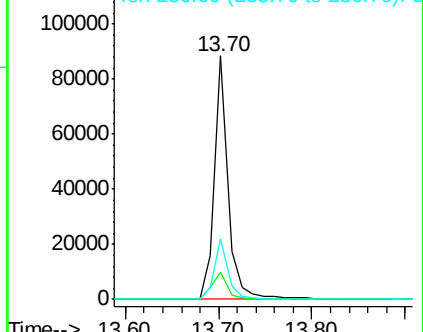

#78

Terphenyl-d14

Concen: 78.51 ng

RT: 12.66 min Scan# 969

Delta R.T. -0.02 min

Lab File: BF089250.D

Acq: 23 Jul 2016 23:59


Tgt Ion:244 Resp: 326472

Ion Ratio Lower Upper

244 100

212 8.2 7.0 10.4



122 16.8 13.8 20.8

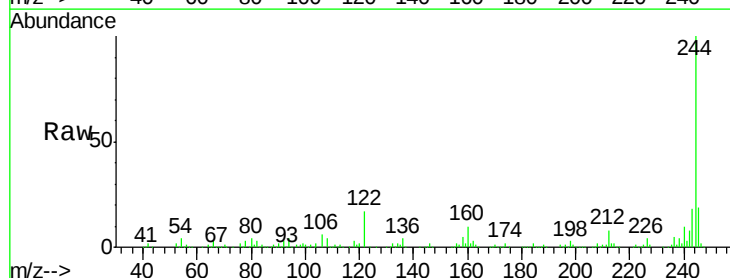


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

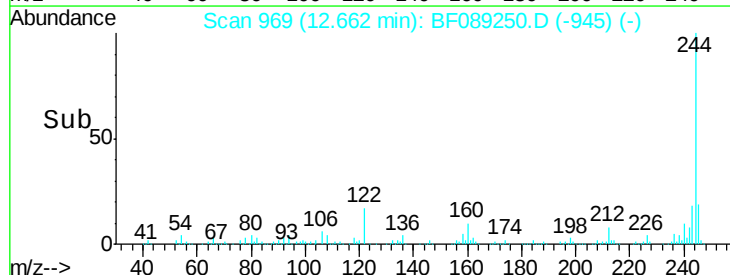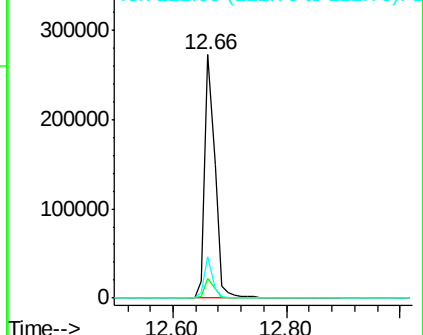


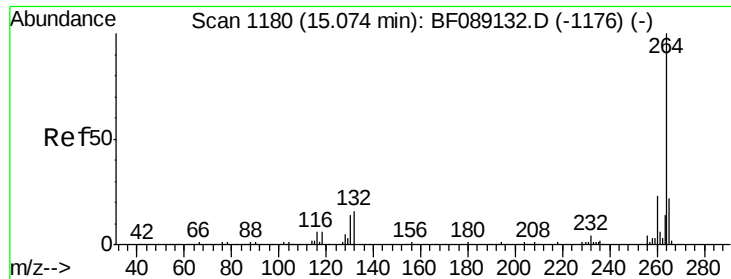

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.05 min Scan# 1178
Delta R.T. -0.02 min
Lab File: BF089250.D
Acq: 23 Jul 2016 23:59

Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.5	27.7
265	20.7	17.3	25.9



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

