

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089251.D
 Acq On : 24 Jul 2016 00:30
 Operator : UM/SJ
 Sample : H4129-08
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSB-12-10.0-12.0

Quant Time: Jul 25 04:54:06 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 03:29:41 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	46696	20.00	ng	0.00
21) Naphthalene-d8	7.86	136	208832	20.00	ng	-0.01
38) Acenaphthene-d10	9.61	164	91281	20.00	ng	0.00
63) Phenanthrene-d10	11.08	188	156376	20.00	ng	0.00
75) Chrysene-d12	13.70	240	98192	20.00	ng	-0.01
86) Perylene-d12	15.05	264	94545	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	461237	150.22	ng	0.00
7) Phenol-d6	6.24	99	606520	153.18	ng	0.00
23) Nitrobenzene-d5	7.15	82	388500	98.85	ng	0.00
41) 2,4,6-Tribromophenol	10.40	330	106263	129.30	ng	0.00
44) 2-Fluorobiphenyl	8.95	172	662419	99.99	ng	0.00
78) Terphenyl-d14	12.66	244	399438	88.23	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.35	163	283652	40.49	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089251.D
Acq On : 24 Jul 2016 00:30
Operator : UM/SJ
Sample : H4129-08
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSB-12-10.0-12.0

Quant Time: Jul 25 04:54:06 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 03:29:41 2016
Response via : Initial Calibration

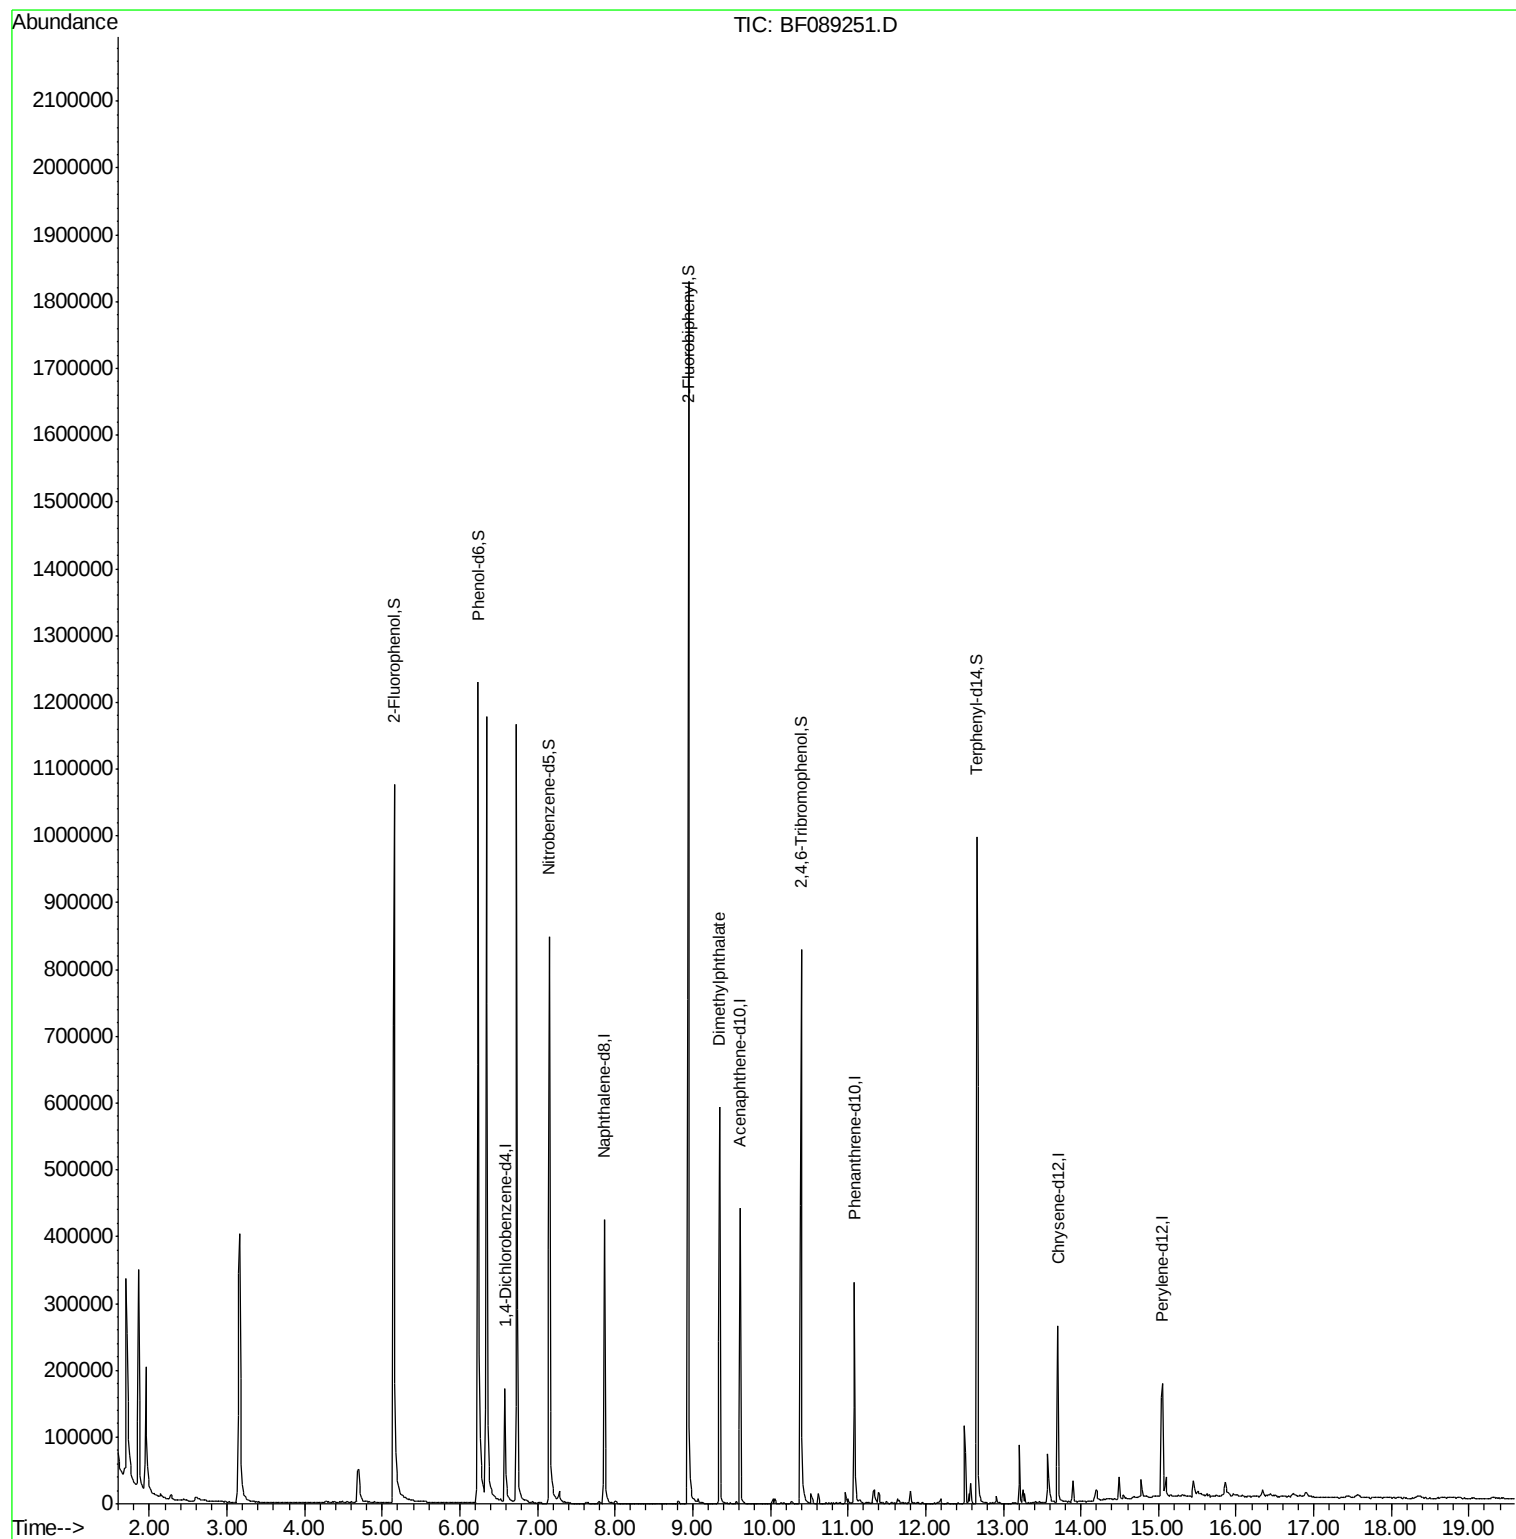

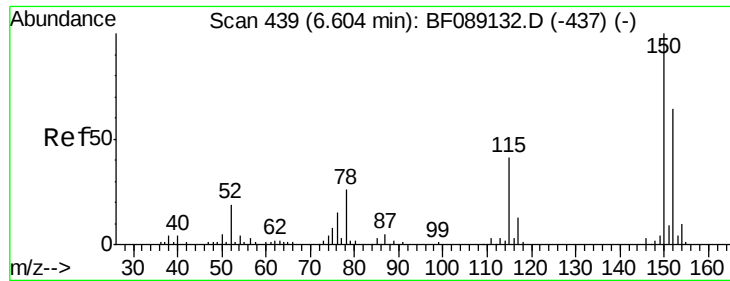

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 437

Delta R.T. 0.00 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30

Instrument :

BNA_F

ClientSampleId :

KSB-12-10.0-12.0


Tgt Ion:152 Resp: 46696

Ion Ratio Lower Upper

152 100

150 157.5 125.1 187.7




115 60.2 51.1 76.7

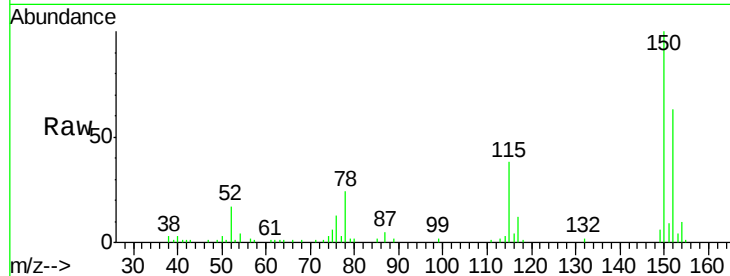

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

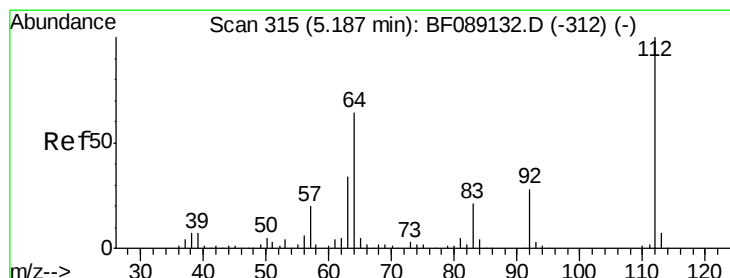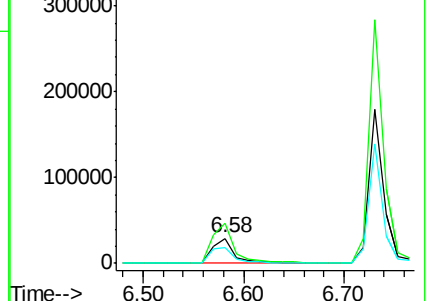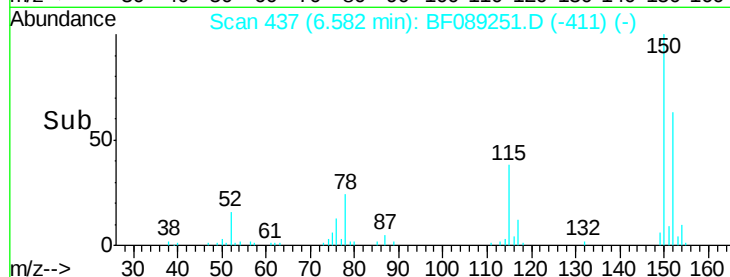

#5

2-Fluorophenol

Concen: 150.22 ng

RT: 5.15 min Scan# 312

Delta R.T. 0.00 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30


Tgt Ion:112 Resp: 461237

Ion Ratio Lower Upper

112 100

64 51.9 51.0 76.4



63 28.2 27.3 40.9

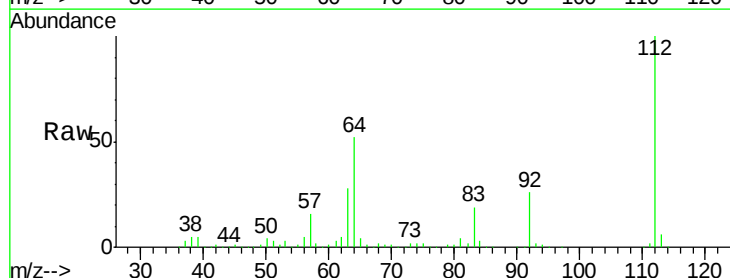


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

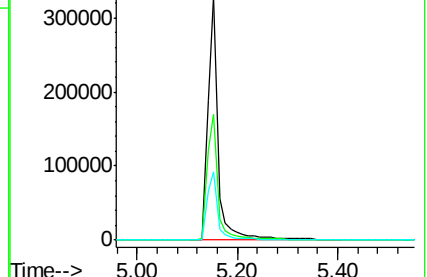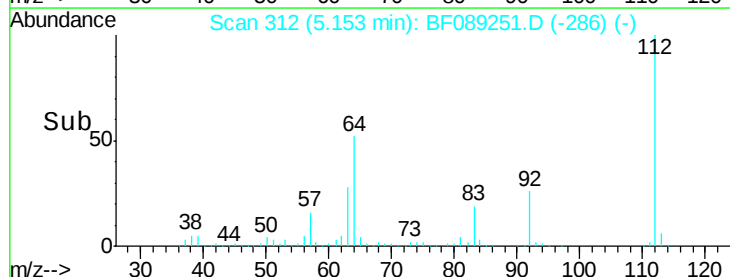

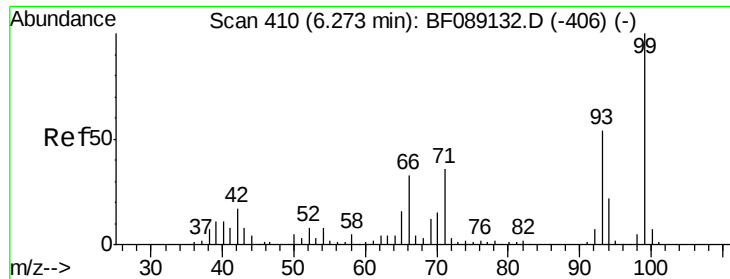

#7

Phenol-d6

Concen: 153.18 ng

RT: 6.24 min Scan# 407

Delta R.T. 0.00 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30

Instrument :

BNA_F

ClientSampleId :

KSB-12-10.0-12.0


Tgt Ion: 99 Resp: 606520

Ion Ratio Lower Upper

99 100

42 17.4 13.5 20.3




71 37.9 28.9 43.3

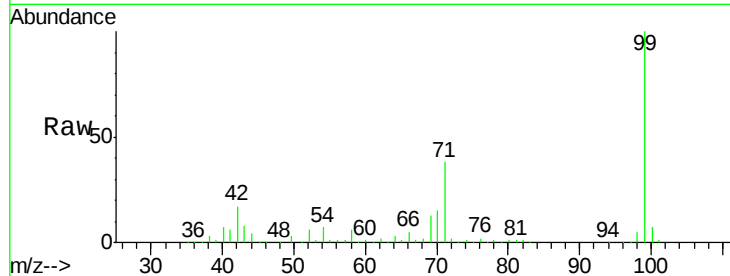

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

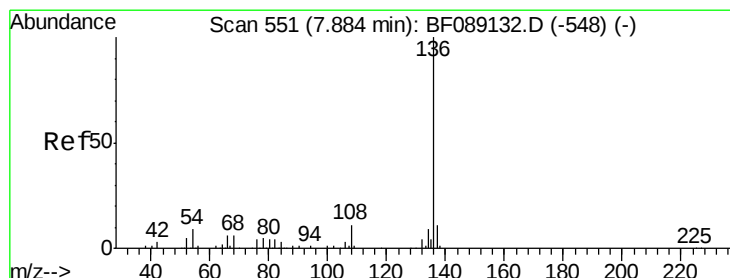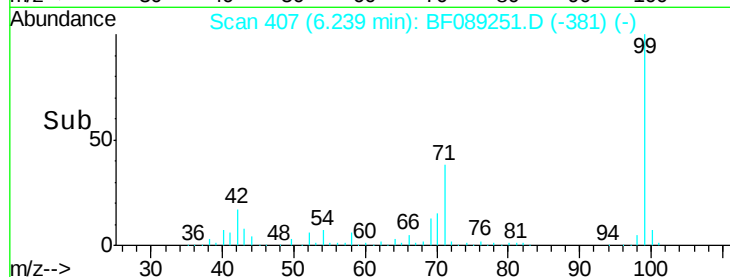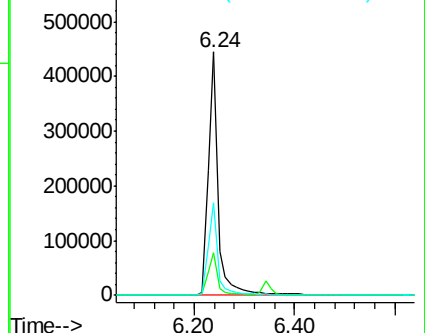

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.01 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30

Tgt Ion: 136 Resp: 208832


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 7.2 7.0 10.4

68 5.8 5.0 7.6


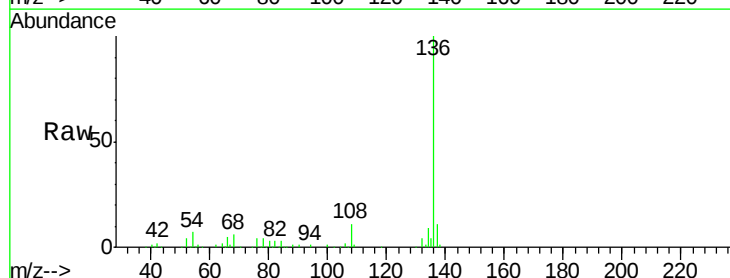



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

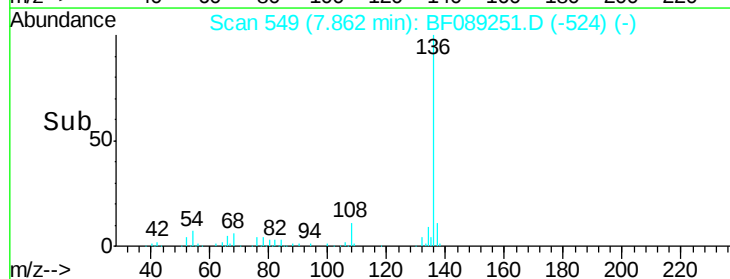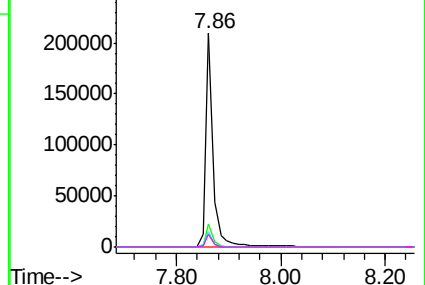


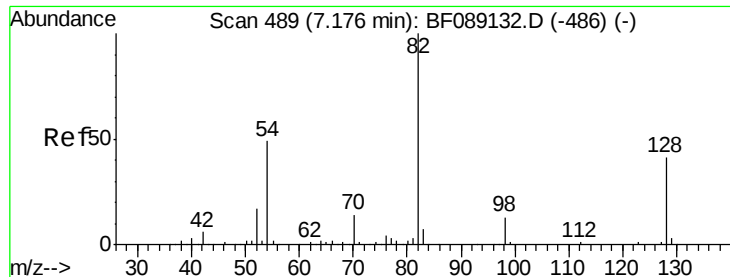




#23
 Nitrobenzene-d5
 Concen: 98.85 ng
 RT: 7.15 min Scan# 487
 Delta R.T. 0.00 min
 Lab File: BF089251.D
 Acq: 24 Jul 2016 00:30

Instrument :
 BNA_F
 ClientSampleId :
 KSB-12-10.0-12.0

Tgt Ion: 82 Resp: 388500
 Ion Ratio Lower Upper
 82 100
 128 43.0 33.0 49.6
 54 45.9 39.0 58.4

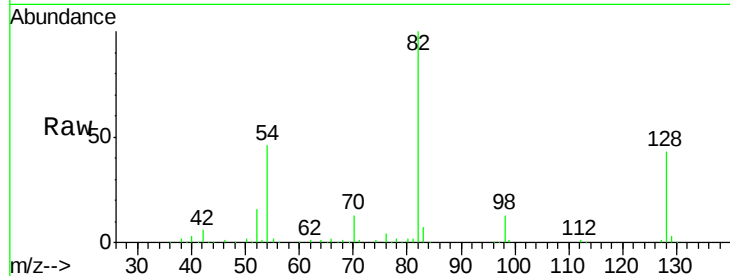


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

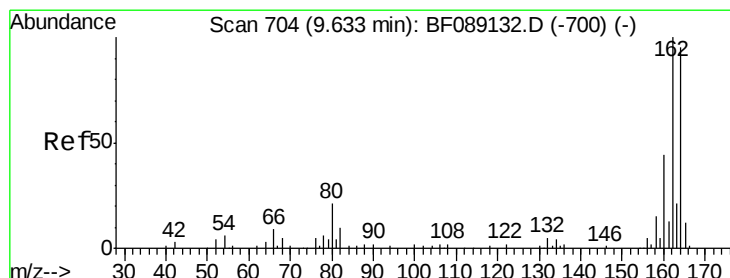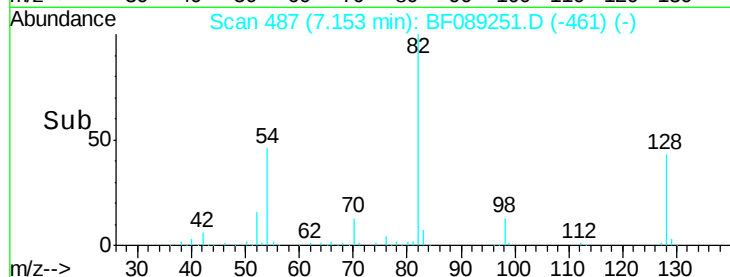
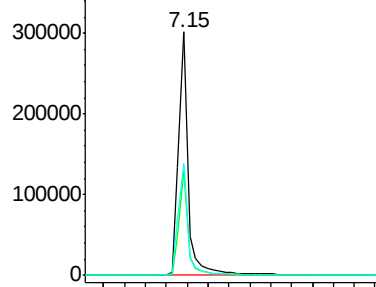



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 702
 Delta R.T. 0.00 min
 Lab File: BF089251.D
 Acq: 24 Jul 2016 00:30

Tgt Ion: 164 Resp: 91281
 Ion Ratio Lower Upper
 164 100
 162 104.6 84.1 126.1
 160 47.5 37.1 55.7

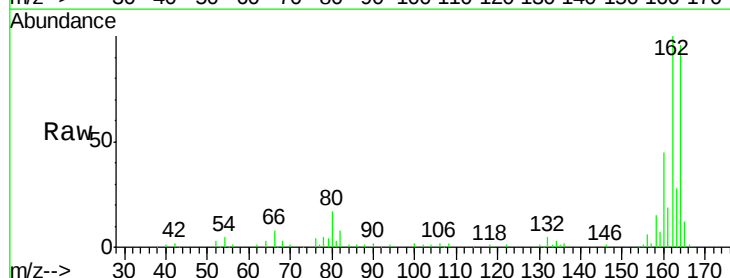

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

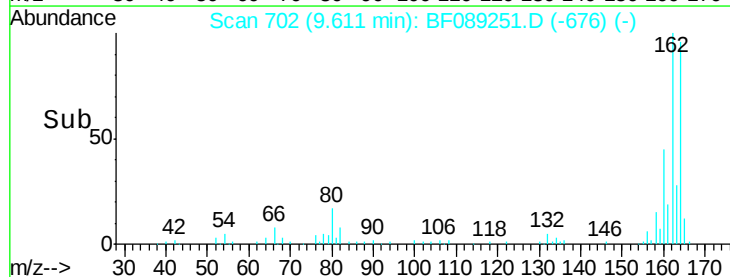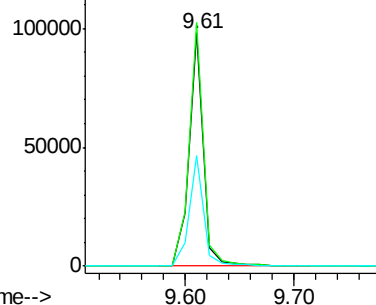


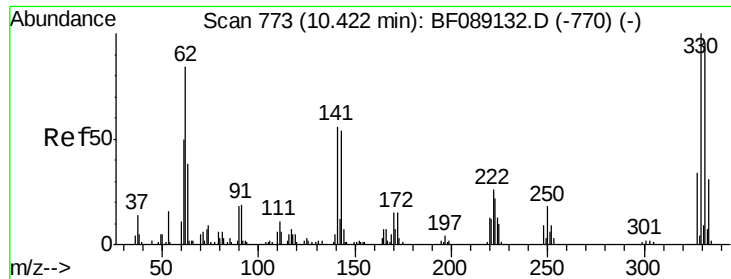




#41
 2,4,6-Tribromophenol
 Concen: 129.30 ng
 RT: 10.40 min Scan# 771
 Delta R.T. 0.00 min
 Lab File: BF089251.D
 Acq: 24 Jul 2016 00:30

Instrument :
 BNA_F
 ClientSampleId :
 KSB-12-10.0-12.0

Tgt Ion:330 Resp: 106263
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.2 115.8
 141 49.4 42.2 63.2

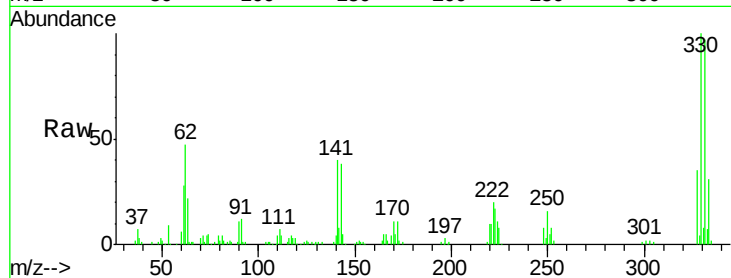


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

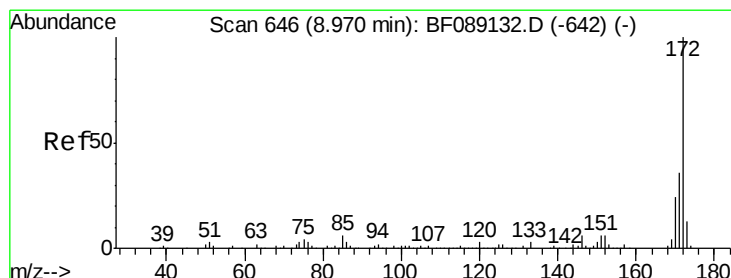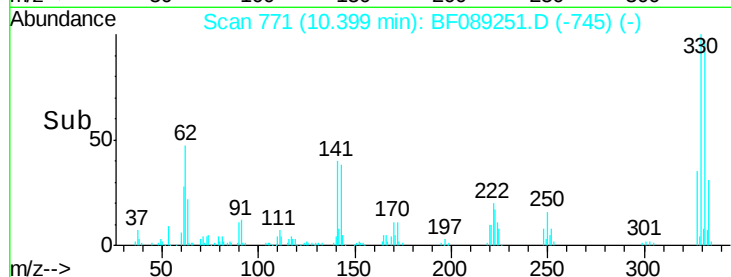
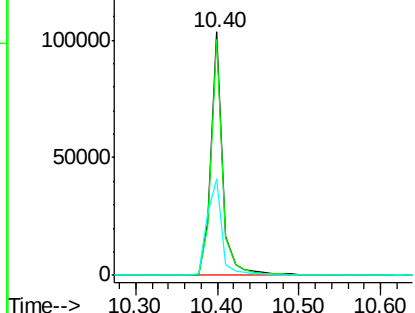



#44
 2-Fluorobiphenyl
 Concen: 99.99 ng
 RT: 8.95 min Scan# 644
 Delta R.T. 0.00 min
 Lab File: BF089251.D
 Acq: 24 Jul 2016 00:30

Tgt Ion:172 Resp: 662419
 Ion Ratio Lower Upper
 172 100
 171 36.5 29.2 43.8
 170 24.2 19.1 28.7

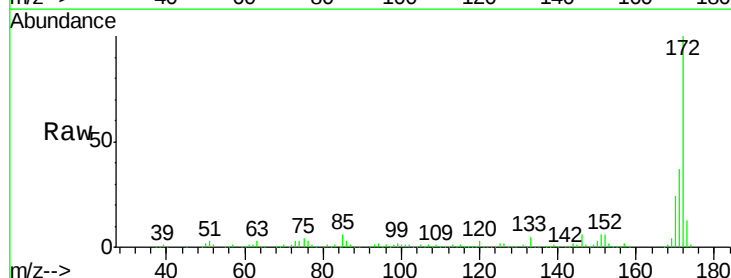

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



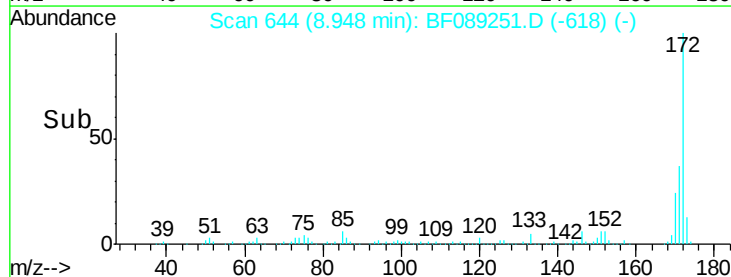
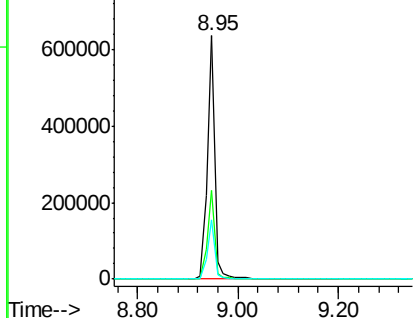


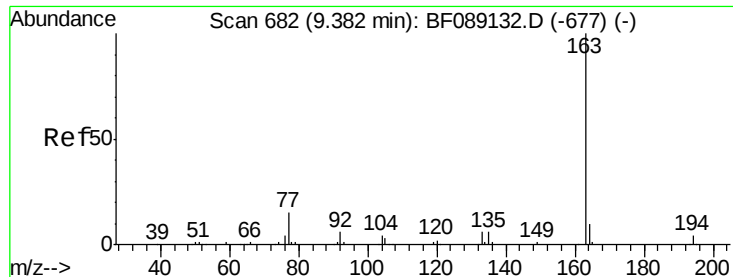

#49
Dimethylphthalate
Concen: 40.49 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.01 min
Lab File: BF089251.D
Acq: 24 Jul 2016 00:30




Instrument :
BNA_F
ClientSampleId :
KSB-12-10.0-12.0


Tgt Ion:163 Resp: 283652
Ion Ratio Lower Upper
163 100
194 3.6 2.9 4.3
164 9.8 7.6 11.4

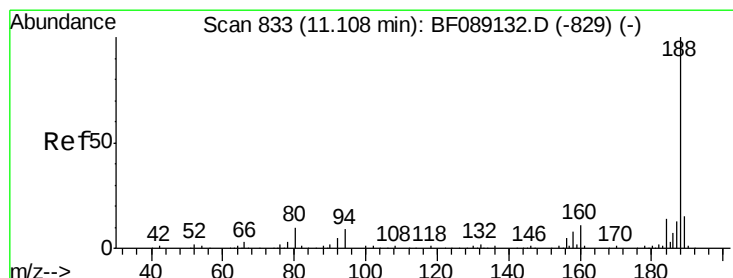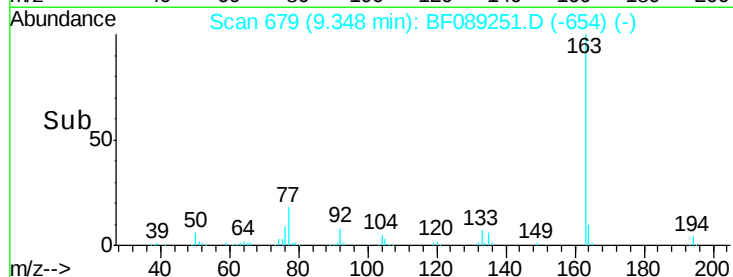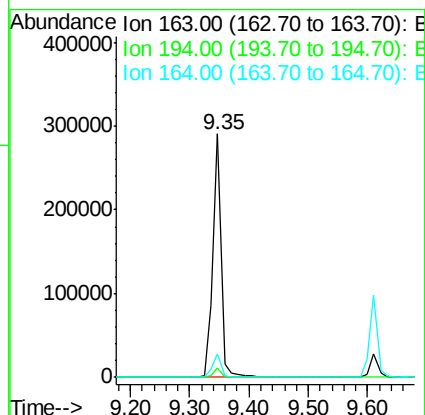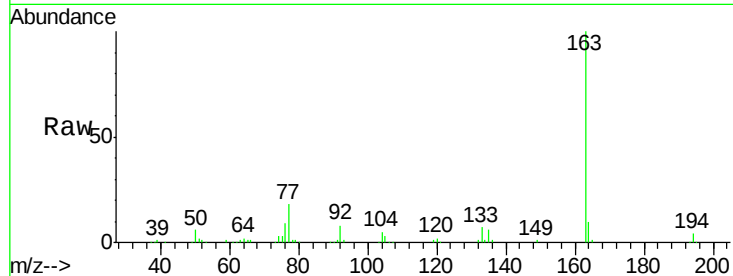

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.08 min Scan# 831
Delta R.T. 0.00 min
Lab File: BF089251.D
Acq: 24 Jul 2016 00:30

Tgt Ion:188 Resp: 156376
Ion Ratio Lower Upper
188 100
94 7.6 7.0 10.4
80 8.4 7.7 11.5

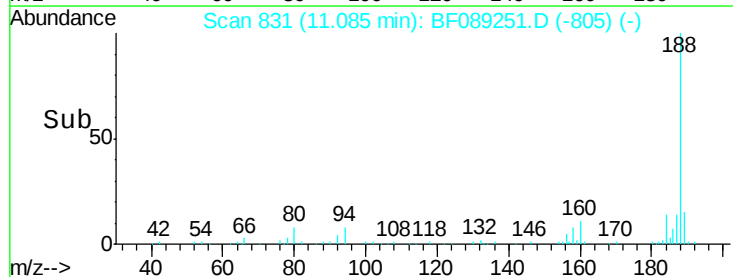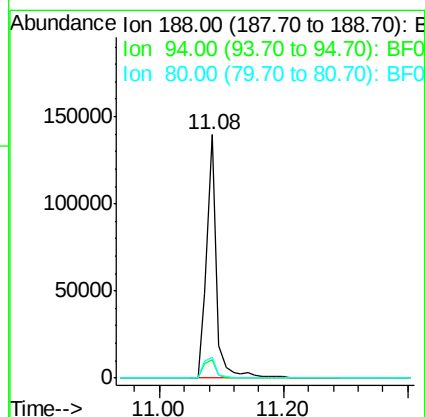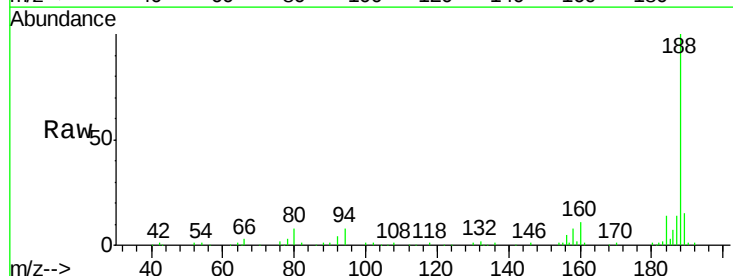

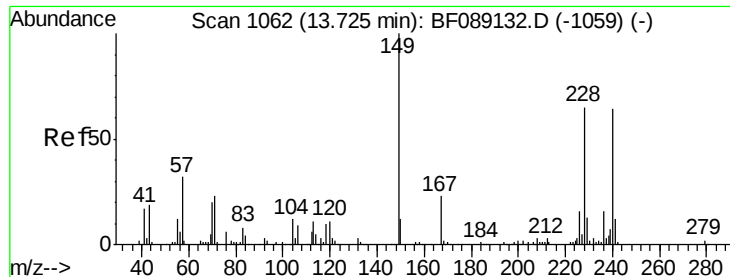

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.70 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30

Instrument :

BNA_F

ClientSampleId :

KSB-12-10.0-12.0


Tgt Ion:240 Resp: 98192

Ion Ratio Lower Upper

240 100

120 12.0 13.6 20.4#




236 25.5 20.5 30.7

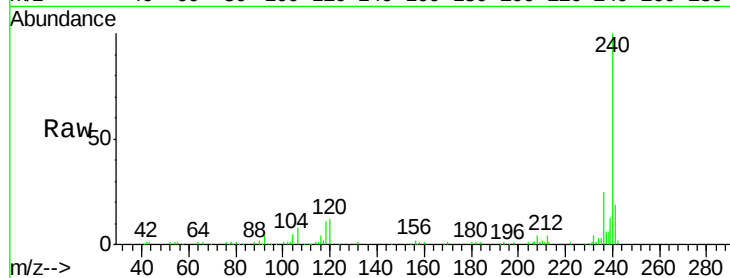

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

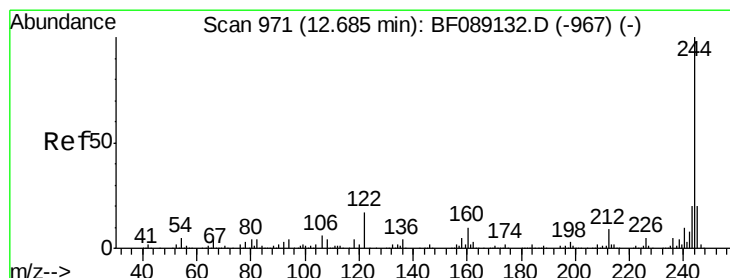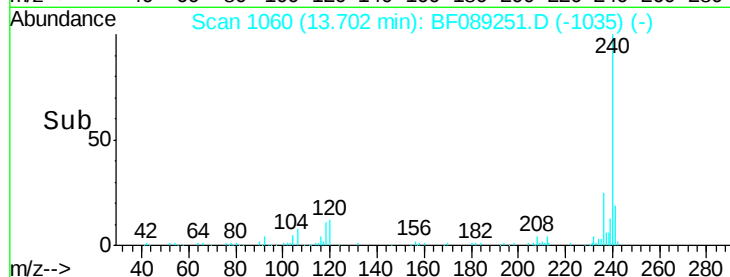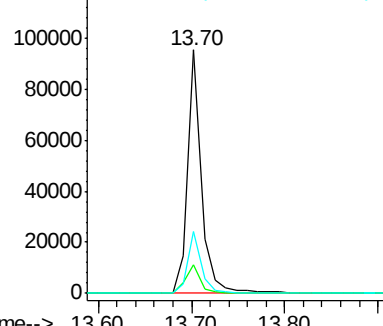

#78

Terphenyl-d14

Concen: 88.23 ng

RT: 12.66 min Scan# 969

Delta R.T. -0.01 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30


Tgt Ion:244 Resp: 399438

Ion Ratio Lower Upper

244 100

212 8.4 7.0 10.4



122 16.9 13.8 20.8



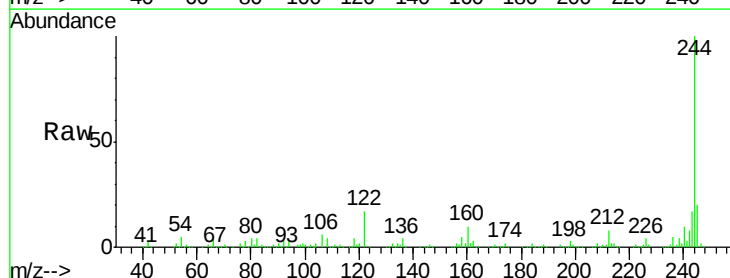


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

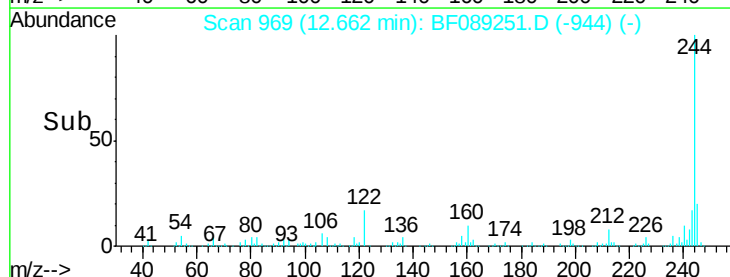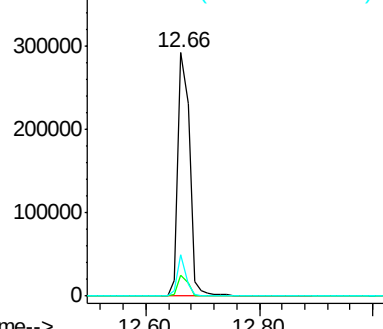

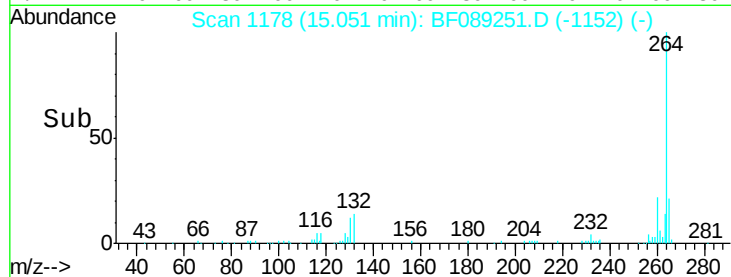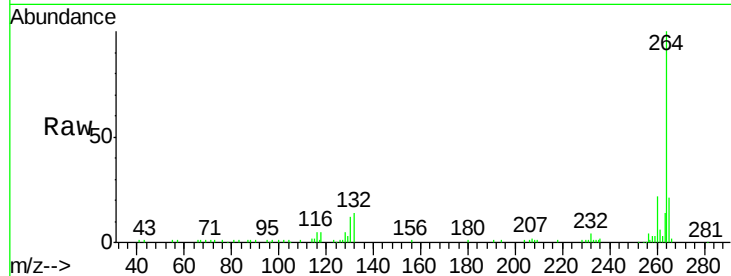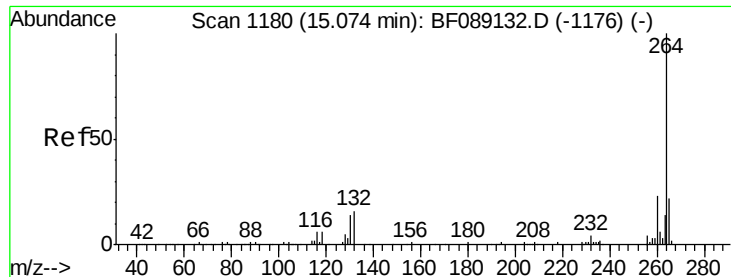

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.05 min Scan# 1178

Delta R.T. 0.00 min

Lab File: BF089251.D

Acq: 24 Jul 2016 00:30

Instrument :

BNA_F

ClientSampleId :

KSB-12-10.0-12.0

Tgt Ion: 264 Resp: 94545

Ion Ratio Lower Upper

264 100

260 22.4 18.5 27.7

265 21.3 17.3 25.9

