

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089265.D
 Acq On : 24 Jul 2016 7:35
 Operator : UM/SJ
 Sample : H4129-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSB-17-8.0-10.0

Quant Time: Jul 25 05:21:12 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 03:29:41 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	46810	20.00	ng	0.00
21) Naphthalene-d8	7.86	136	203994	20.00	ng	-0.01
38) Acenaphthene-d10	9.61	164	87863	20.00	ng	0.00
63) Phenanthrene-d10	11.08	188	139840	20.00	ng	0.00
75) Chrysene-d12	13.70	240	92876	20.00	ng	-0.01
86) Perylene-d12	15.05	264	89442	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	428006	139.06	ng	0.01
7) Phenol-d6	6.24	99	572665	144.28	ng	0.00
23) Nitrobenzene-d5	7.15	82	377268	98.27	ng	0.00
41) 2,4,6-Tribromophenol	10.40	330	97807	123.64	ng	0.00
44) 2-Fluorobiphenyl	8.95	172	590494	92.60	ng	0.00
78) Terphenyl-d14	12.66	244	293872	68.63	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.35	163	269280	39.94	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089265.D
Acq On : 24 Jul 2016 7:35
Operator : UM/SJ
Sample : H4129-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSB-17-8.0-10.0

Quant Time: Jul 25 05:21:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 03:29:41 2016
Response via : Initial Calibration

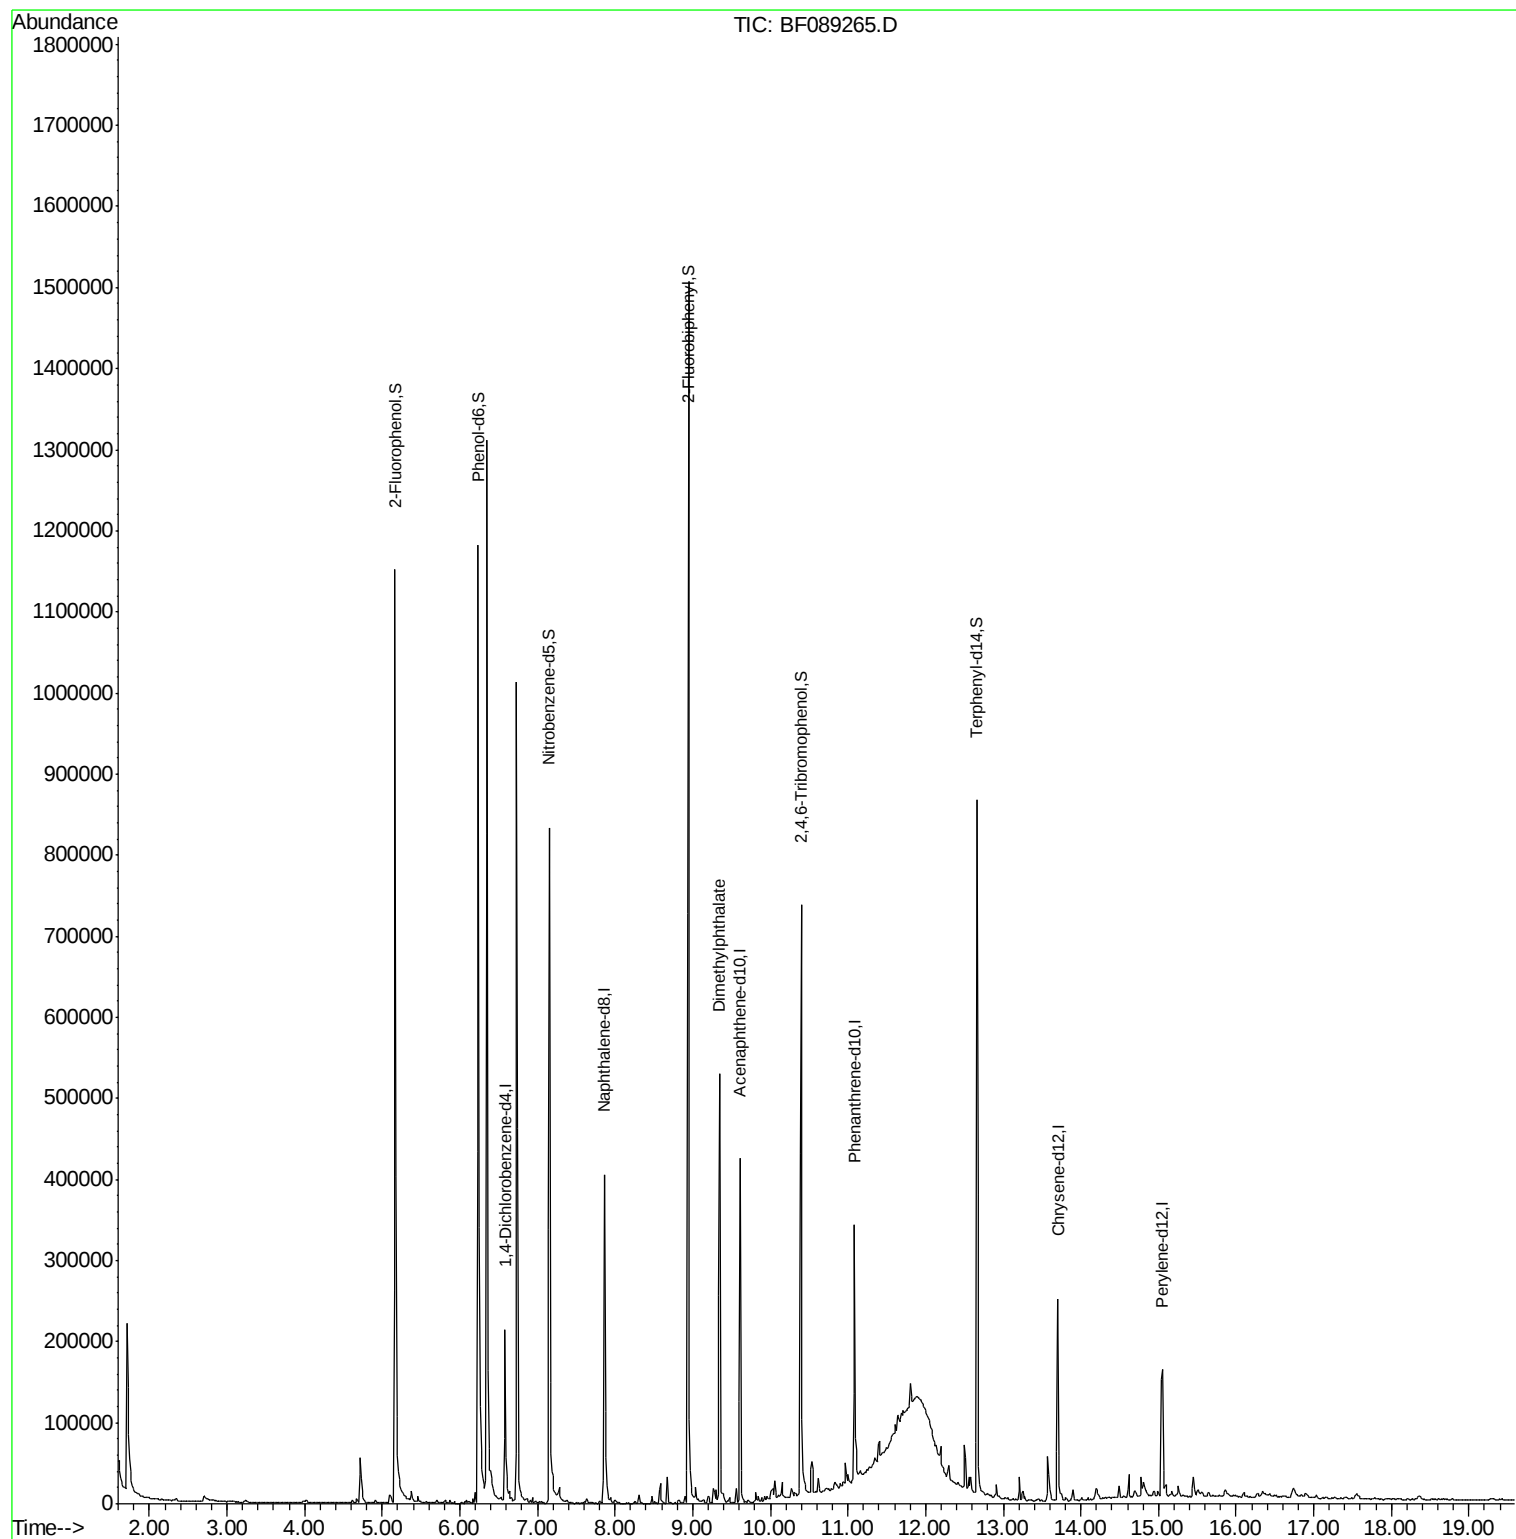


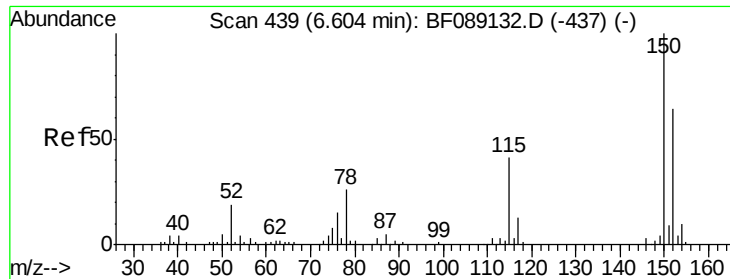




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.58 min Scan# 437
 Delta R.T. -0.00 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Instrument :
 BNA_F
 ClientSampleId :
 KSB-17-8.0-10.0

Tgt Ion:152 Resp: 46810
 Ion Ratio Lower Upper
 152 100
 150 154.3 125.1 187.7
 115 62.1 51.1 76.7

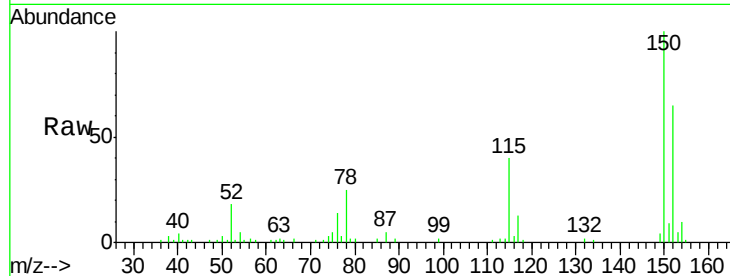


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

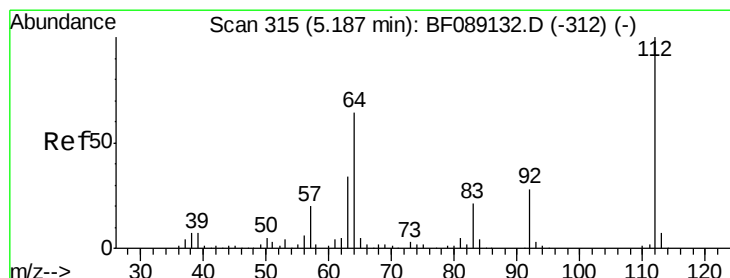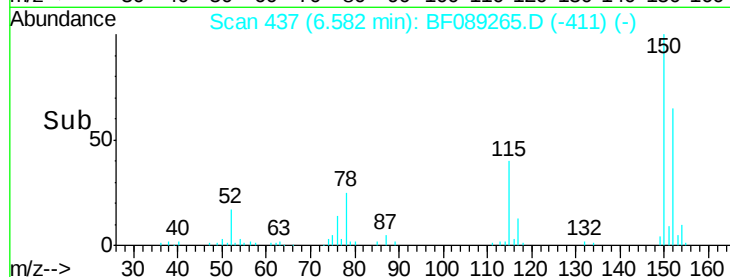
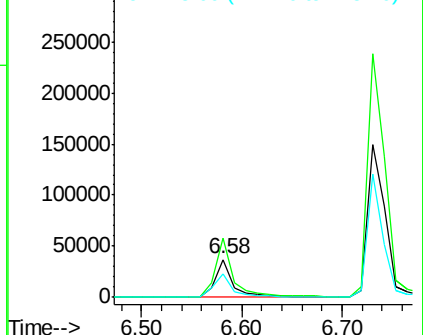



#5
 2-Fluorophenol
 Concen: 139.06 ng
 RT: 5.16 min Scan# 313
 Delta R.T. 0.01 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Tgt Ion:112 Resp: 428006
 Ion Ratio Lower Upper
 112 100
 64 61.4 51.0 76.4
 63 33.0 27.3 40.9

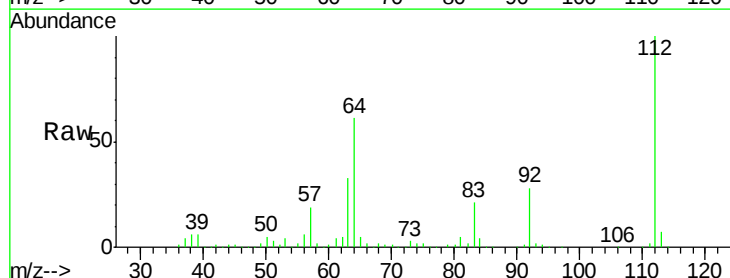

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

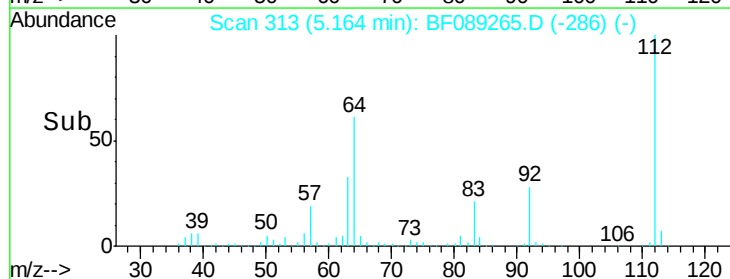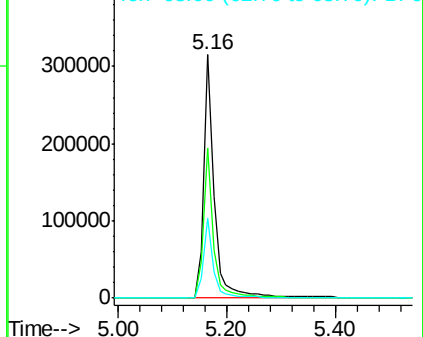

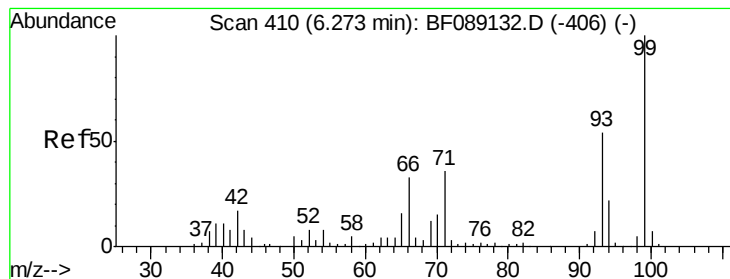

#7

Phenol-d6

Concen: 144.28 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.00 min

Lab File: BF089265.D

Acq: 24 Jul 2016 7:35

Instrument :

BNA_F

ClientSampleId :

KSB-17-8.0-10.0


Tgt Ion: 99 Resp: 572665

Ion Ratio Lower Upper

99 100

42 18.1 13.5 20.3




71 37.9 28.9 43.3

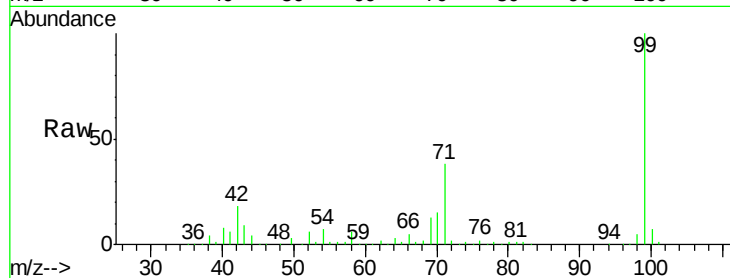

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

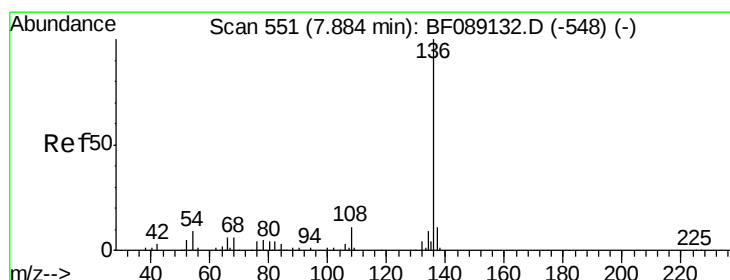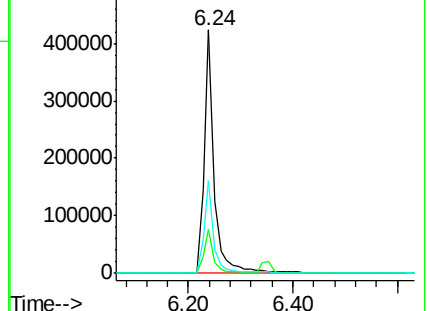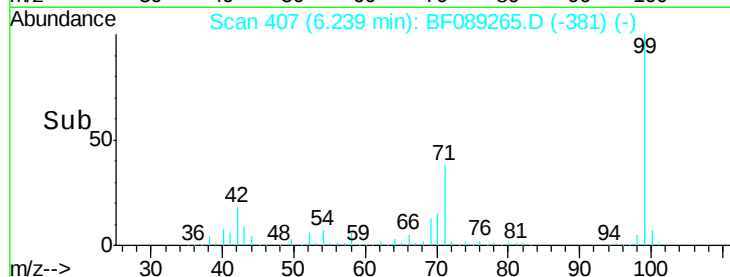

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.01 min

Lab File: BF089265.D

Acq: 24 Jul 2016 7:35

Tgt Ion: 136 Resp: 203994


Ion Ratio Lower Upper

136 100

137 10.9 8.8 13.2

54 7.9 7.0 10.4

68 5.9 5.0 7.6


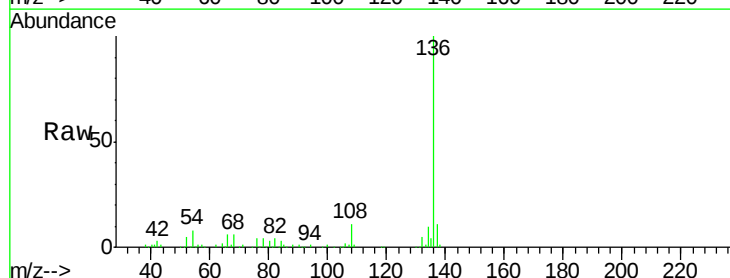



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

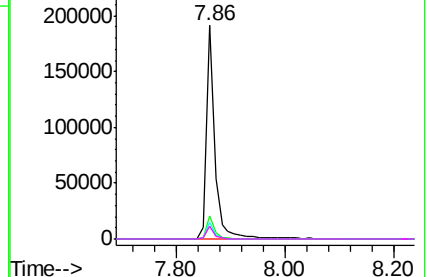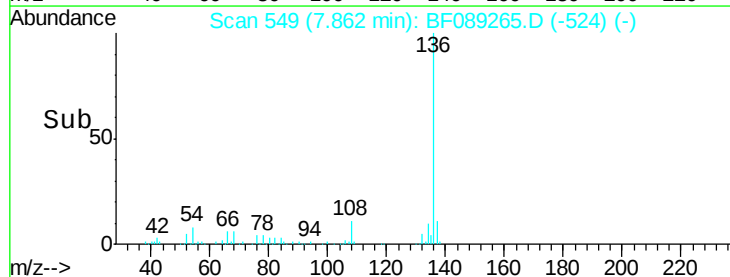


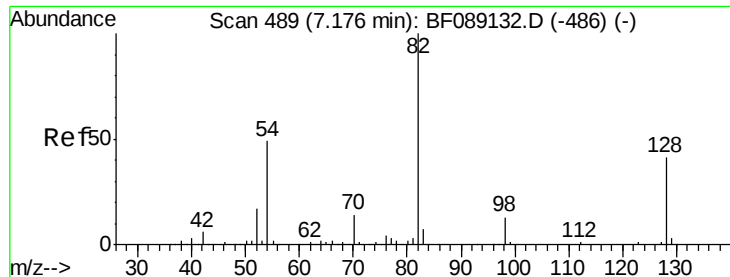




#23
 Nitrobenzene-d5
 Concen: 98.27 ng
 RT: 7.15 min Scan# 487
 Delta R.T. -0.00 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Instrument :
 BNA_F
 ClientSampleId :
 KSB-17-8.0-10.0

Tgt Ion: 82 Resp: 377268
 Ion Ratio Lower Upper
 82 100
 128 43.7 33.0 49.6
 54 46.7 39.0 58.4

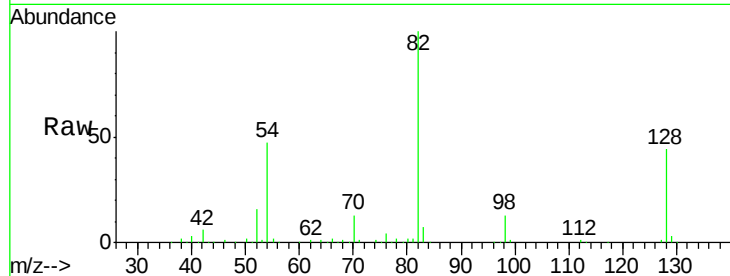


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

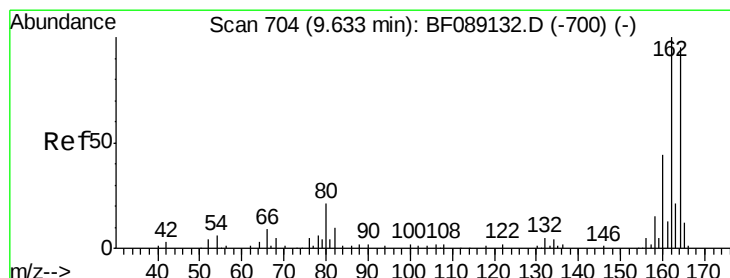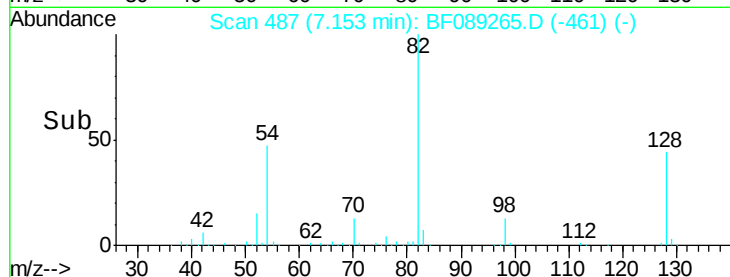
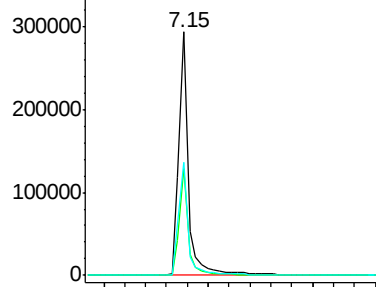



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.00 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Tgt Ion: 164 Resp: 87863
 Ion Ratio Lower Upper
 164 100
 162 106.6 84.1 126.1
 160 47.0 37.1 55.7

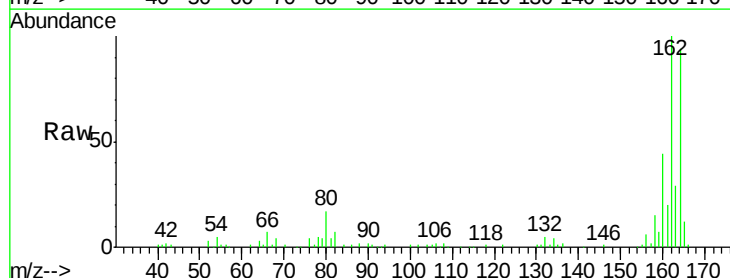

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

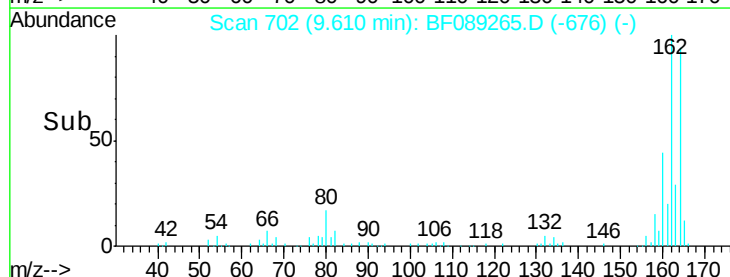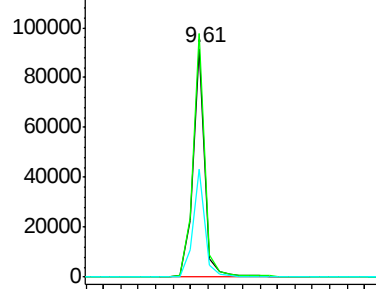


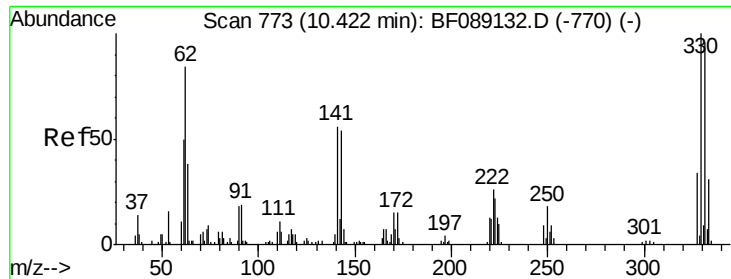




#41
 2,4,6-Tribromophenol
 Concen: 123.64 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.00 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Instrument :
 BNA_F
 ClientSampleId :
 KSB-17-8.0-10.0

Tgt Ion: 330 Resp: 97807
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.2 115.8
 141 47.4 42.2 63.2

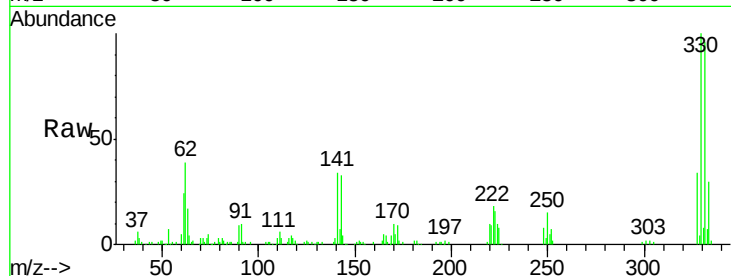


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

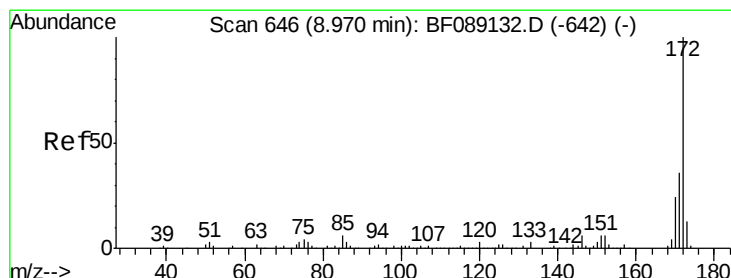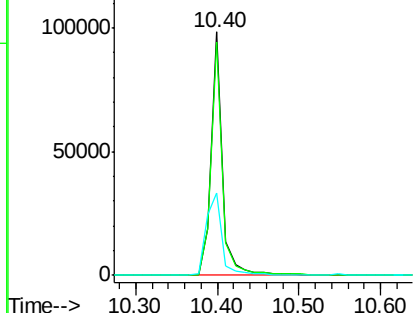
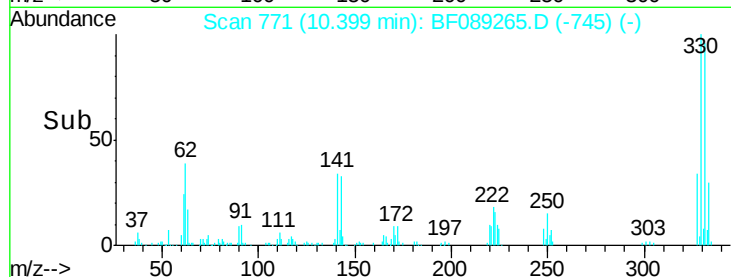



#44
 2-Fluorobiphenyl
 Concen: 92.60 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.00 min
 Lab File: BF089265.D
 Acq: 24 Jul 2016 7:35

Tgt Ion: 172 Resp: 590494
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.2 43.8
 170 23.6 19.1 28.7

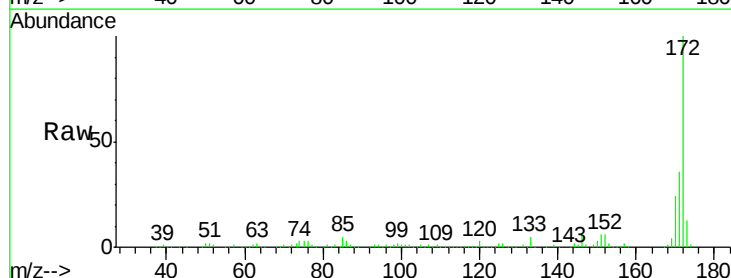

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

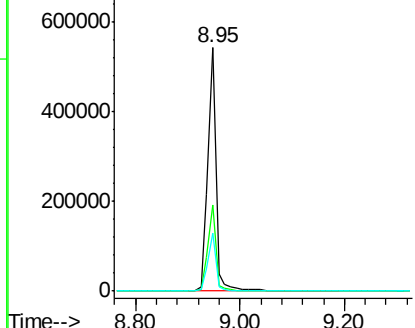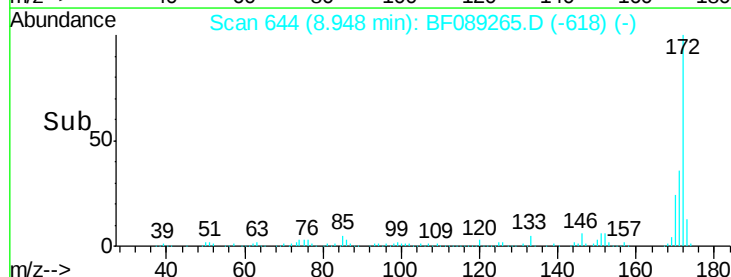


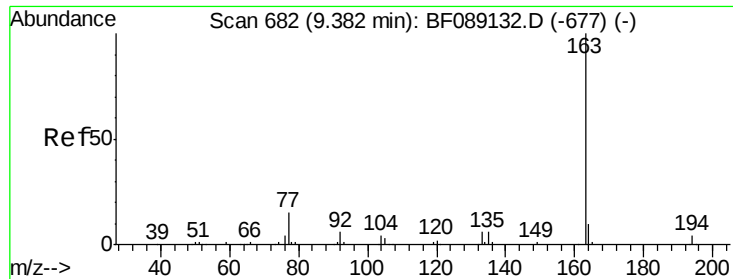




#49
Dimethylphthalate
Concen: 39.94 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.01 min
Lab File: BF089265.D
Acq: 24 Jul 2016 7:35

Instrument :
BNA_F
ClientSampleId :
KSB-17-8.0-10.0

Tgt Ion:163 Resp: 269280
Ion Ratio Lower Upper
163 100
194 3.7 2.9 4.3
164 9.6 7.6 11.4

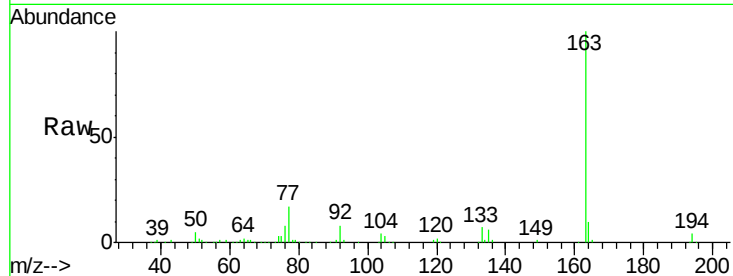


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

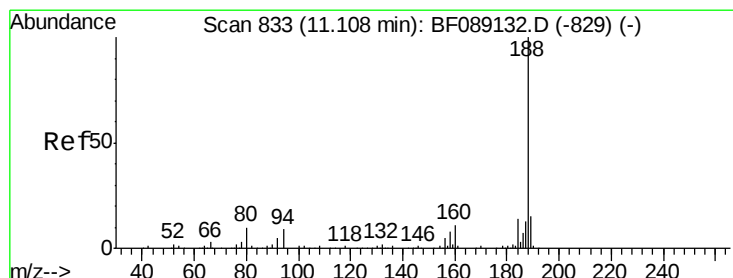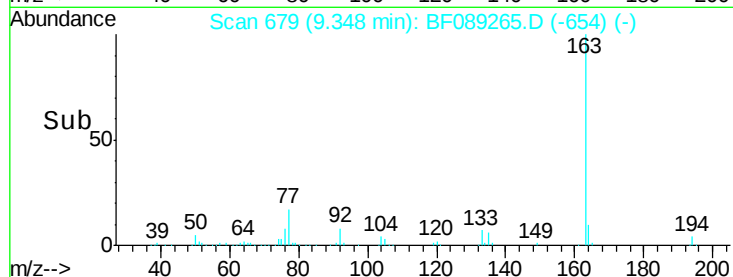
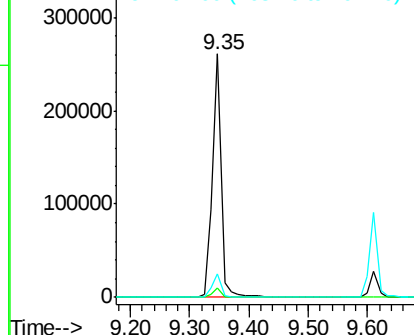



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.08 min Scan# 831
Delta R.T. -0.00 min
Lab File: BF089265.D
Acq: 24 Jul 2016 7:35

Tgt Ion:188 Resp: 139840
Ion Ratio Lower Upper
188 100
94 8.0 7.0 10.4
80 8.7 7.7 11.5

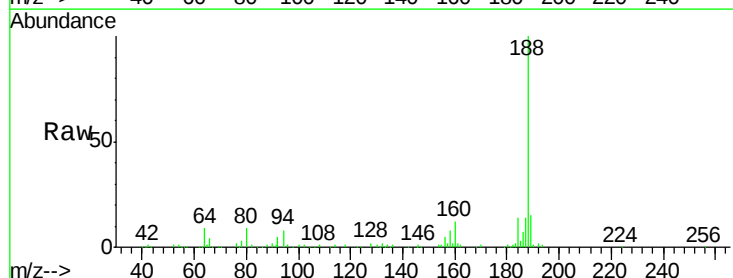

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

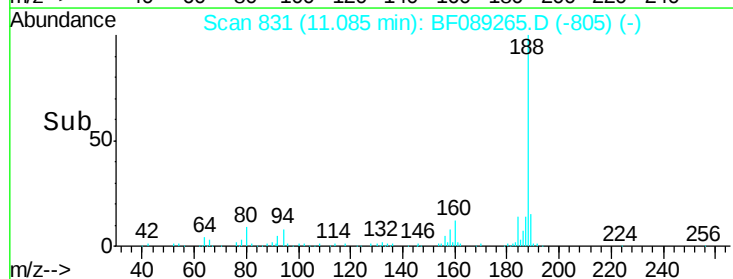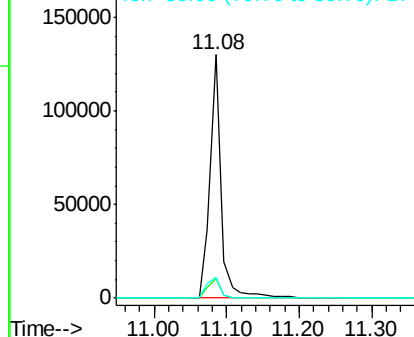

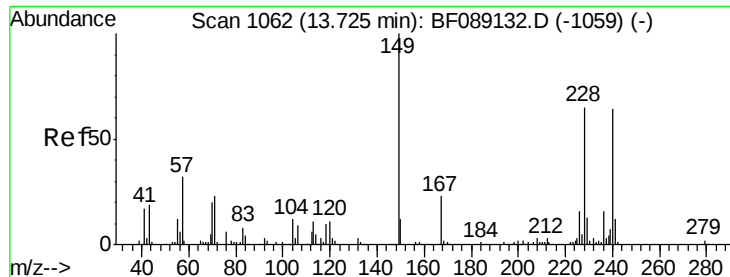

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.70 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BF089265.D

Acq: 24 Jul 2016 7:35

Instrument :

BNA_F

ClientSampleId :

KSB-17-8.0-10.0


Tgt Ion:240 Resp: 92876

Ion Ratio Lower Upper

240 100

120 11.3 13.6 20.4#




236 26.0 20.5 30.7

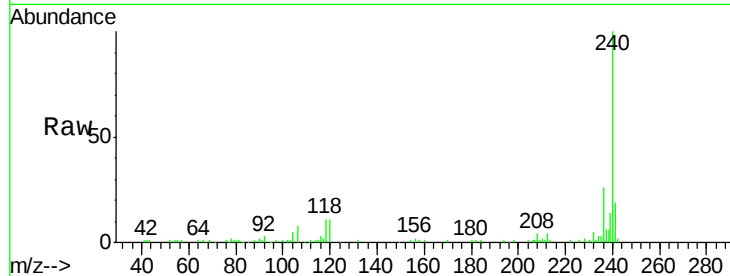

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

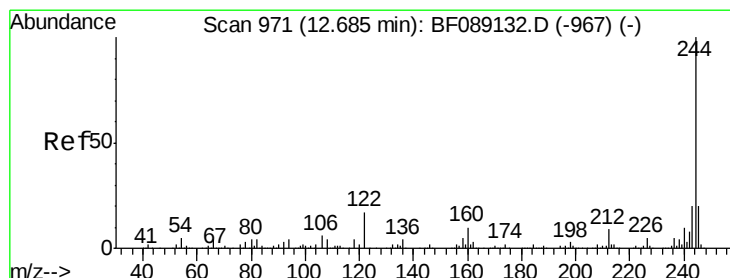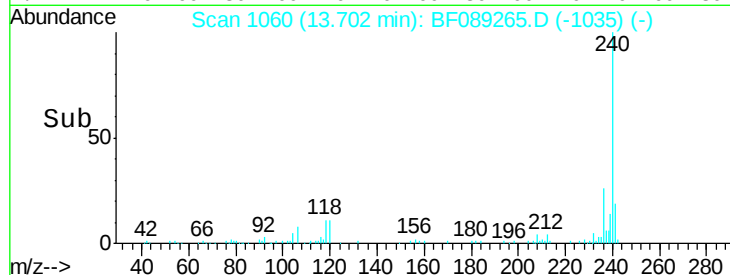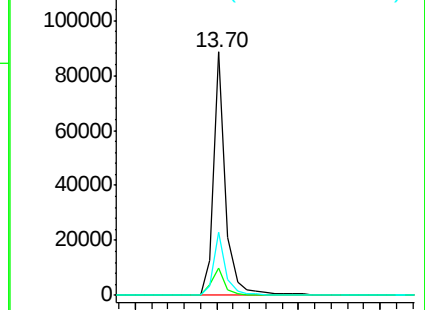

#78

Terphenyl-d14

Concen: 68.63 ng

RT: 12.66 min Scan# 969

Delta R.T. -0.01 min

Lab File: BF089265.D

Acq: 24 Jul 2016 7:35


Tgt Ion:244 Resp: 293872

Ion Ratio Lower Upper

244 100

212 8.4 7.0 10.4



122 17.1 13.8 20.8

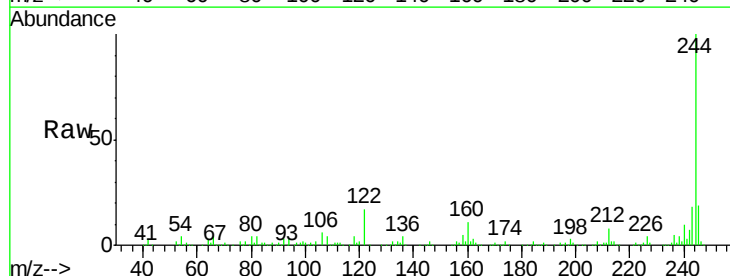


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

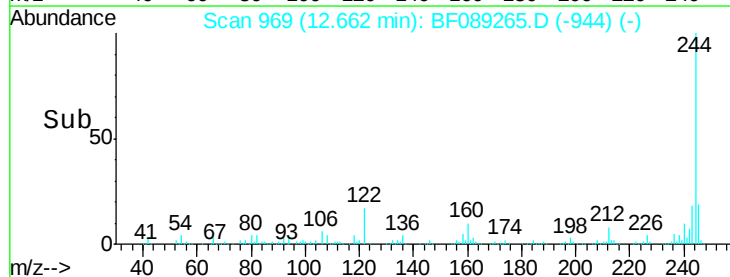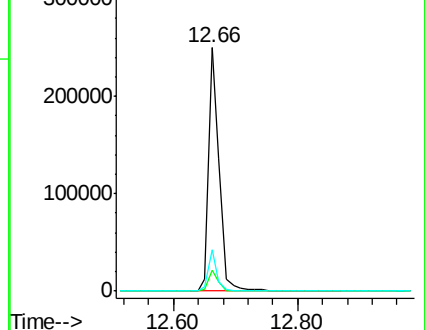

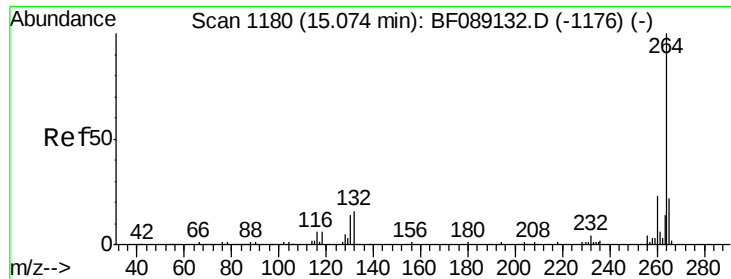

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.05 min Scan# 1178
Delta R.T. -0.00 min
Lab File: BF089265.D
Acq: 24 Jul 2016 7:35

Instrument :
BNA_F
ClientSampleId :
KSB-17-8.0-10.0

Tgt Ion: 264 Resp: 89442
Ion Ratio Lower Upper
264 100
260 23.8 18.5 27.7
265 21.2 17.3 25.9

