

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
 Data File : BF089225.D
 Acq On : 23 Jul 2016 8:53
 Operator : UM/SJ
 Sample : H4121-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-MW1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.713	10	11	61	rVB	791269	1703557	89.43%	13.590%
2	4.684	270	271	277	rBV	12467	22863	1.20%	0.182%
3	5.153	310	312	333	rBV4	282346	471442	24.75%	3.761%
4	6.227	405	406	414	rBV	182563	301873	15.85%	2.408%
5	6.342	414	416	435	rVB	854192	1031503	54.15%	8.229%
6	6.582	435	437	448	rBV	186154	259771	13.64%	2.072%
7	6.730	448	450	460	rVB	978064	1057147	55.50%	8.433%
8	7.153	484	487	505	rBV	741181	1002060	52.61%	7.994%
9	7.862	547	549	560	rBV	361750	395823	20.78%	3.158%
10	8.948	641	644	646	rBV	1625761	1904825	100.00%	15.195%
11	9.348	677	679	684	rVB	18954	26536	1.39%	0.212%
12	9.611	699	702	704	rBV	426248	439483	23.07%	3.506%
13	9.999	734	736	743	rBB	29298	36084	1.89%	0.288%
14	10.399	768	771	781	rVB	722852	954656	50.12%	7.616%
15	11.085	829	831	835	rBV	405622	444248	23.32%	3.544%
16	11.439	861	862	865	rVB	26261	27192	1.43%	0.217%
17	12.056	914	916	921	rBB2	22276	34791	1.83%	0.278%
18	12.502	953	955	958	rBV	25325	29572	1.55%	0.236%
19	12.674	967	970	972	rBV	1157917	1675311	87.95%	13.364%
20	13.211	1015	1017	1019	rBV	21633	21880	1.15%	0.175%
21	13.702	1058	1060	1075	rBV	391767	411747	21.62%	3.285%
22	15.040	1175	1177	1181	rBV	195398	283174	14.87%	2.259%


Sum of corrected areas: 12535538

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089225.D
Acq On : 23 Jul 2016 8:53
Operator : UM/SJ
Sample : H4121-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-MW1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

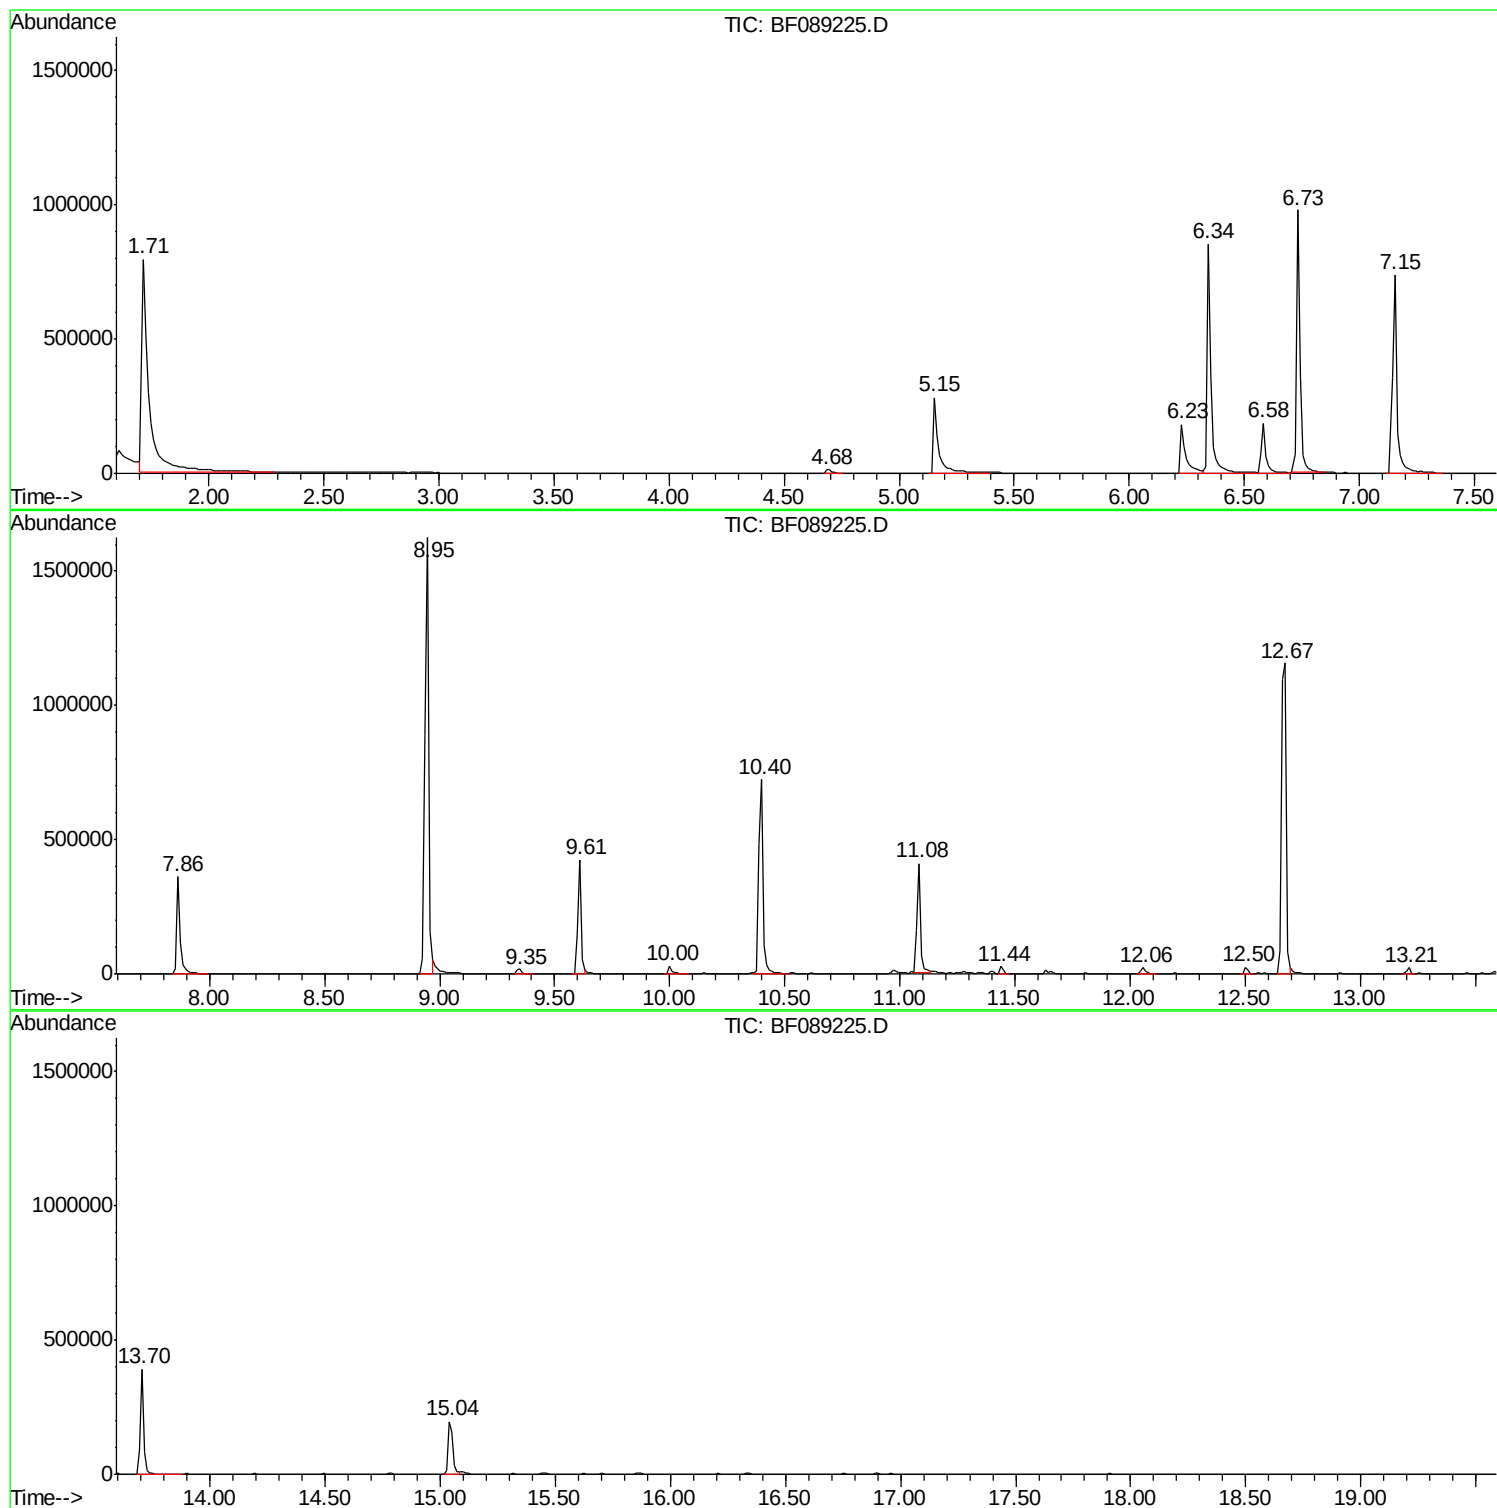

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089225.D
Acq On : 23 Jul 2016 8:53
Operator : UM/SJ
Sample : H4121-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-MW1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.34 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.34	79.42 ng	1031500	1,4-Dichlorobenzene-d4	6.58

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	14
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

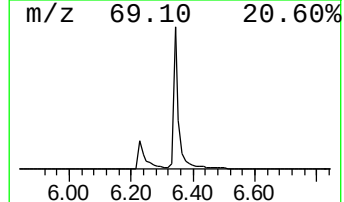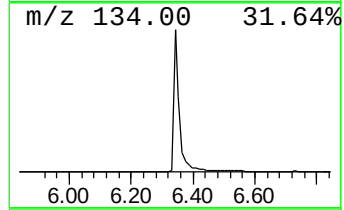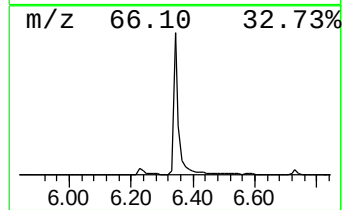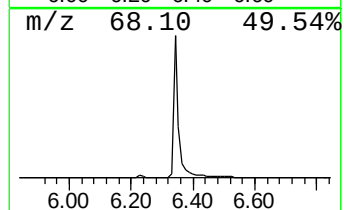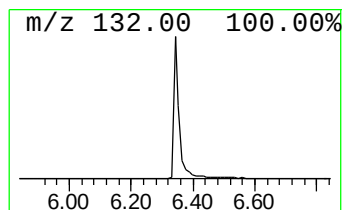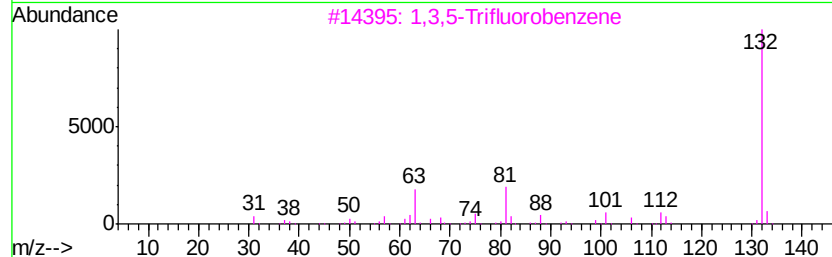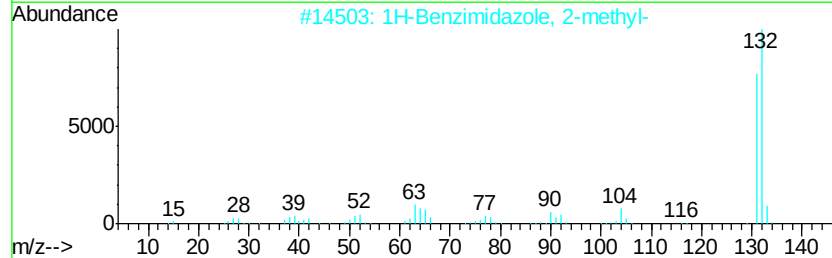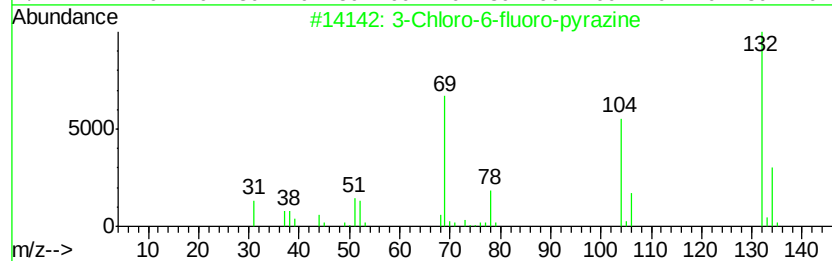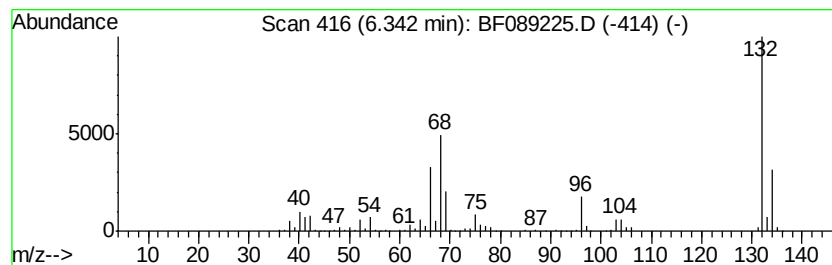

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072316\
Data File : BF089225.D
Acq On : 23 Jul 2016 8:53
Operator : UM/SJ
Sample : H4121-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-MW1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.34	6.34	79.4	ng	1031500	1	6.58	259771	20.0