
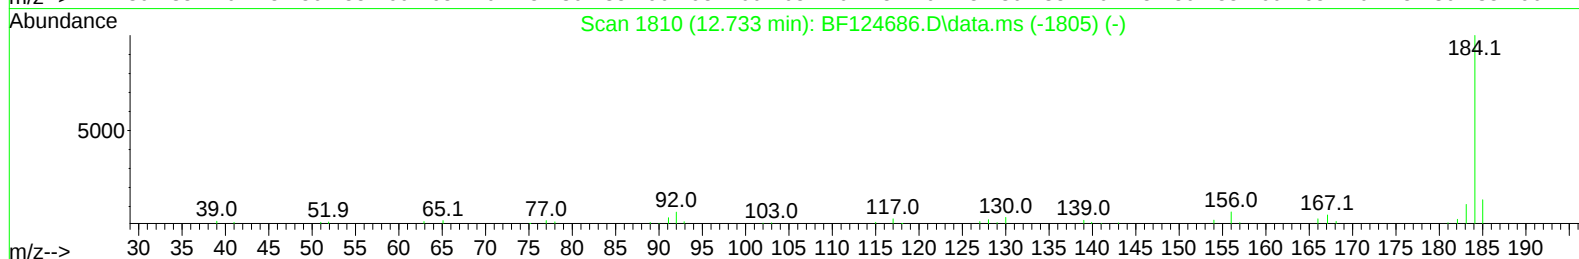
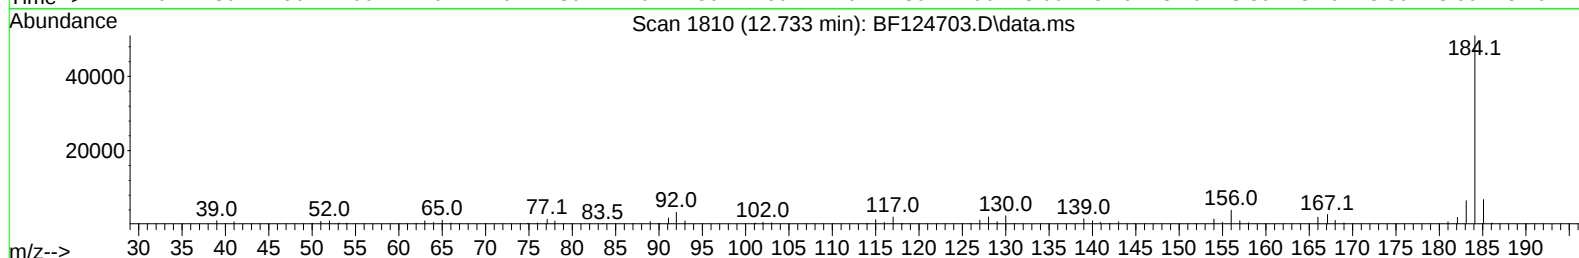


Quant Time: Jul 23 11:39:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

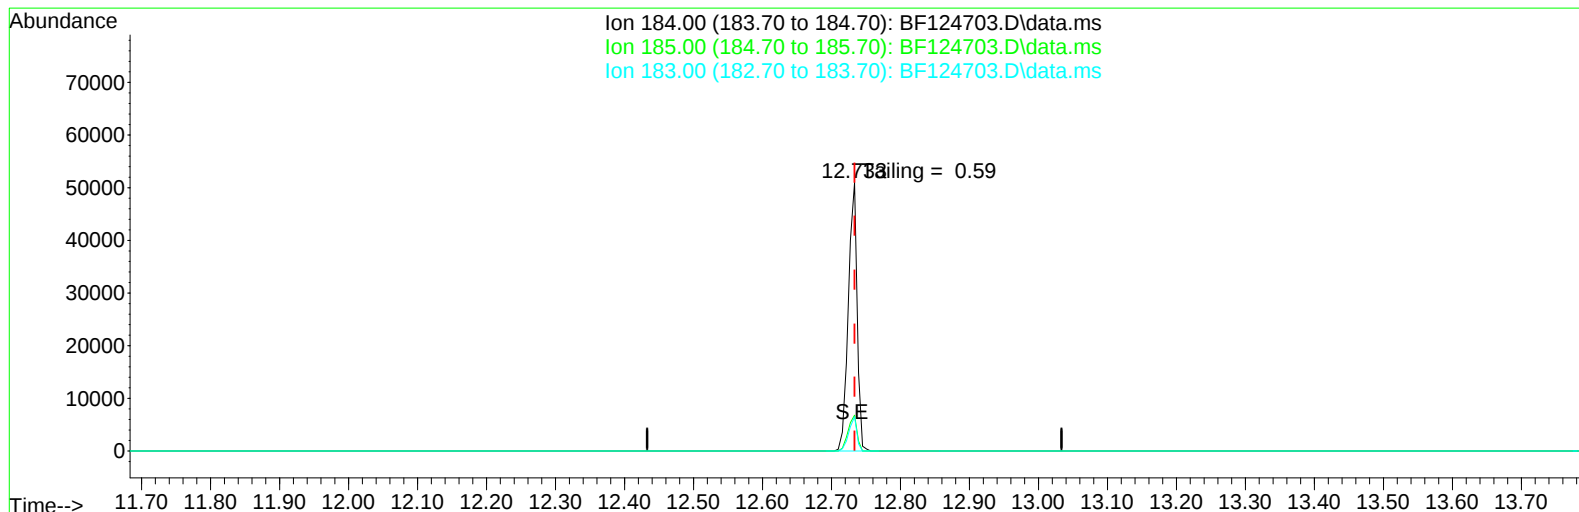

TIC: BF124703.D\data.ms

(77) Benzidine




12.733min (+ 0.000) 0.00 ng

response **45096**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.36
183.00	10.10	12.79#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
Data File : BF124703.D
Acq On : 23 Jul 2021 8:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 11:39:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

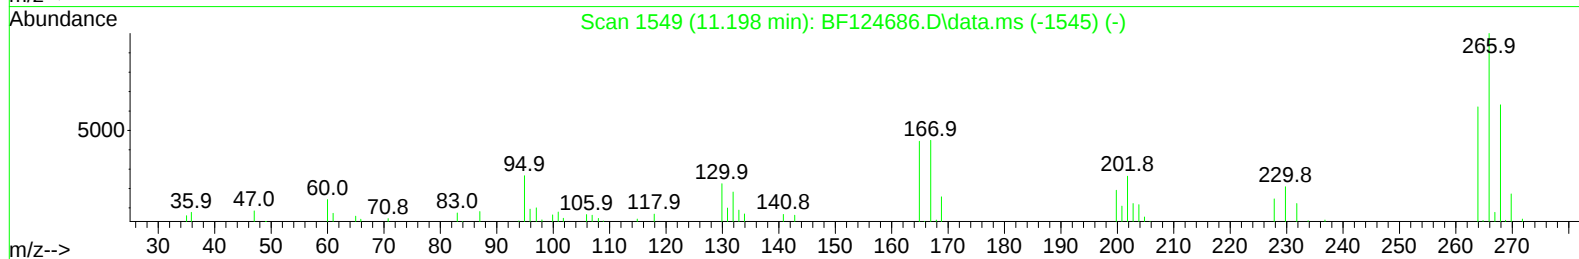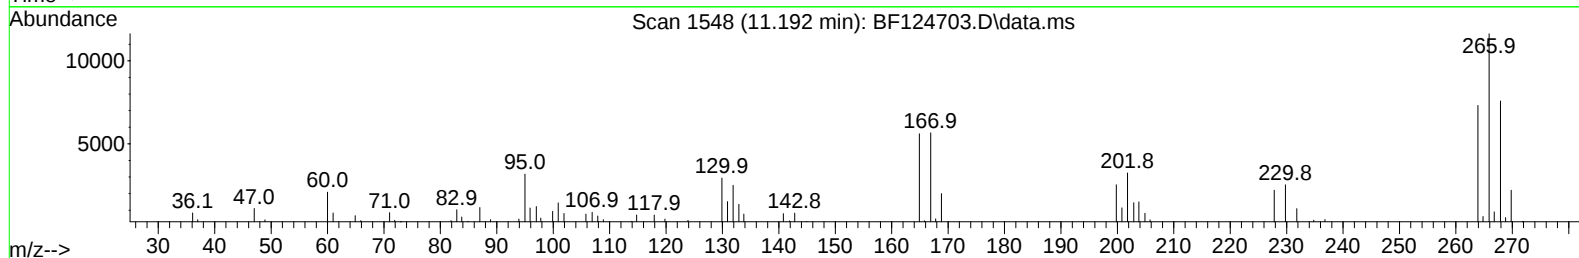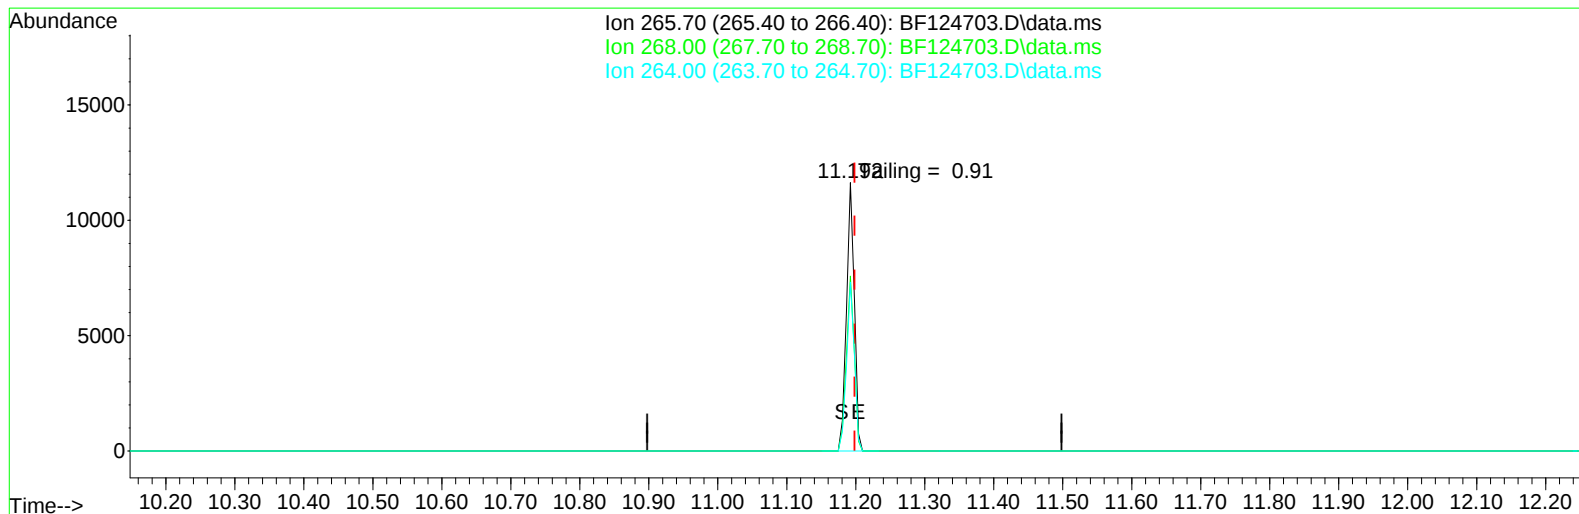

TIC: BF124703.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 0.00 ng

response 9216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.15
264.00	69.90	62.89
0.00	0.00	0.00