
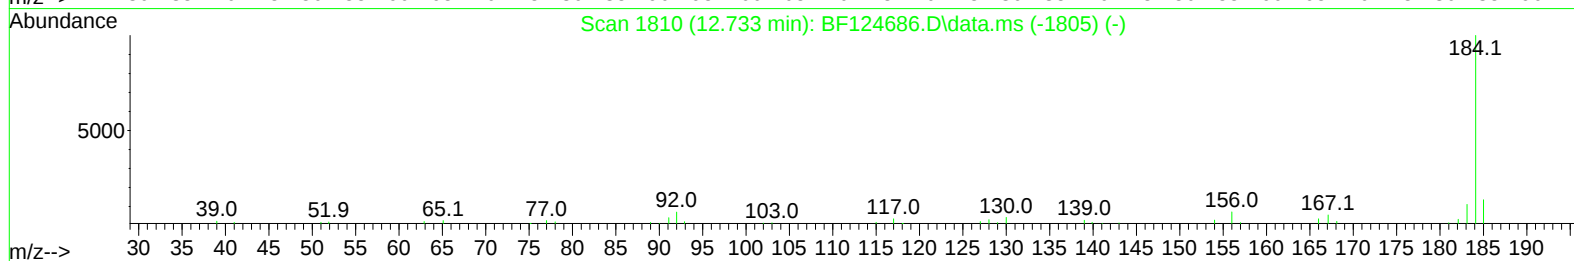
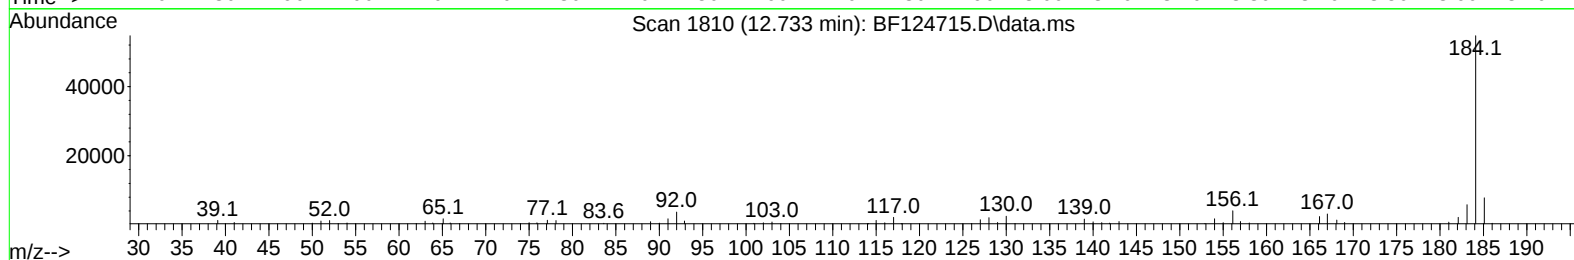


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
Data File : BF124715.D
Acq On : 23 Jul 2021 16:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 16:51:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

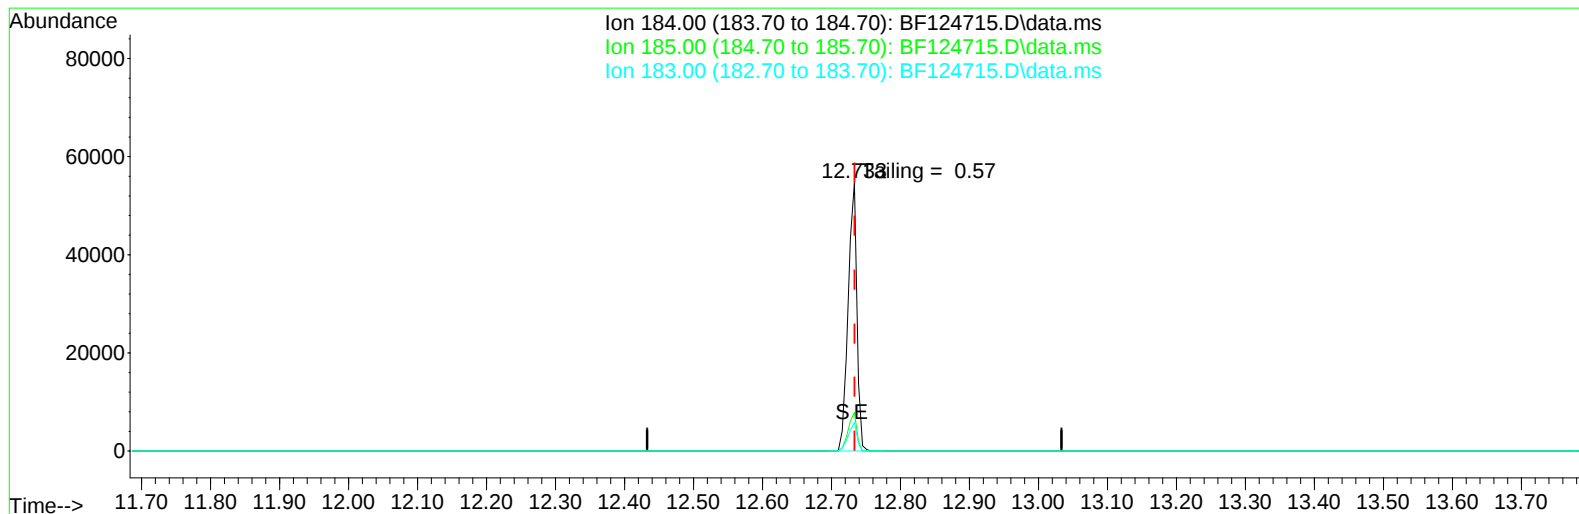

TIC: BF124715.D\data.ms

(77) Benzidine




12.733min (-0.000) 0.00 ng

response 48060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.30
183.00	10.10	10.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
Data File : BF124715.D
Acq On : 23 Jul 2021 16:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 16:51:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

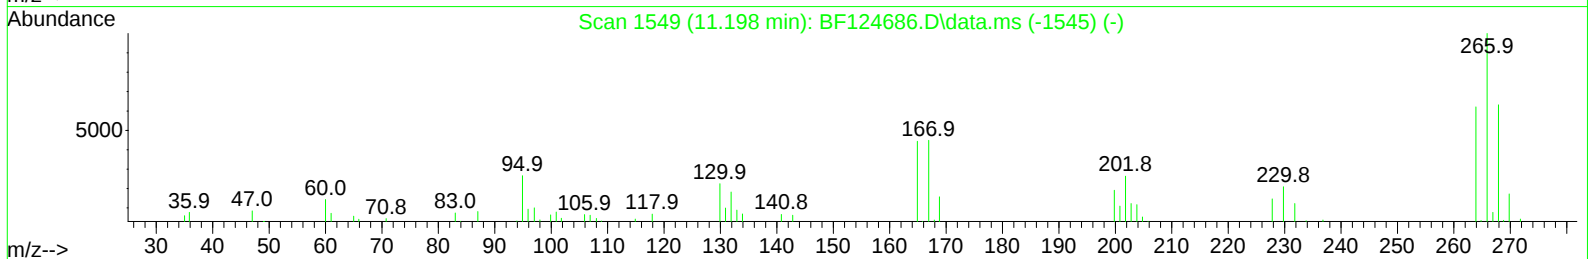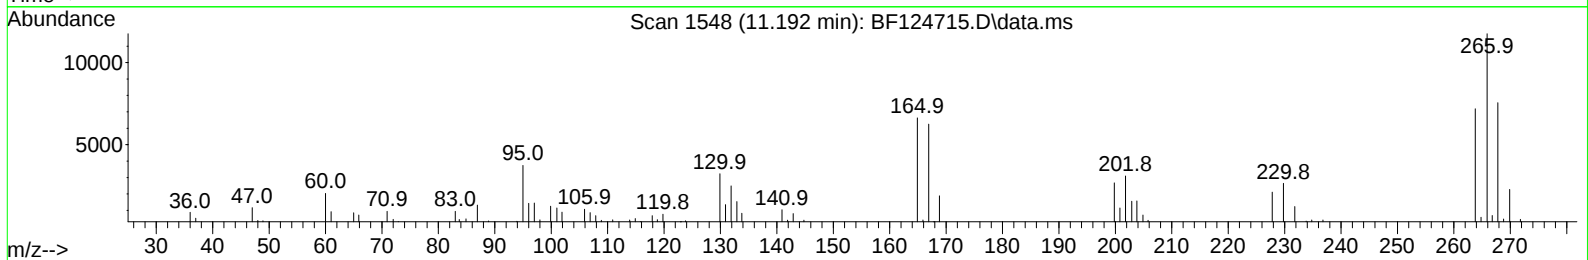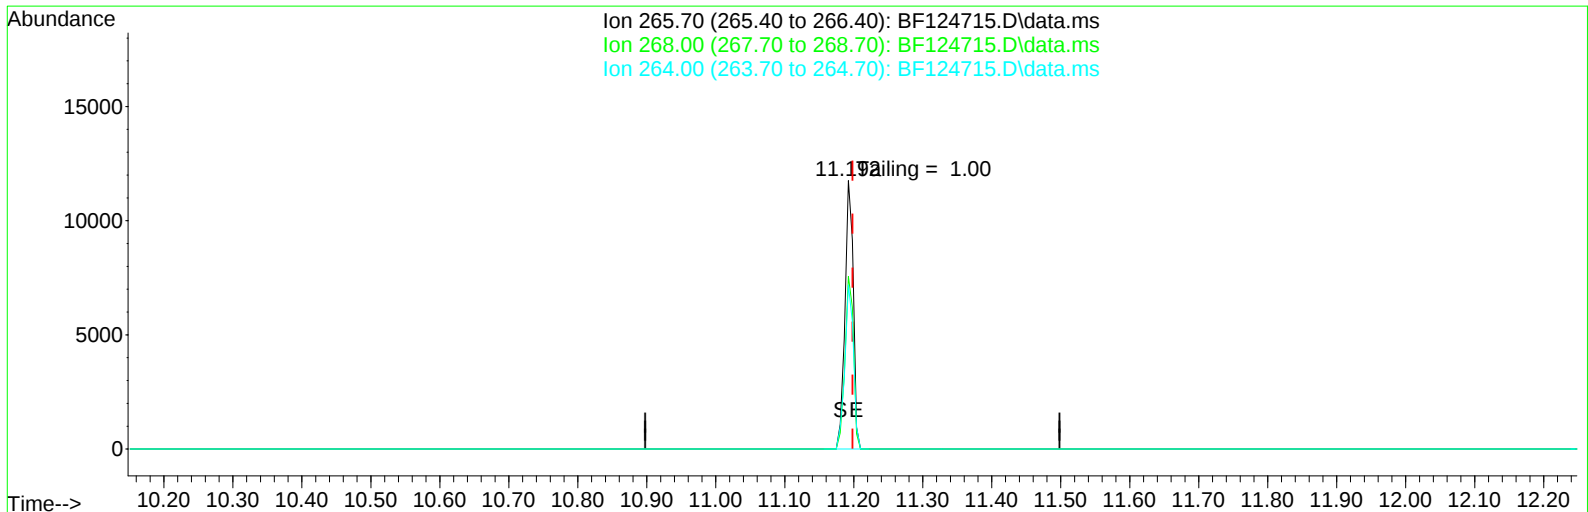

TIC: BF124715.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 0.00 ng

response 9791

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.30
264.00	69.90	61.13
0.00	0.00	0.00