


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
 Data File : BF124703.D
 Acq On : 23 Jul 2021 8:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

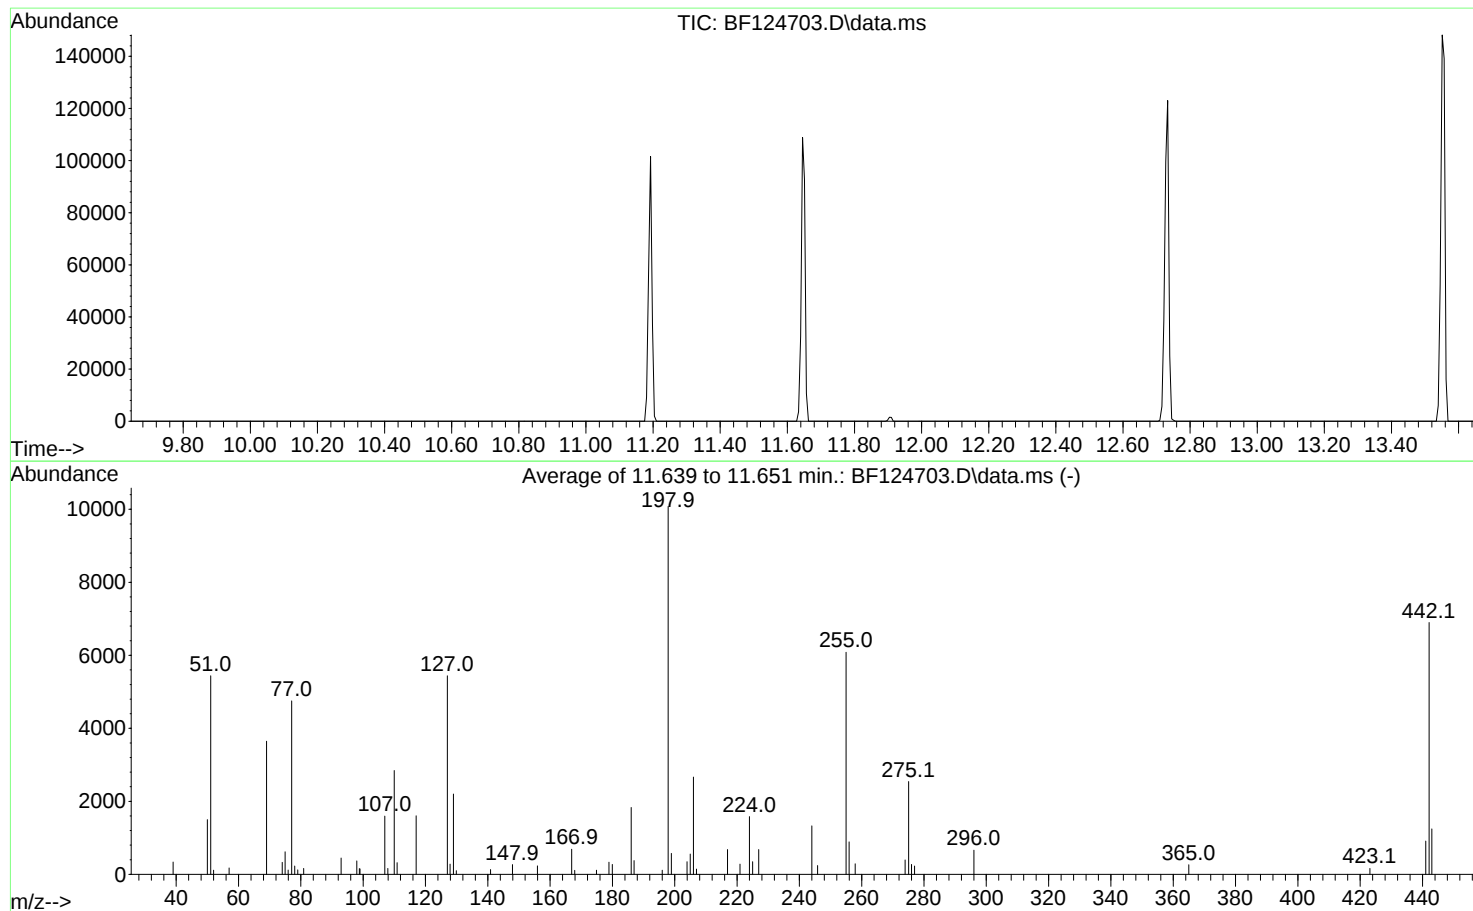

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	5441	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	3646	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	5441	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10076	PASS
199	198	5	9	5.7	573	PASS
275	198	10	60	25.2	2542	PASS
365	198	1	100	2.6	265	PASS
441	198	0.01	100	9.1	912	PASS
442	442	50	100	100.0	6899	PASS
443	442	15	24	18.1	1247	PASS

DDT Breakdown




Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
7/23/2021	BNA_F	<u>BF124703.D</u>
Compound Name	Response	Retention Time
DDT	26130	13.55
DDD	0	13.25
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	26130	0.00


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
Data File : BF124703.D
Acq On    : 23 Jul 2021    8:31
Operator  : JU/CG
Sample    : DFTPP
Misc      :
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 23 11:39:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

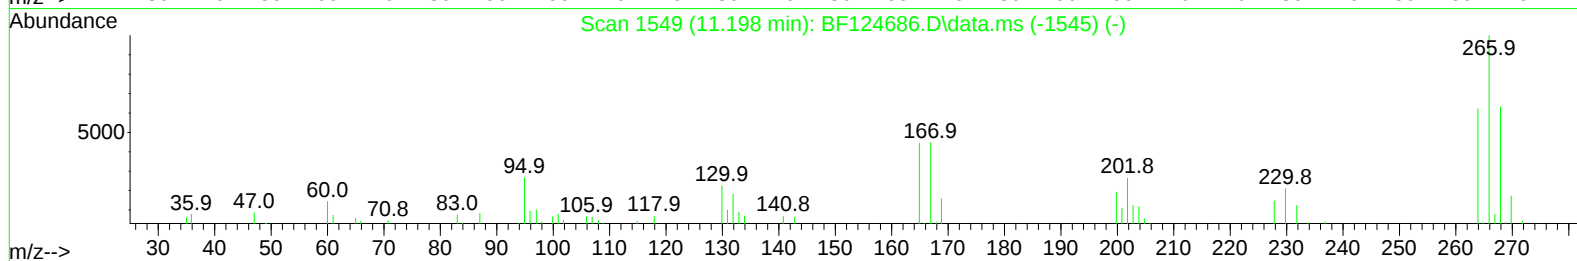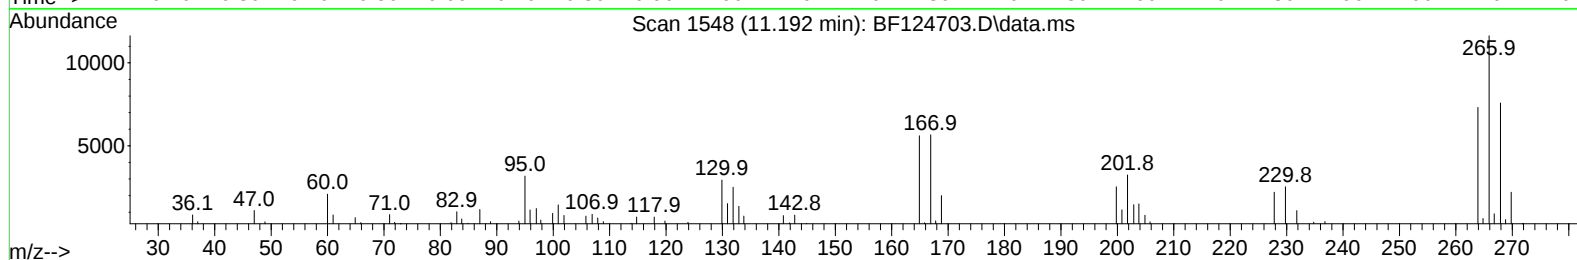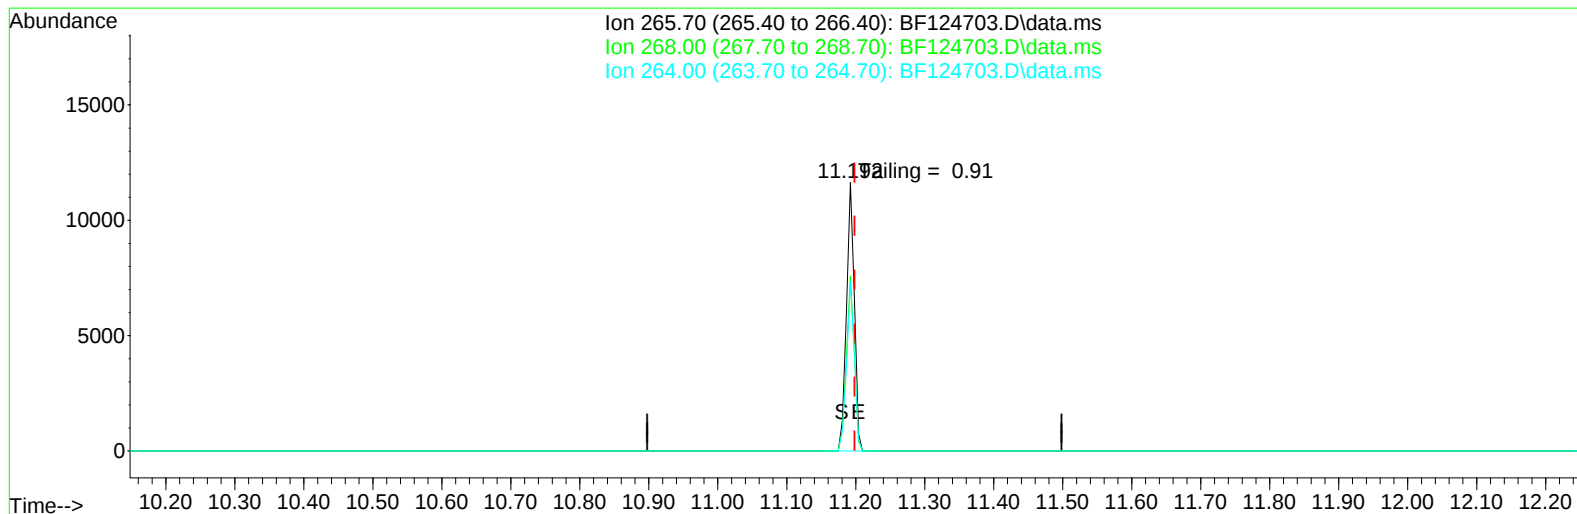

TIC: BF124703.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 0.00 ng

response	9216
----------	------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.15
264.00	69.90	62.89
0.00	0.00	0.00