
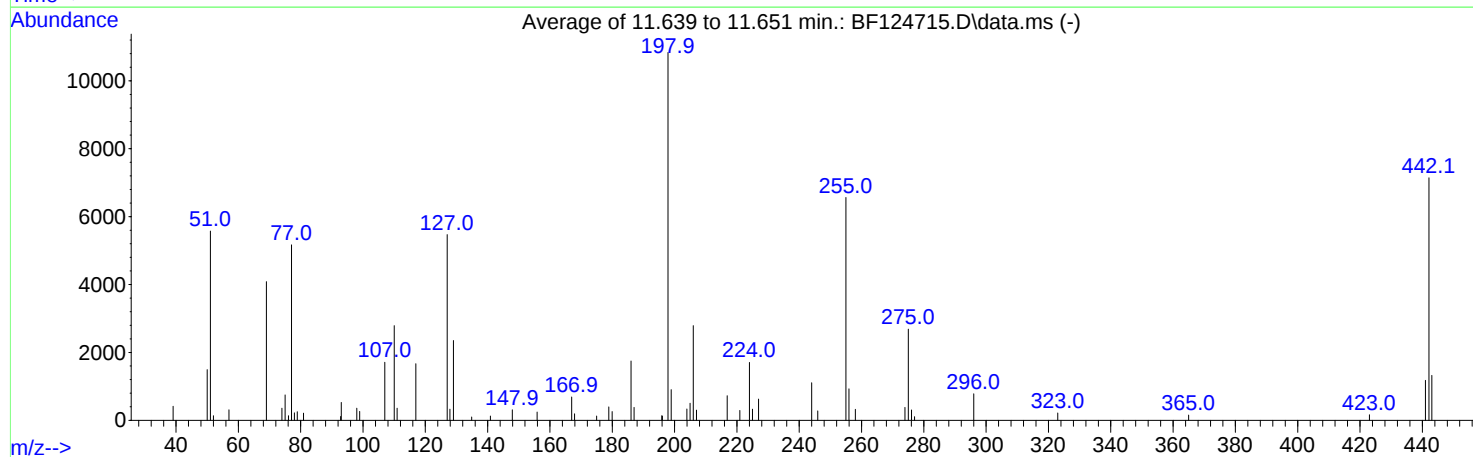


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
 Data File : BF124715.D
 Acq On : 23 Jul 2021 16:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

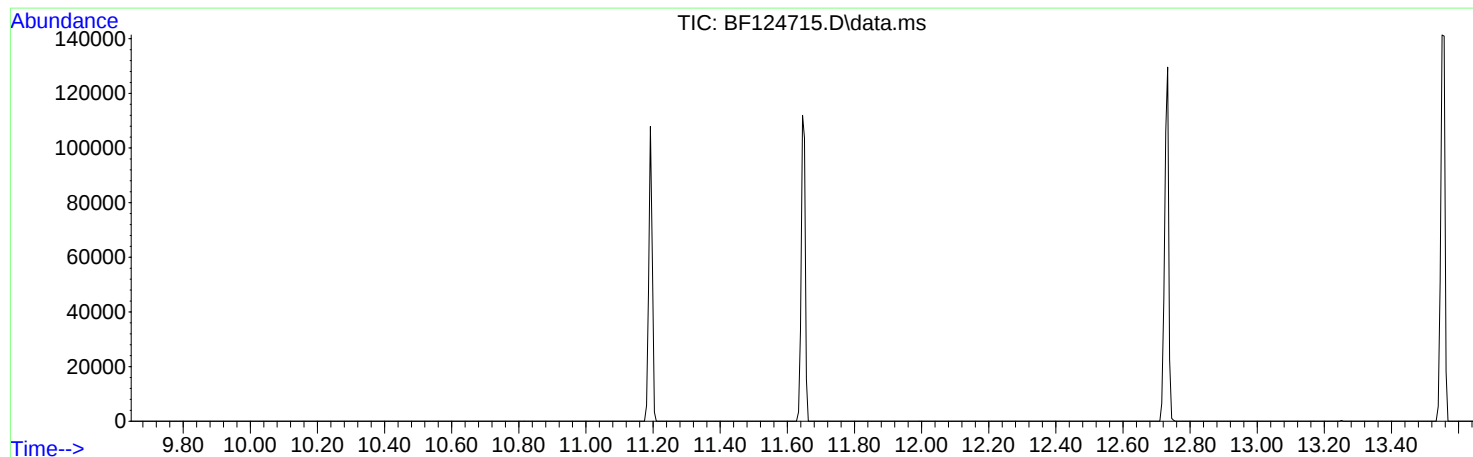




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	5576	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.7	4087	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	5473	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10833	PASS
199	198	5	9	8.3	904	PASS
275	198	10	60	24.8	2687	PASS
365	198	1	100	1.4	156	PASS
441	198	0.01	100	10.9	1179	PASS
442	442	50	100	100.0	7144	PASS
443	442	15	24	18.5	1324	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\
 Data File : BF124715.D
 Acq On : 23 Jul 2021 16:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 23 16:51:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 15:28:57 2021
 Response via : Initial Calibration

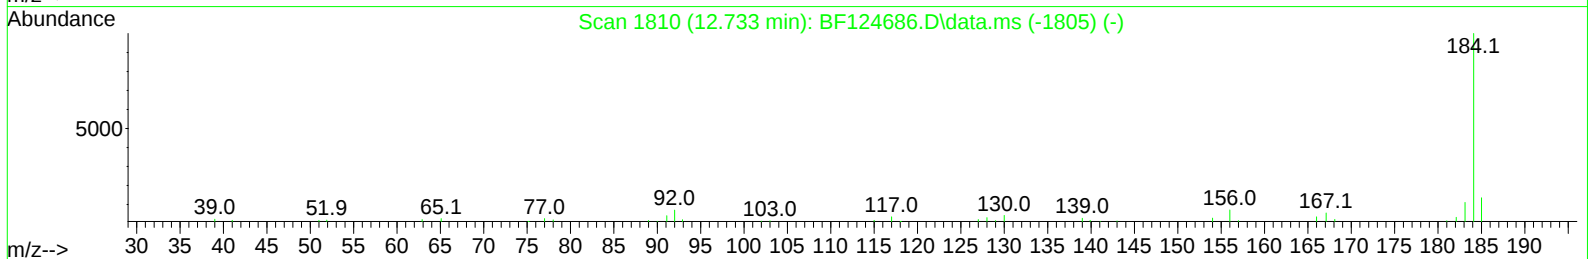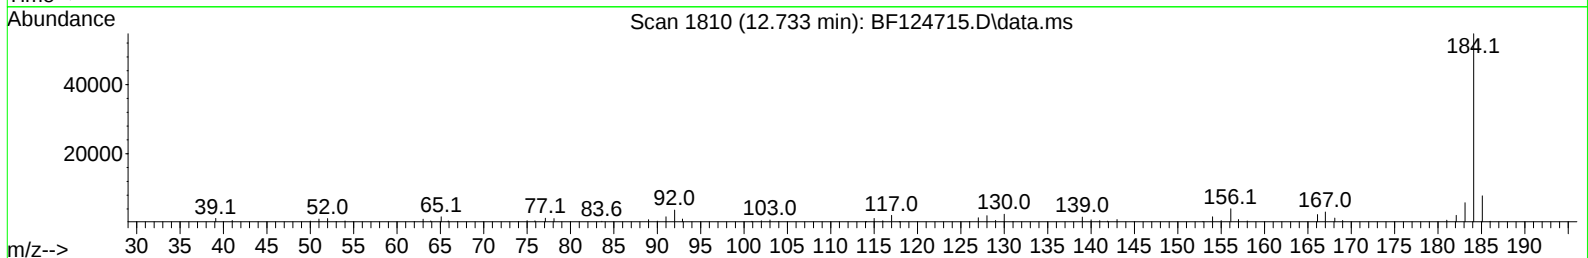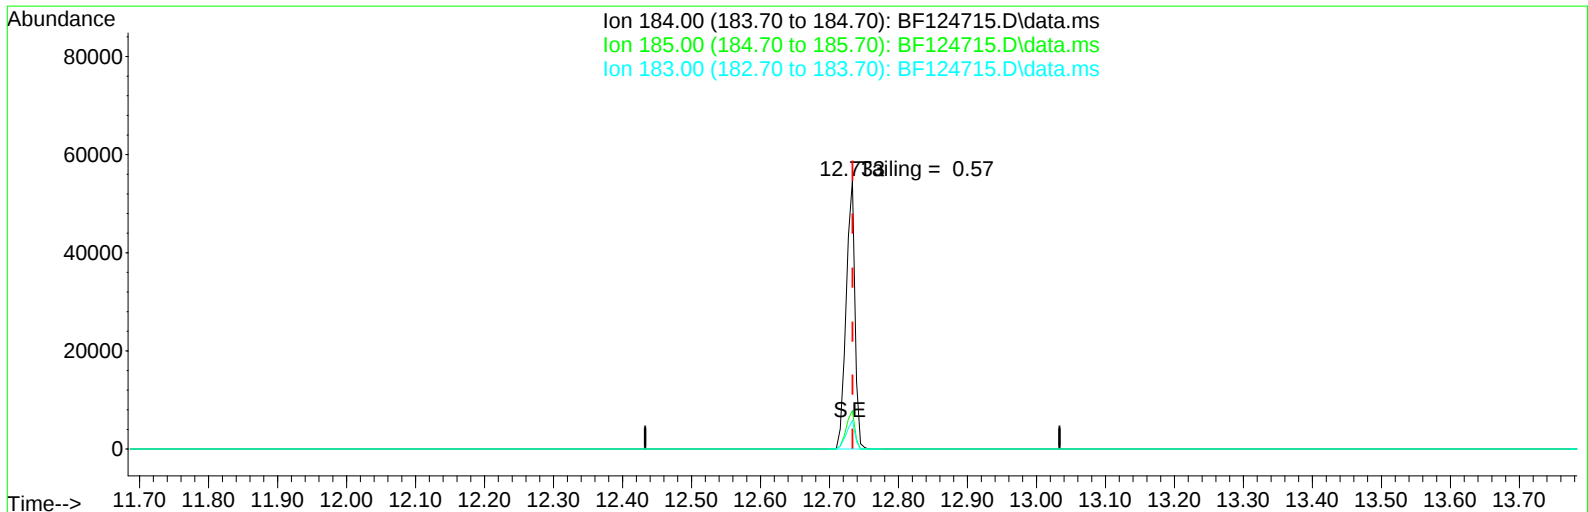

TIC: BF124715.D\data.ms

(77) Benzidine

12.733min (-0.000) 0.00 ng




response 48060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.30
183.00	10.10	10.68
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072321\  
Data File : BF124715.D  
Acq On    : 23 Jul 2021  16:12  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 23 16:51:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

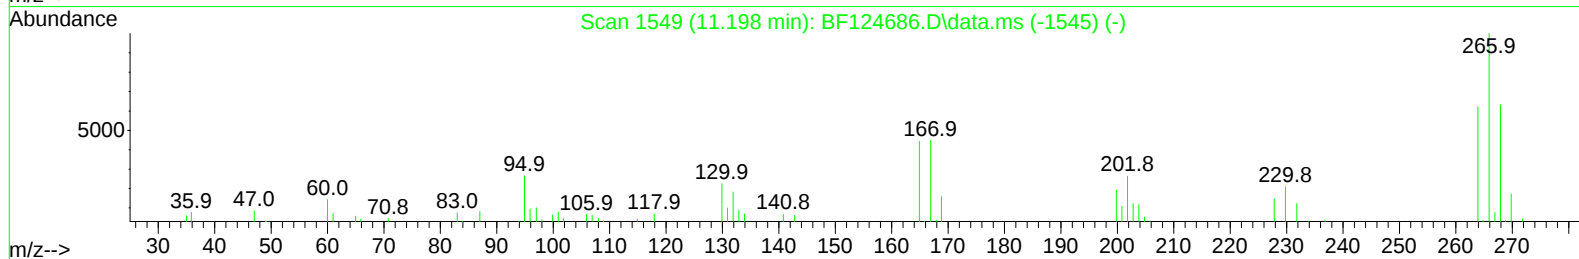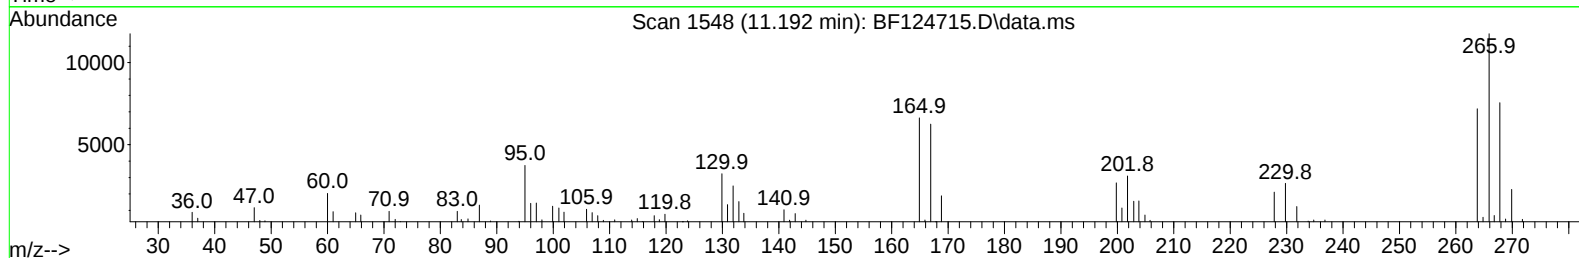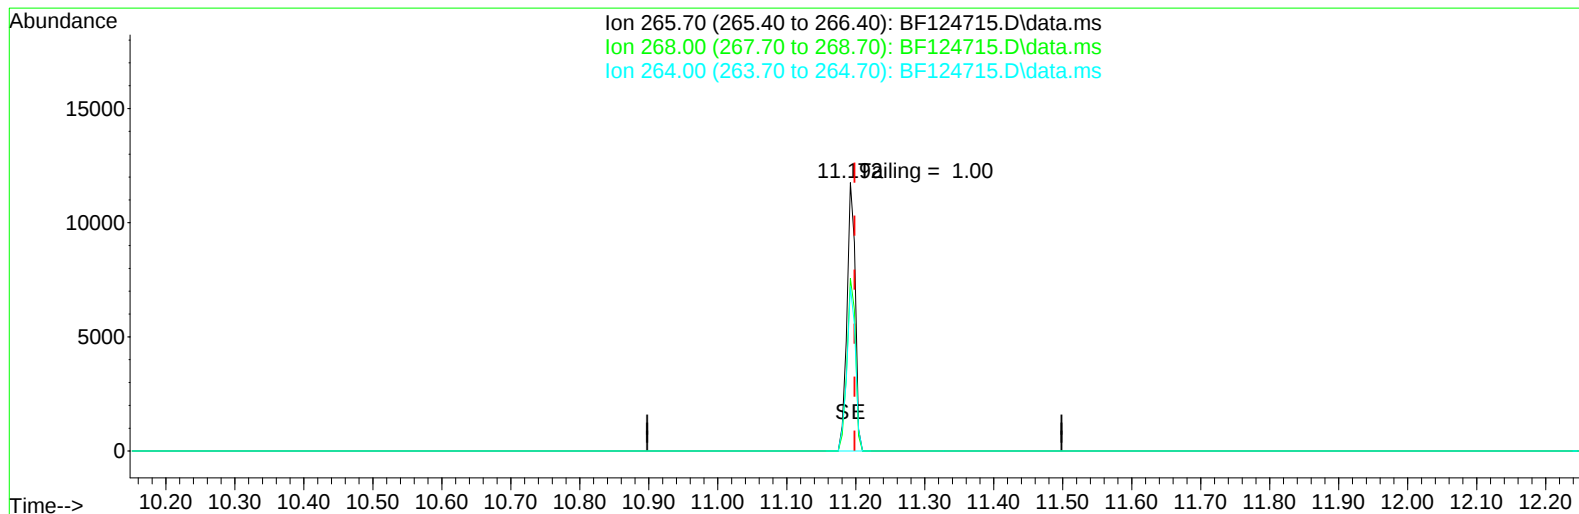

TIC: BF124715.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 0.00 ng

response 9791

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.30
264.00	69.90	61.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/23/2021	BNA_F	BF124715.D
Compound Name	Response	Retention Time
DDT	26176	13.55
DDD	112	13.25
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
112	26288	0.43

Instrument :
BNA_F
ClientSampleId :
DFTPP