
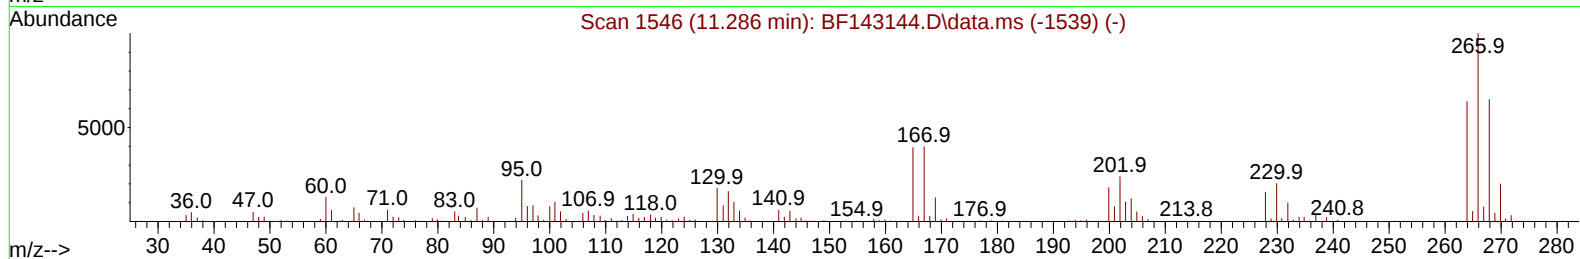
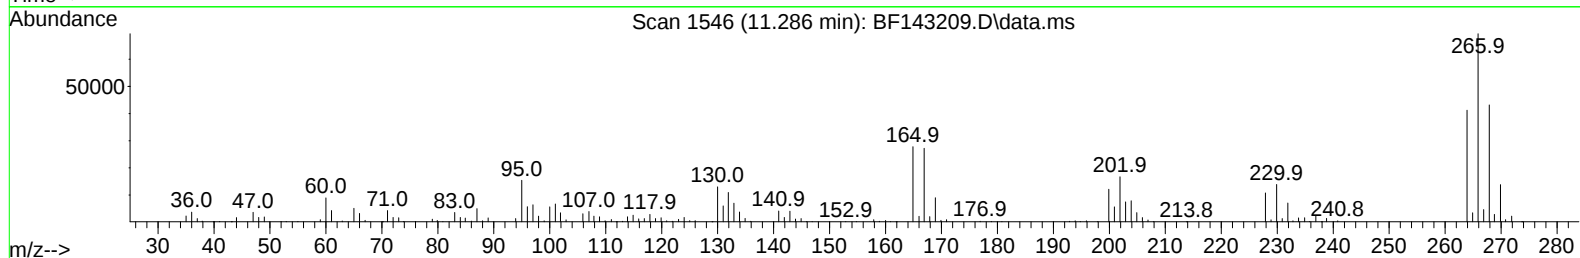


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072325\
Data File : BF143209.D
Acq On : 23 Jul 2025 13:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 15:17:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

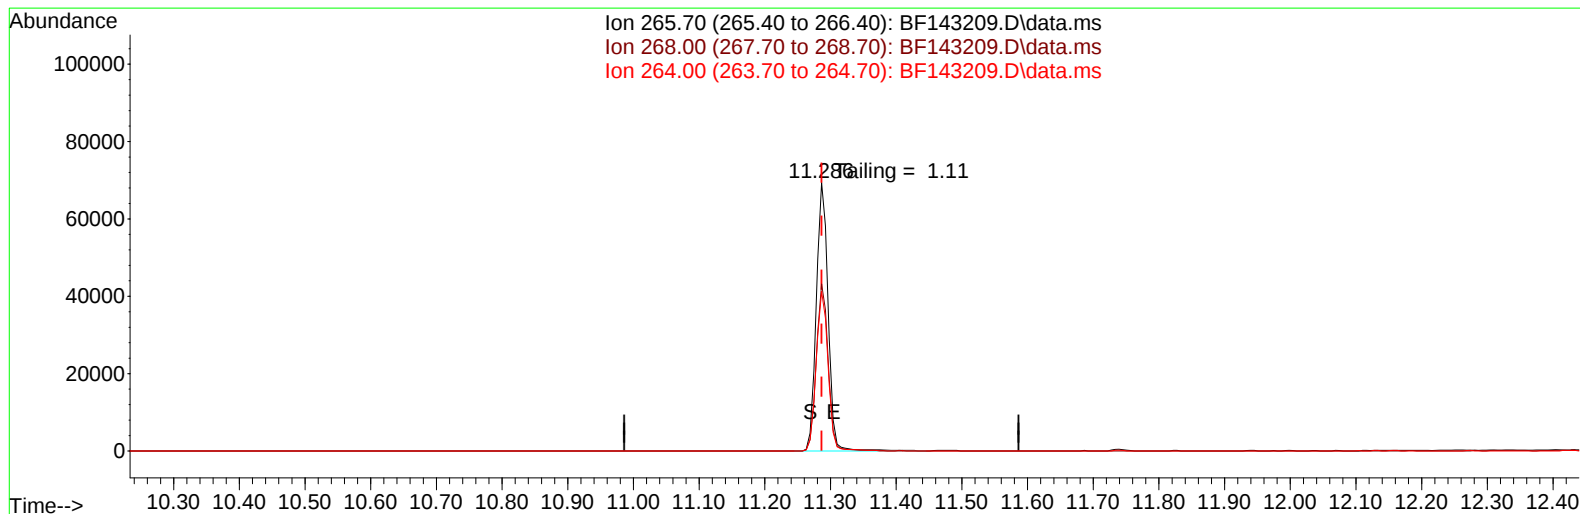

TIC: BF143209.D\data.ms

(70) Pentachlorophenol (C)




11.286min (+ 0.000) 14501.34 ng

response 87636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.26
264.00	63.80	59.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072325\
Data File : BF143209.D
Acq On : 23 Jul 2025 13:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 15:17:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

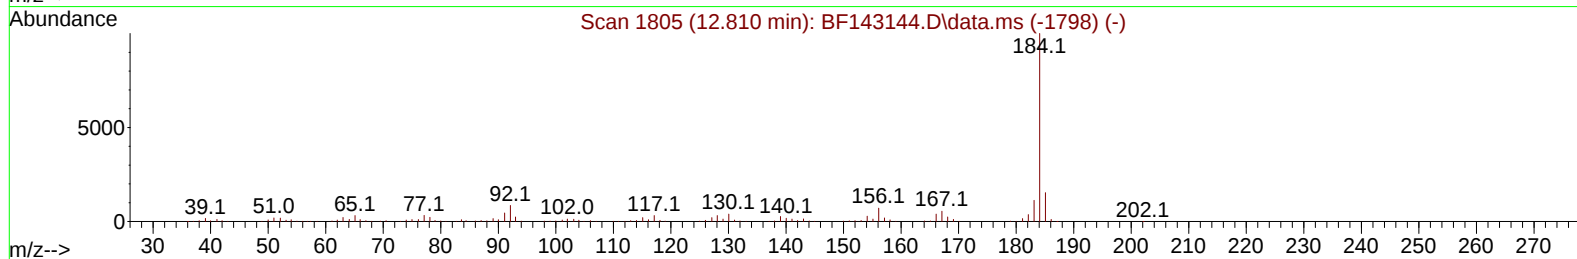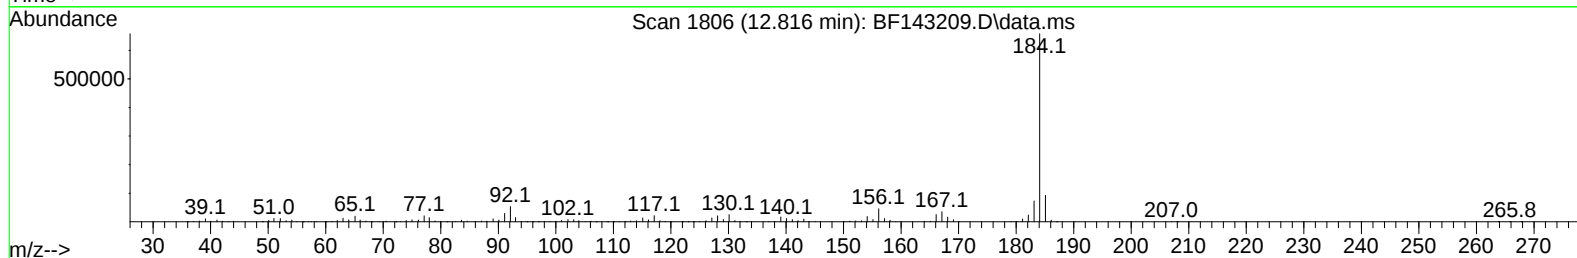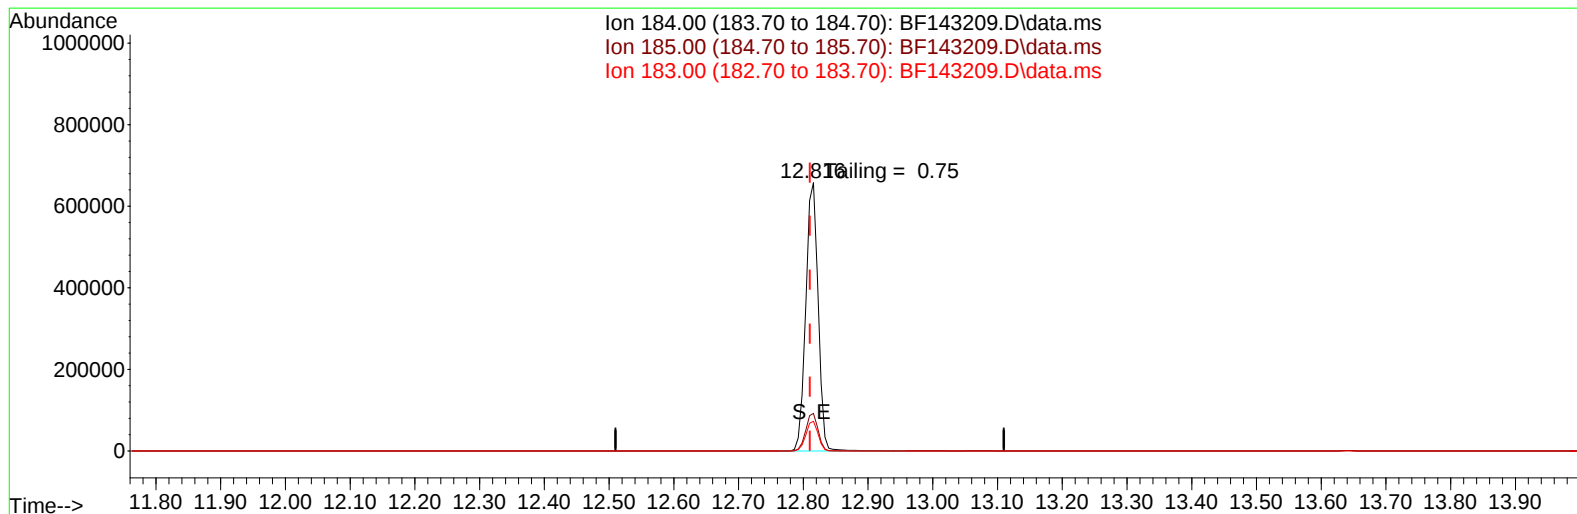

TIC: BF143209.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 876486

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.03
183.00	11.20	11.13
0.00	0.00	0.00