
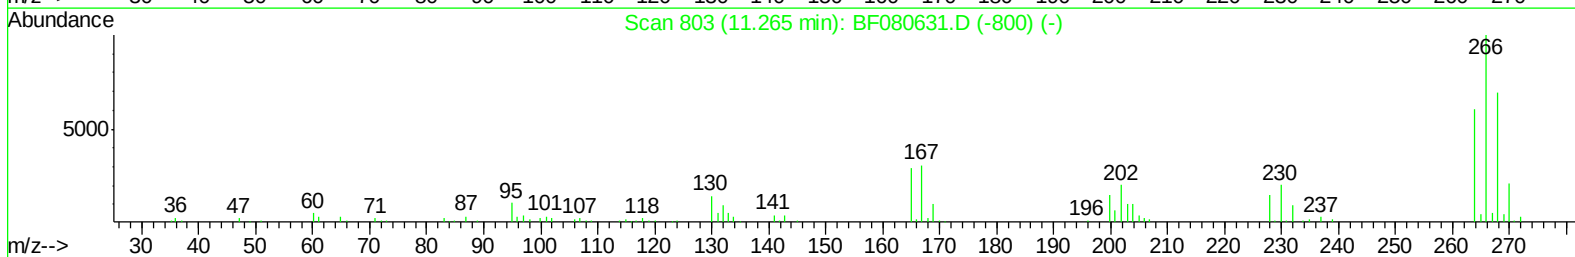
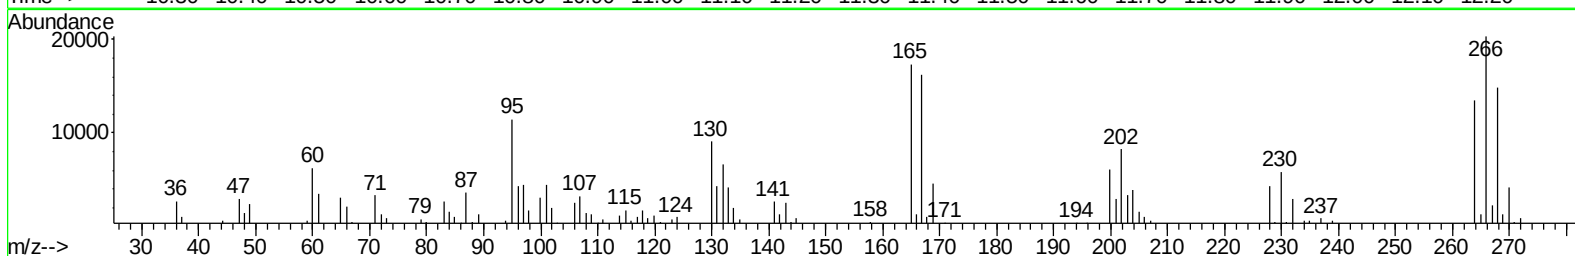


Data Path : Z:\HPCHEM1\BNA_F\Data\BF072415\
Data File : BF080648.D
Acq On : 25 Jul 2015 3:37
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 07:04:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 25 04:28:42 2015
Response via : Initial Calibration

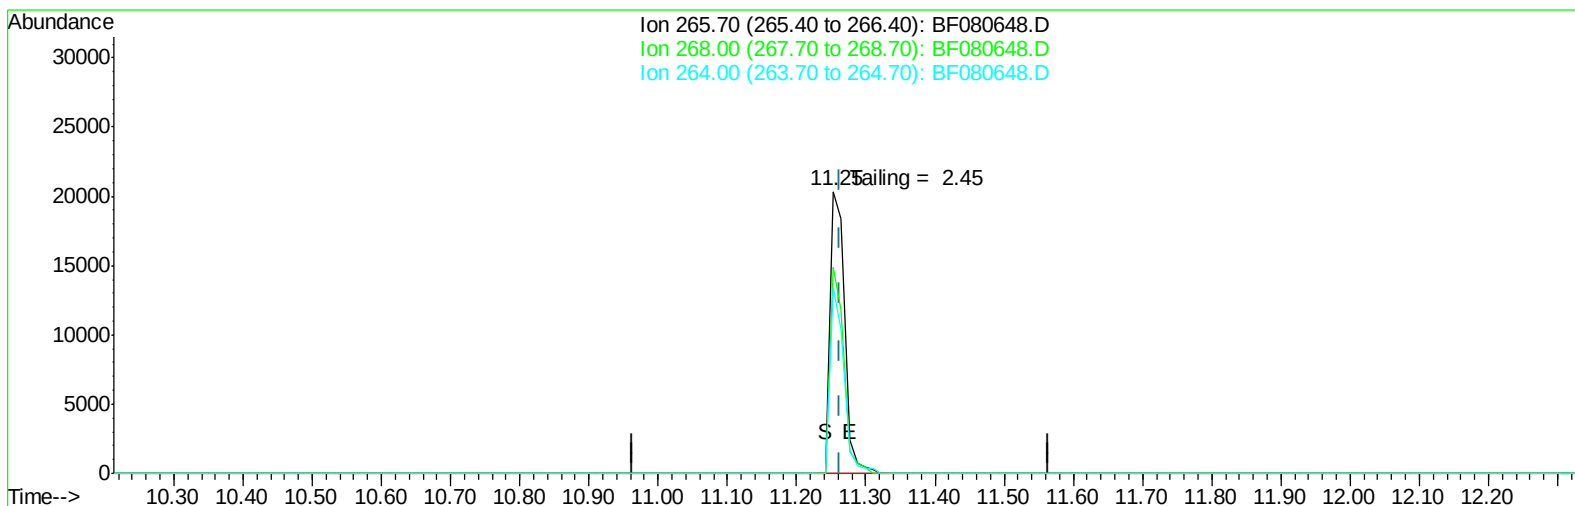

TIC: BF080648.D

(69) Pentachlorophenol (C)




11.253min (-0.011) 0.00ng

response 29205

Ion	Exp%	Act%
265.70	100	100
268.00	69.50	73.02
264.00	60.90	66.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF072415\
Data File : BF080648.D
Acq On : 25 Jul 2015 3:37
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 07:04:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 25 04:28:42 2015
Response via : Initial Calibration

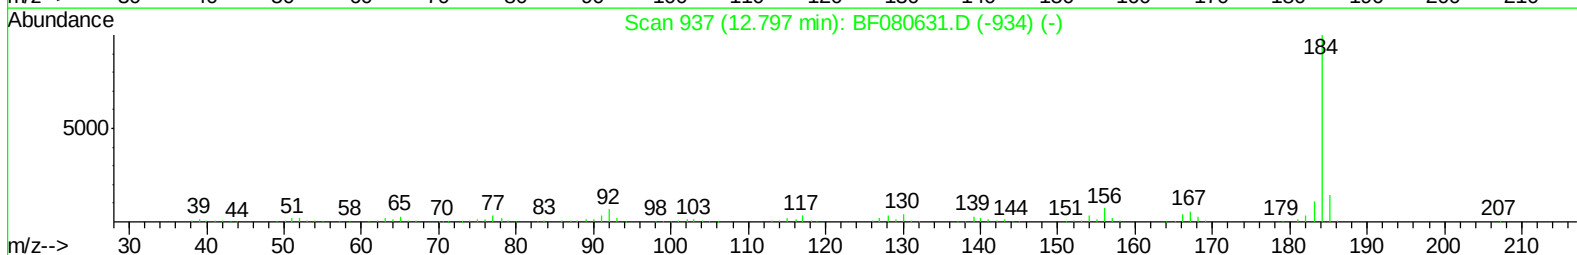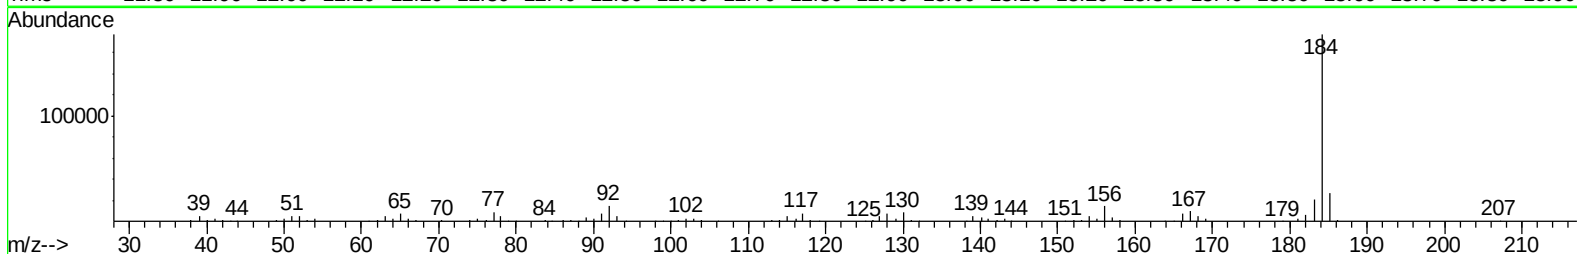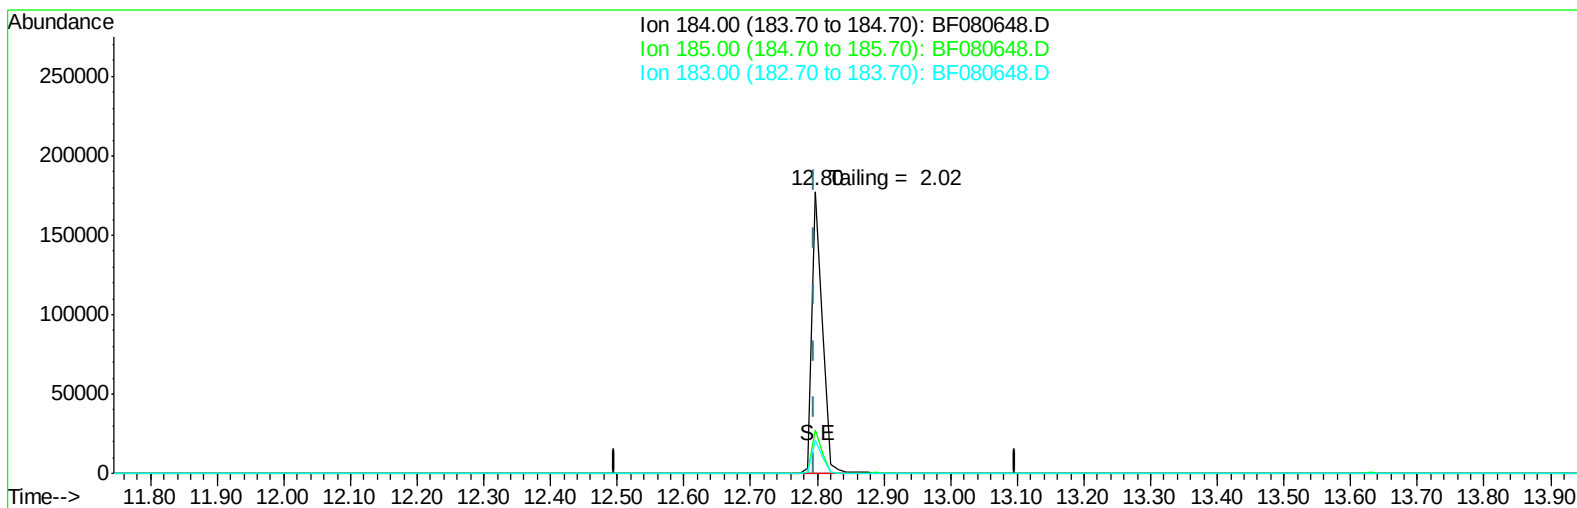

TIC: BF080648.D

(76) Benzidine

12.796min (-0.000) 0.00ng

response 192724

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	15.39
183.00	11.30	12.02
0.00	0.00	0.00