

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
 Data File : BF080663.D
 Acq On : 25 Jul 2015 11:18
 Operator : TP/UM
 Sample : G3053-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SYSDIS-07212015

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.230	269	275	277	rBV	17355475	36199444	100.00%	76.399%
2	5.504	296	299	302	rBV2	327099	523796	1.45%	1.105%
3	5.756	319	321	324	rBV	392037	374434	1.03%	0.790%
4	6.693	401	403	407	rBV2	787869	979525	2.71%	2.067%
5	6.933	421	424	427	rBV2	330471	584327	1.61%	1.233%
6	7.104	435	439	441	rVB2	2100824	2610583	7.21%	5.510%
7	7.493	470	473	477	rBV2	826562	1091101	3.01%	2.303%
8	9.287	628	630	633	rVB	1233453	1345908	3.72%	2.841%
9	9.973	687	690	692	rBV	473479	406006	1.12%	0.857%
10	10.750	756	758	761	rBV2	504135	607100	1.68%	1.281%
11	11.459	817	820	822	rBV	445258	410289	1.13%	0.866%
12	13.082	960	962	965	rBV	1321808	1421175	3.93%	2.999%
13	14.259	1062	1065	1067	rBV	401991	402593	1.11%	0.850%
14	15.928	1209	1211	1214	rBV	301504	425879	1.18%	0.899%


Sum of corrected areas: 47382160

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
Data File : BF080663.D
Acq On : 25 Jul 2015 11:18
Operator : TP/UM
Sample : G3053-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SYSDIS-07212015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

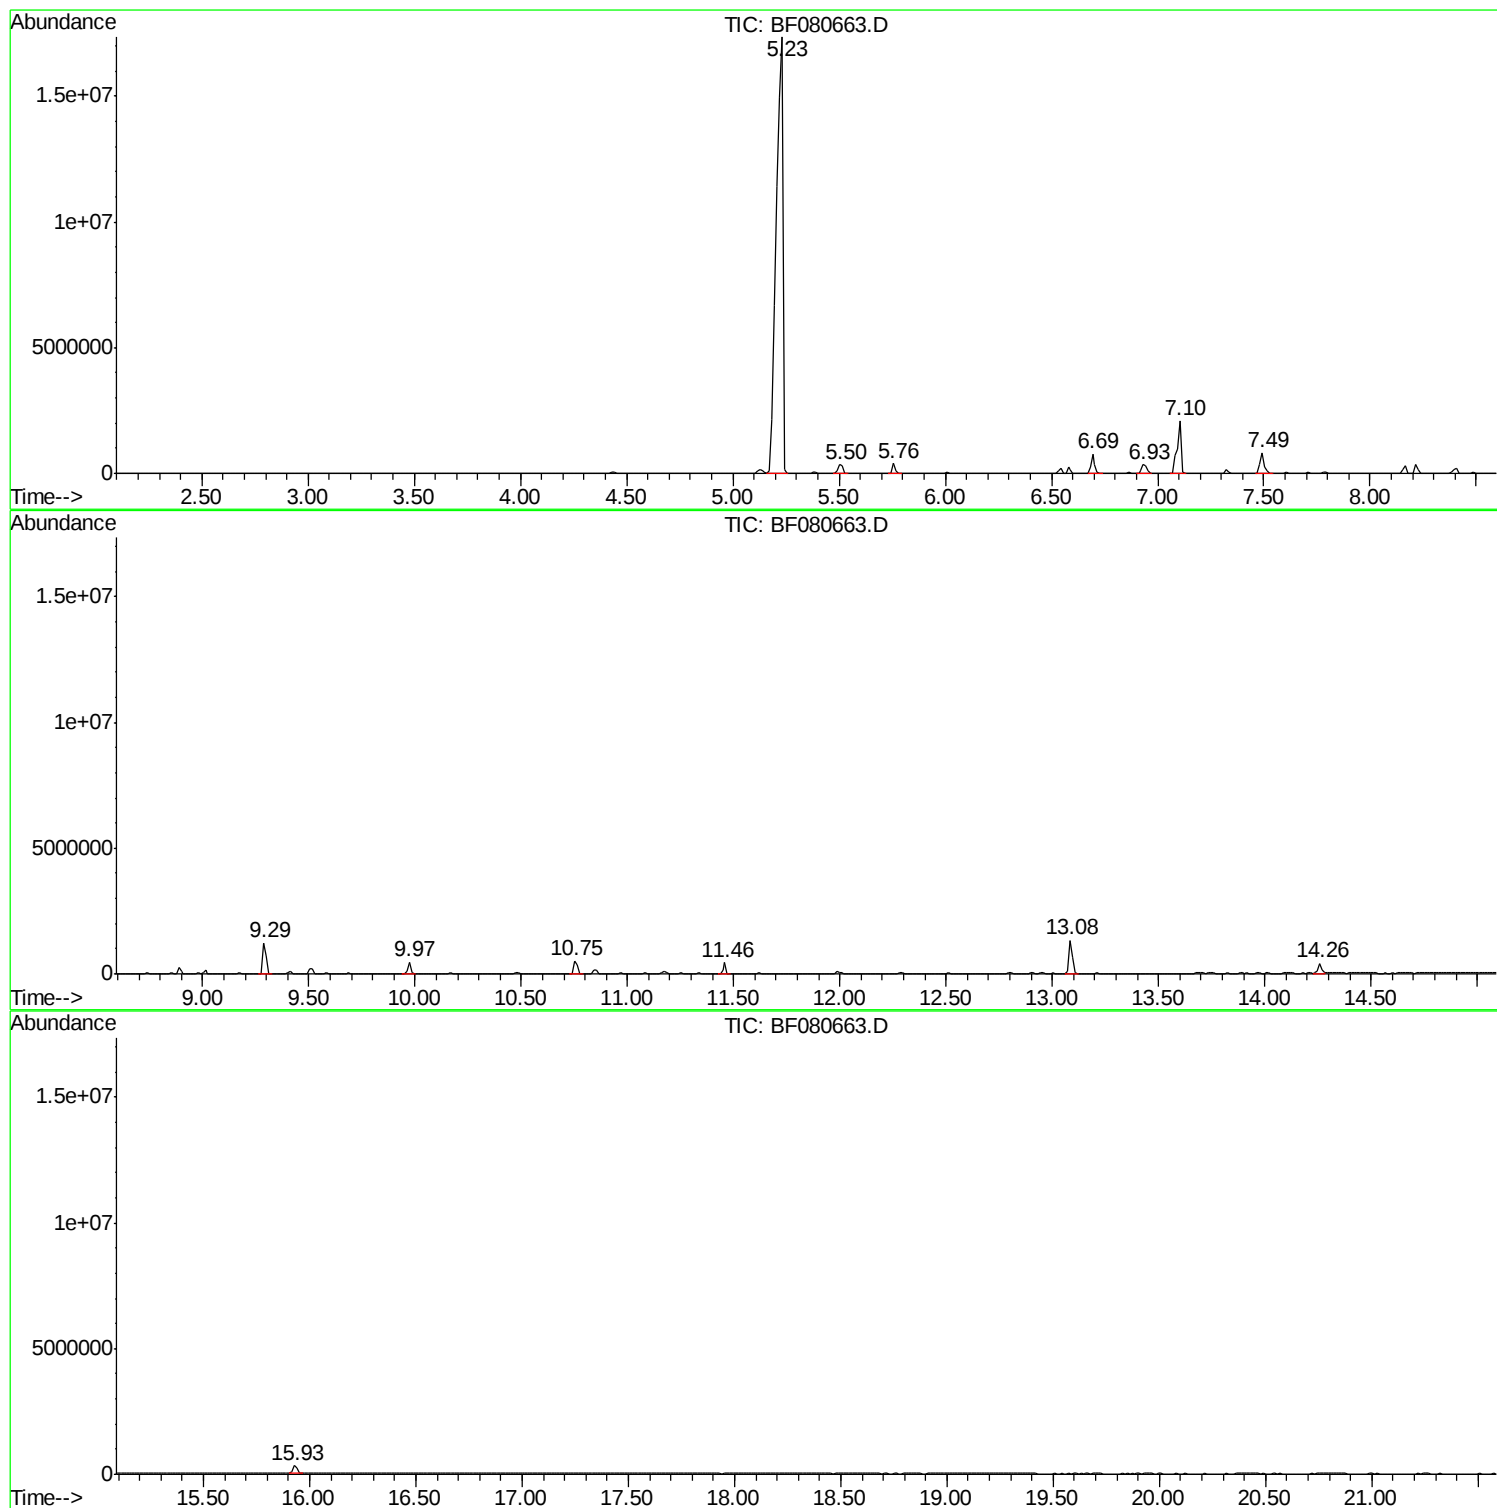

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
Data File : BF080663.D
Acq On : 25 Jul 2015 11:18
Operator : TP/UM
Sample : G3053-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SYSDIS-07212015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
Data File : BF080663.D
Acq On : 25 Jul 2015 11:18
Operator : TP/UM
Sample : G3053-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SYSDIS-07212015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc