


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
 Data File : BF080627.D
 Acq On : 24 Jul 2015 15:57
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 25 04:28:42 2015

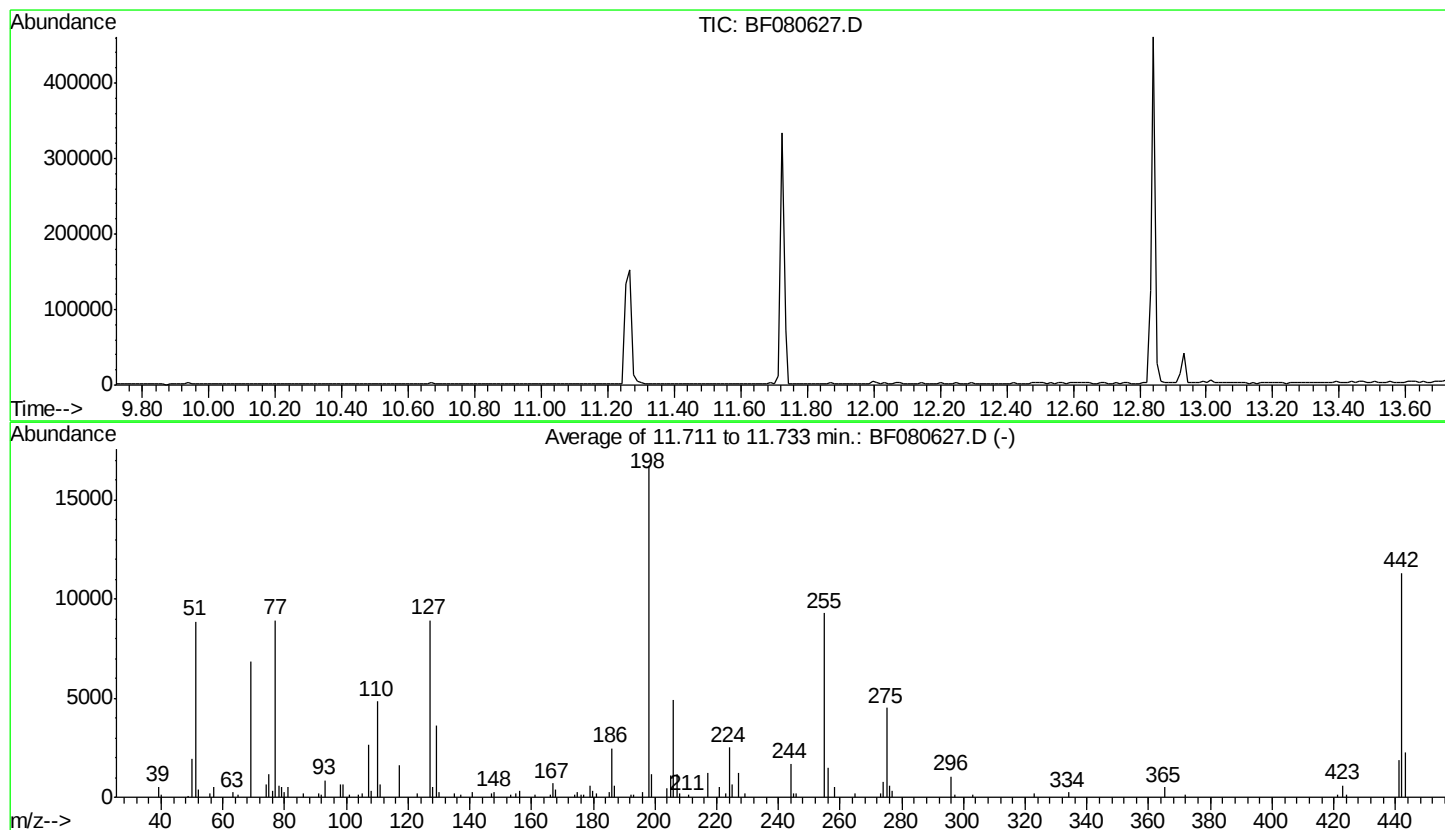

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	8851	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	6811	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	8934	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16711	PASS
199	198	5	9	7.1	1192	PASS
275	198	10	60	27.0	4511	PASS
365	198	1	100	3.0	495	PASS
441	442	0.01	24	16.4	1855	PASS
442	198	50	100	67.6	11298	PASS
443	442	15	24	20.1	2268	PASS