


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072415\
 Data File : BF080648.D
 Acq On : 25 Jul 2015 3:37
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 25 04:28:42 2015

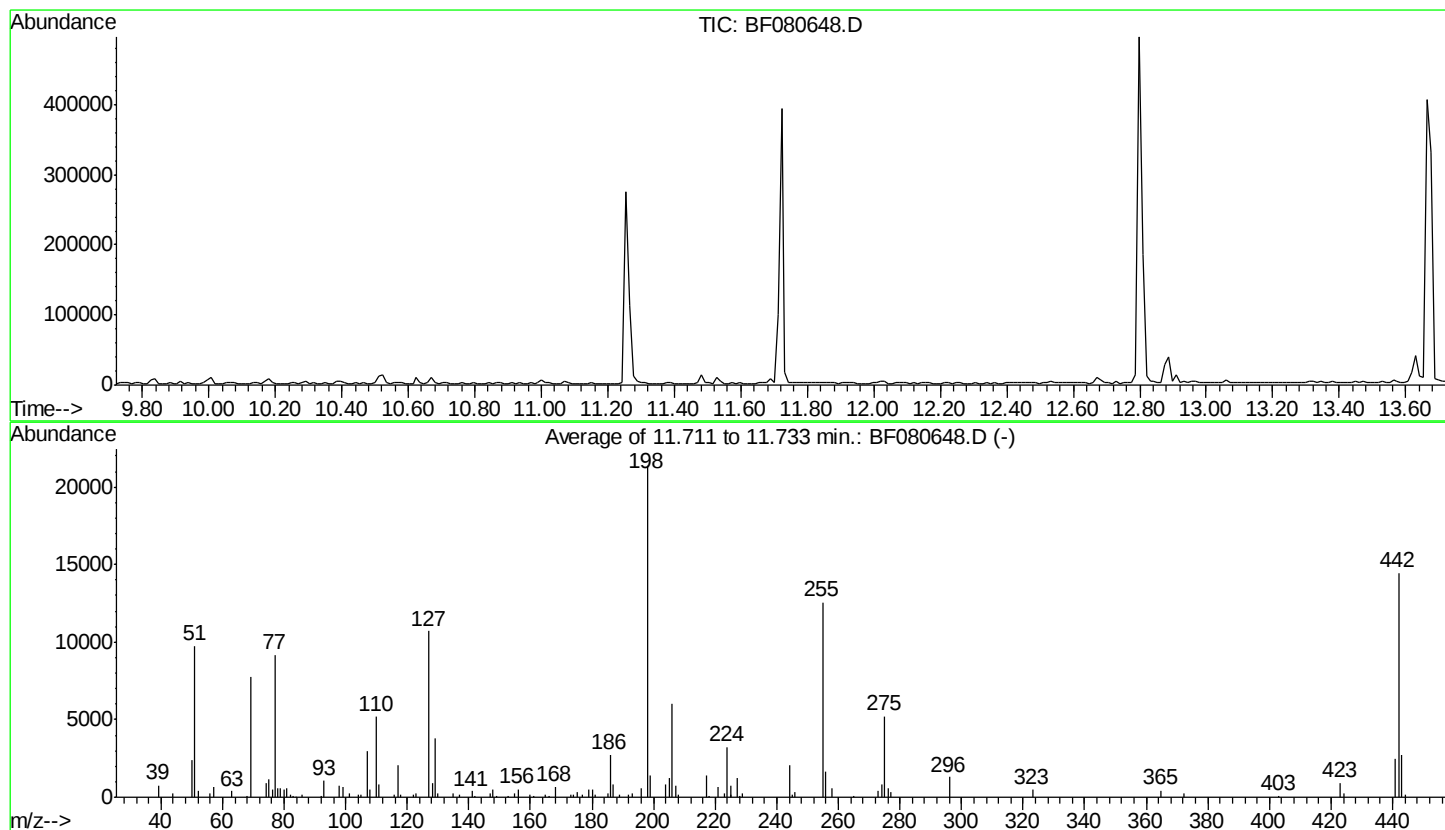

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	9740	PASS
68	69	0.00	2	1.3	102	PASS
69	198	0.00	100	36.5	7800	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	10722	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21376	PASS
199	198	5	9	6.4	1366	PASS
275	198	10	60	24.4	5216	PASS
365	198	1	100	2.0	417	PASS
441	442	0.01	24	17.2	2489	PASS
442	198	50	100	67.6	14452	PASS
443	442	15	24	18.9	2733	PASS