
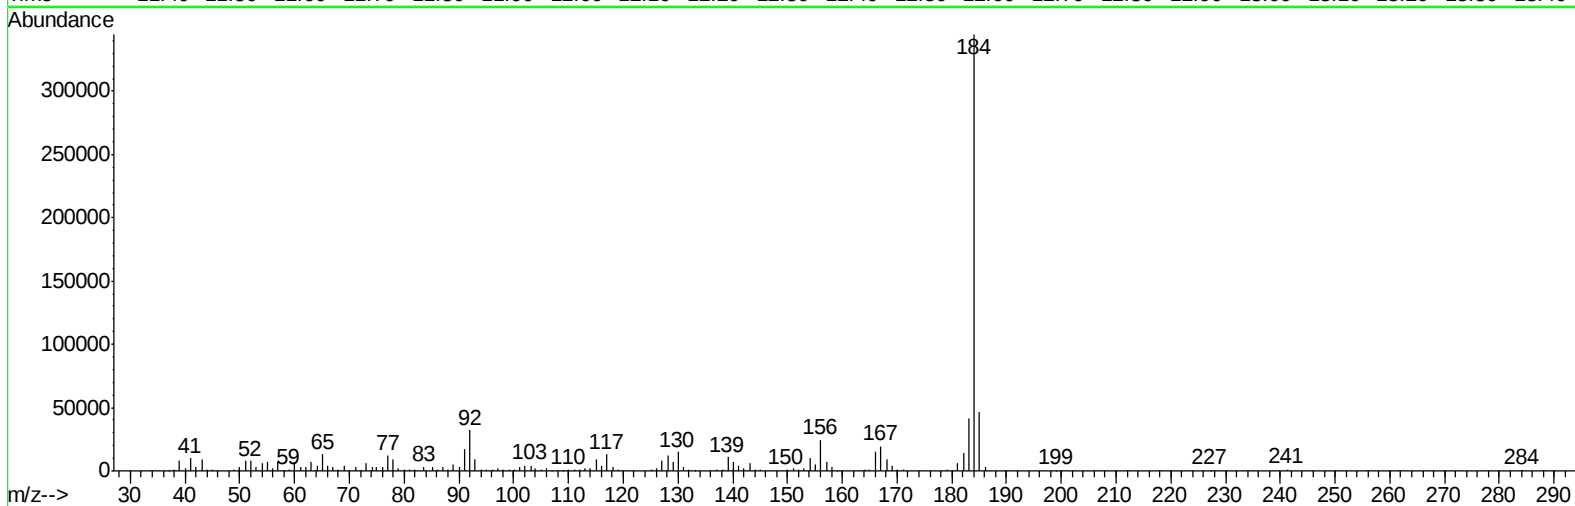


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\
Data File : BF096982.D
Acq On : 24 Jul 2017 10:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 06:55:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:37:00 2017
Response via : Initial Calibration

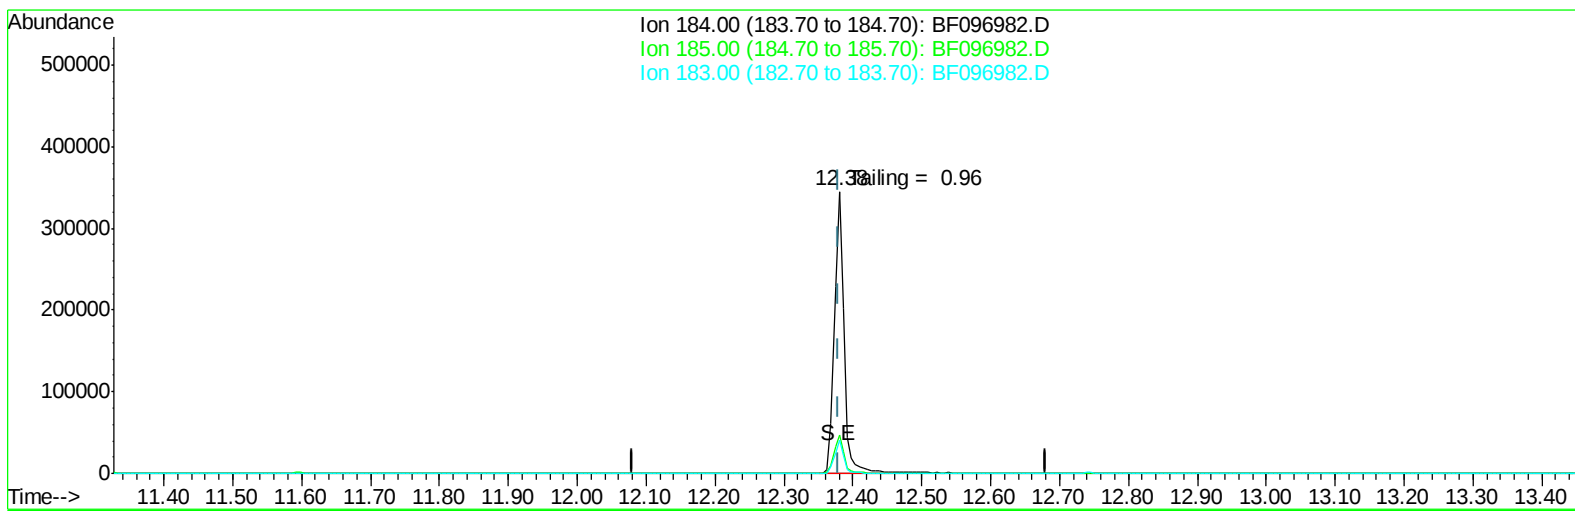

TIC: BF096982.D

(76) Benzidine

12.380min (0.000) 6166.92ng

response 334563

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.61#
183.00	12.20	12.03
0.00	0.00	0.00