
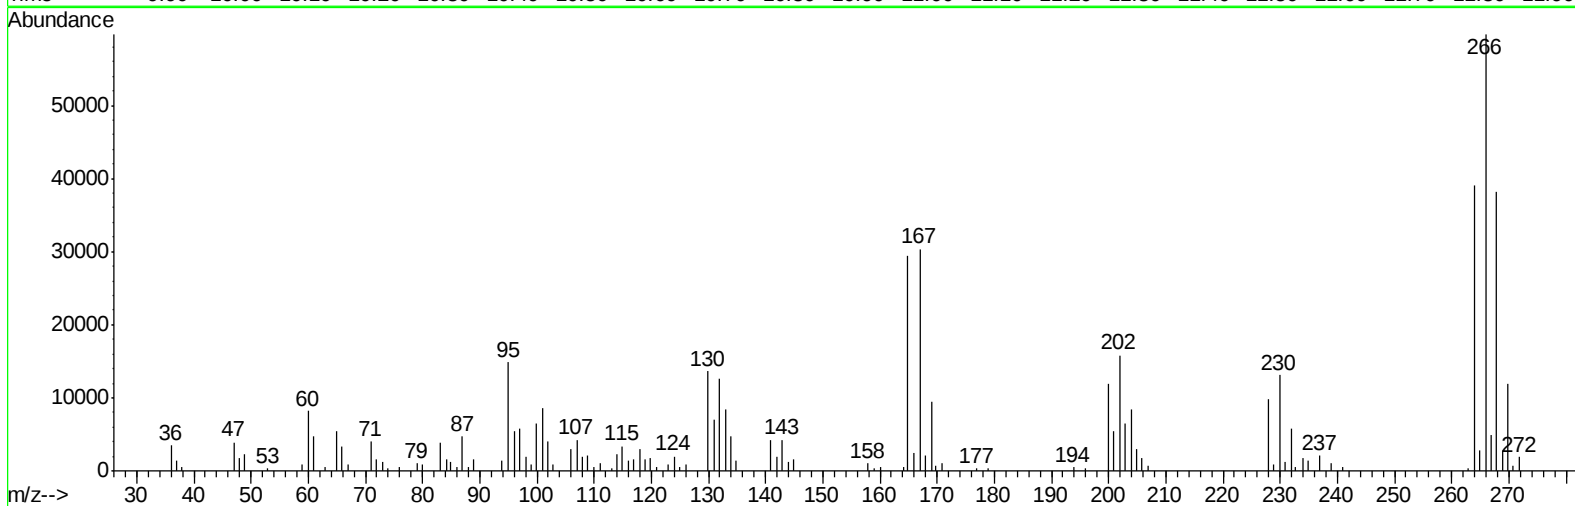


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\  
Data File : BF096990.D  
Acq On : 24 Jul 2017 17:36  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 06:57:31 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 25 01:37:00 2017  
Response via : Initial Calibration

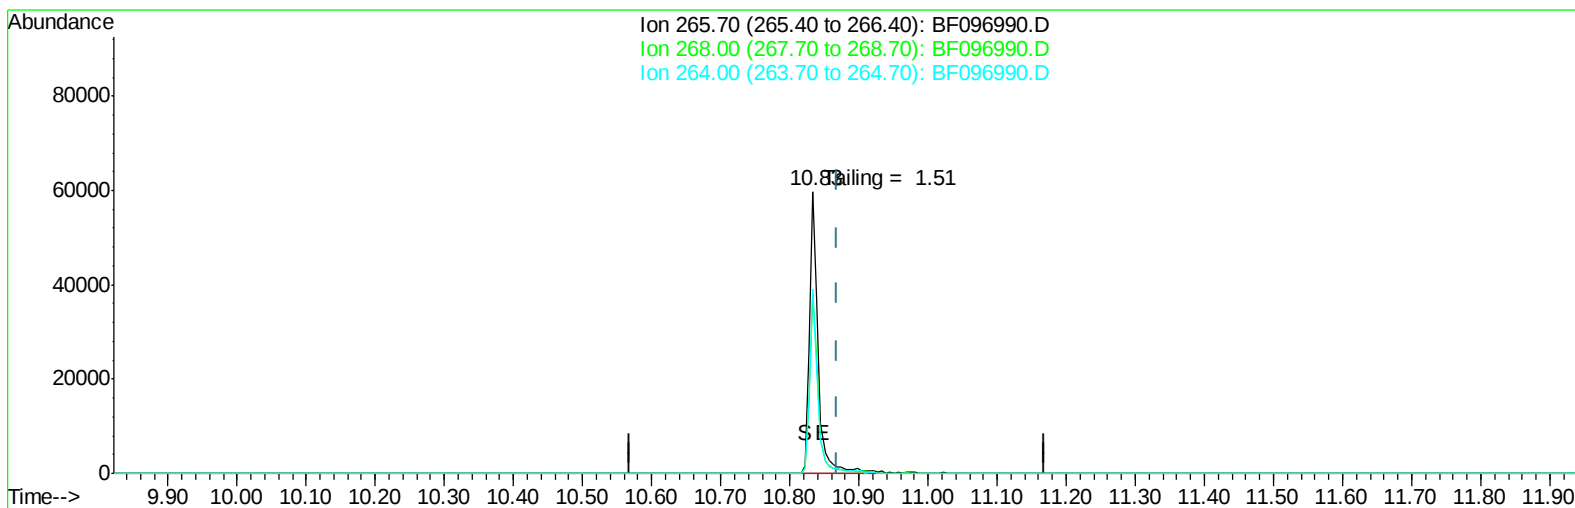

TIC: BF096990.D

(69) Pentachlorophenol (C)

10.833min (-0.035) 70574.75ng

response 53501

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.82 |
| 264.00 | 64.60 | 65.47 |
| 0.00   | 0.00  | 0.00  |