

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\
 Data File : BF097011.D
 Acq On : 25 Jul 2017 3:17
 Operator : SJ/JU
 Sample : I4360-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CEMETERY-11-(0-2)

Quant Time: Jul 25 03:58:37 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 01:37:00 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.52	152	135961	20.00	ng	-0.02
21) Naphthalene-d8	7.80	136	542648	20.00	ng	-0.03
38) Acenaphthene-d10	9.54	164	219006	20.00	ng	-0.04
63) Phenanthrene-d10	11.02	188	321784	20.00	ng	-0.04
75) Chrysene-d12	13.64	240	246252	20.00	ng	-0.04
86) Perylene-d12	15.00	264	220664	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	760149	84.06	ng	-0.03
7) Phenol-d6	6.18	99	981456	90.45	ng	-0.04
23) Nitrobenzene-d5	7.08	82	589892	67.33	ng	-0.04
41) 2,4,6-Tribromophenol	10.33	330	154710	82.76	ng	-0.04
44) 2-Fluorobiphenyl	8.87	172	904370	65.24	ng	-0.04
78) Terphenyl-d14	12.60	244	542376	38.20	ng	-0.04
Target Compounds						
10) Phenol	6.19	94	32830	2.68	ng	Qvalue 100
19) n-Nitroso-di-n-propylamine	7.08	70	77740	11.89	ng	# 87
25) Isophorone	7.08	82	586190	35.97	ng	# 67
49) Dimethylphthalate	9.27	163	118869	7.21	ng	99
56) 2,4-Dinitrotoluene	9.54	165	27683	6.03	ng	# 31
66) 4-Bromophenyl-phenylether	10.33	248	9798	2.98	ng	# 1
85) Indeno(1,2,3-cd)pyrene	16.23	276	8252	3.90	ng	# 84
88) Benzo(k)fluoranthene	14.63	252	26271	2.08	ng	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\
Data File : BF097011.D
Acq On : 25 Jul 2017 3:17
Operator : SJ/JU
Sample : I4360-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CEMETERY-11-(0-2)

Quant Time: Jul 25 03:58:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:37:00 2017
Response via : Initial Calibration




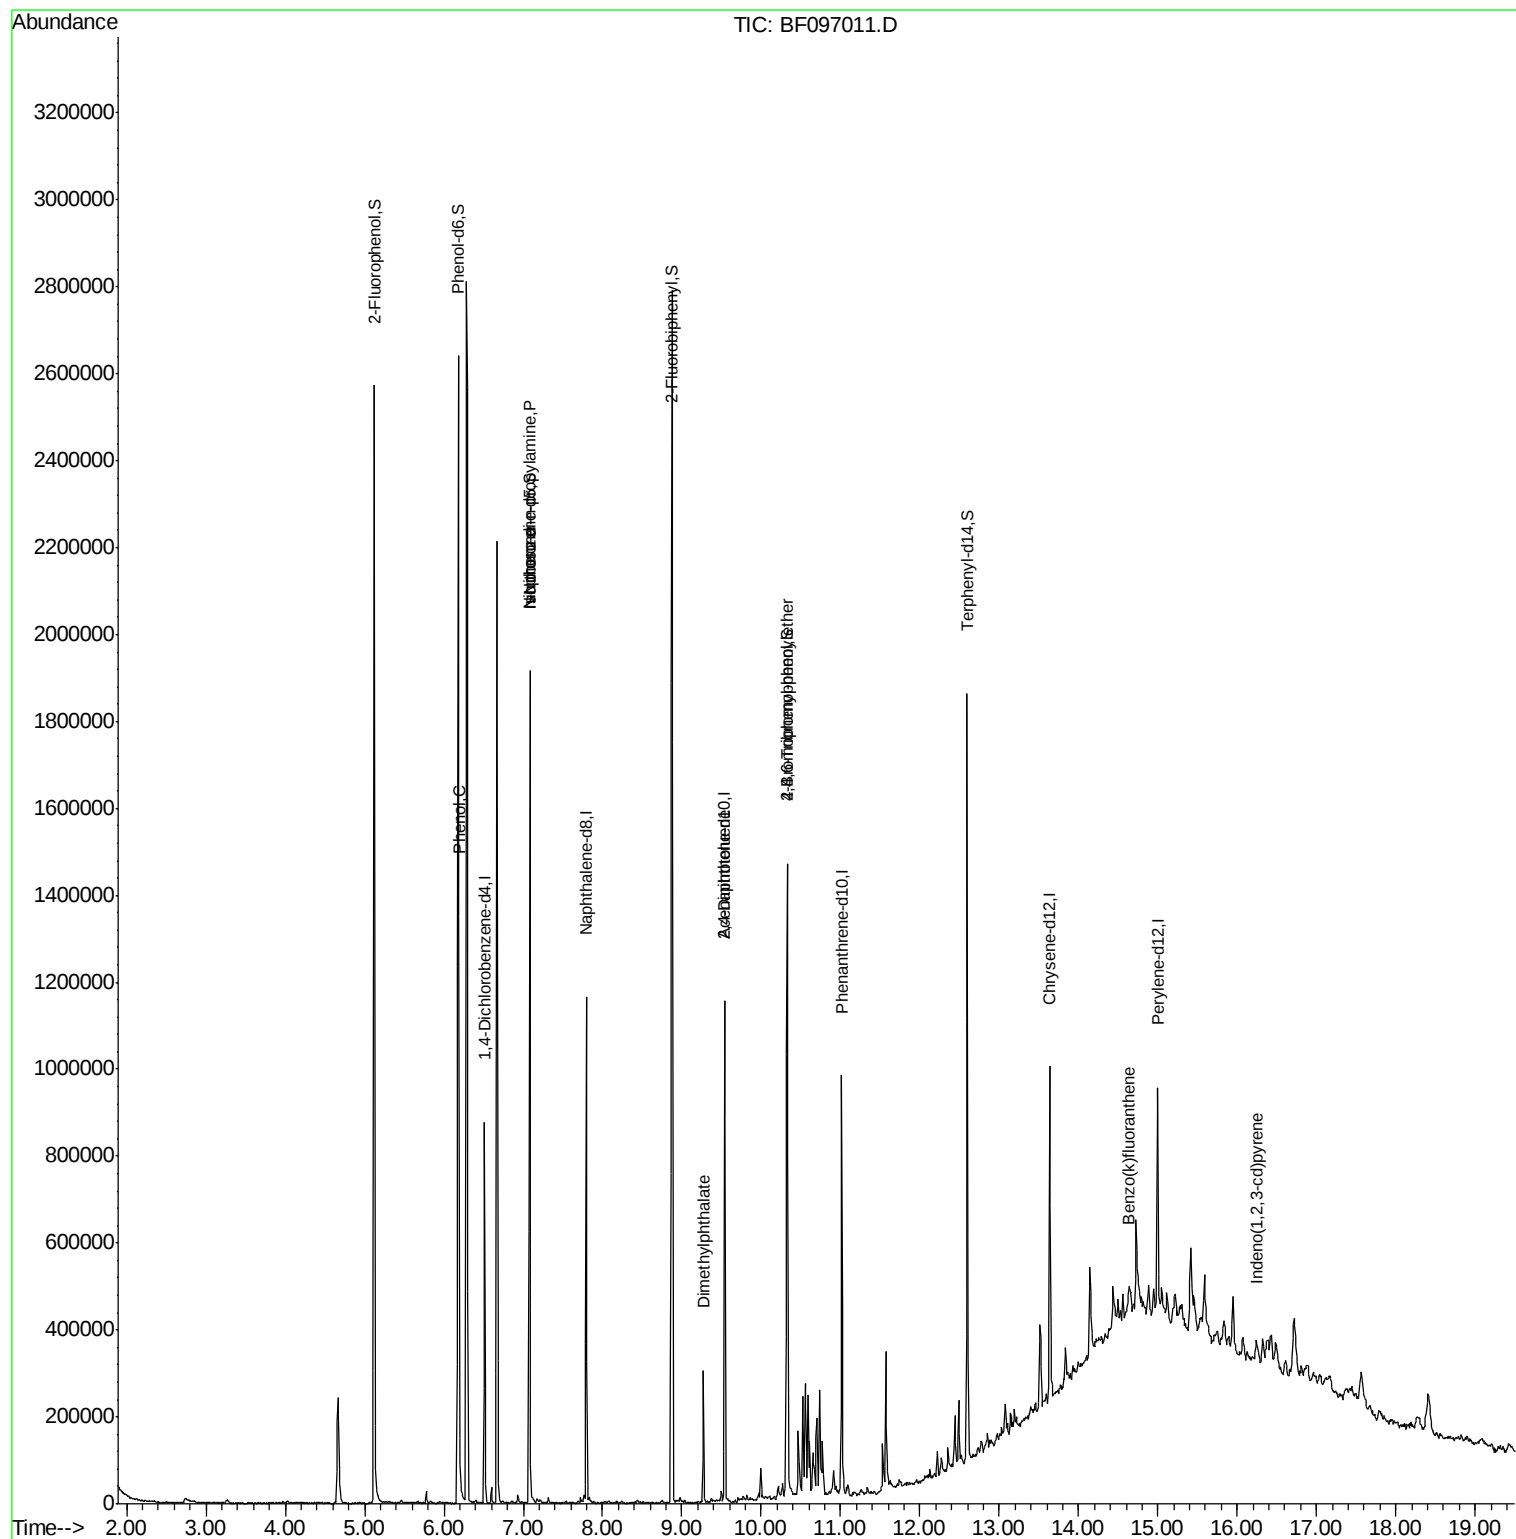


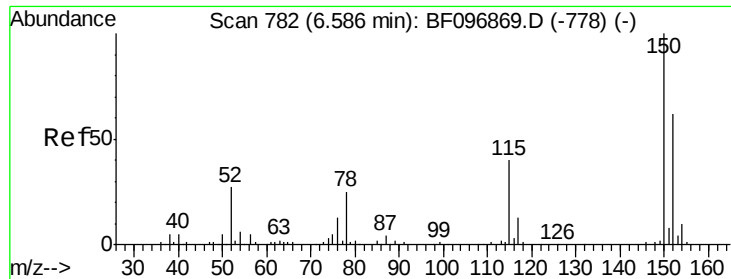

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.52 min Scan# 787
 Delta R.T. -0.02 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17




Instrument :
 BNA_F
 ClientSampleId :
 CEMETERY-11-(0-2)


Tot Ion:152 Resp: 135961
 Ion Ratio Lower Upper
 152 100
 150 155.0 126.2 189.2
 115 62.8 52.2 78.2

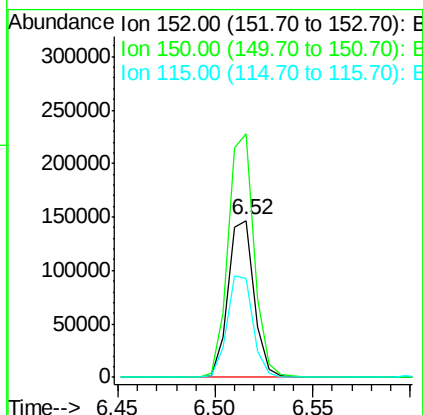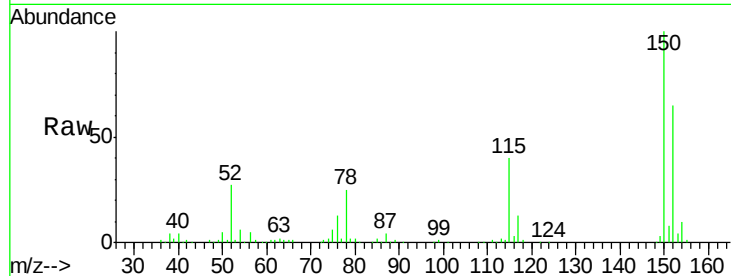

#5
 2-Fluorophenol
 Concen: 84.06 ng
 RT: 5.12 min Scan# 550
 Delta R.T. -0.03 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Tgt Ion:112 Resp: 760149
 Ion Ratio Lower Upper
 112 100
 64 64.4 46.0 69.0
 63 33.6 23.4 35.0

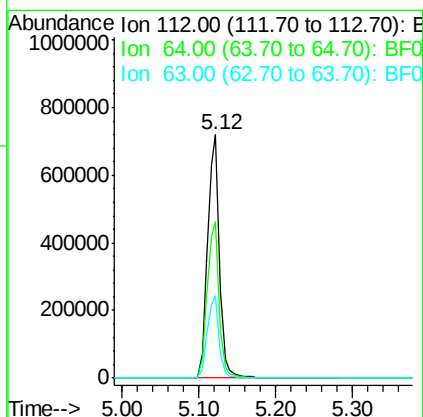



#7

Phenol-d6

Concen: 90.45 ng

RT: 6.18 min Scan# 730

Delta R.T. -0.04 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17

Instrument :

BNA_F

ClientSampleId :

CEMETERY-11-(0-2)





Tot Ion: 99 Resp: 981456

Ion Ratio Lower Upper

99 100

42 22.8 13.5 20.3#

71 32.2 24.5 36.7

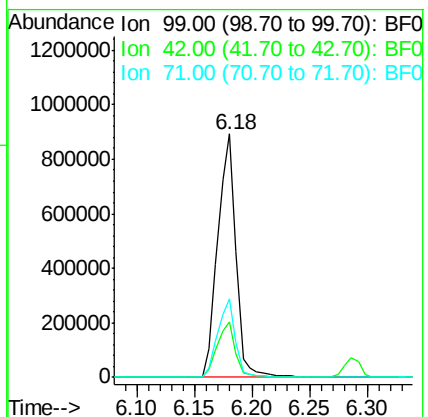

#10

Phenol

Concen: 2.68 ng

RT: 6.19 min Scan# 732

Delta R.T. -0.04 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17




Tgt Ion: 94 Resp: 32830




Ion Ratio Lower Upper

94 100

65 30.3 9.9 49.9

66 43.1 23.1 63.1



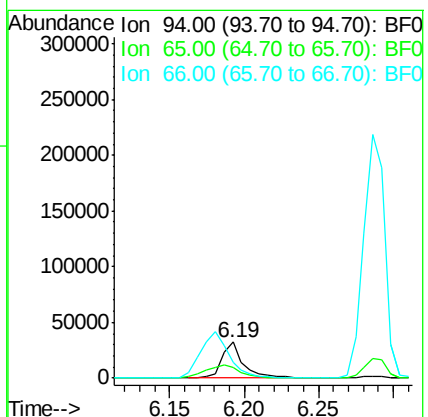



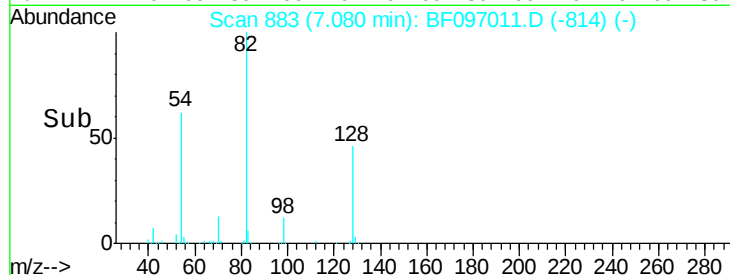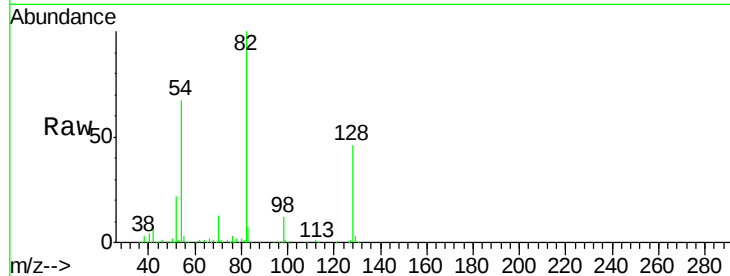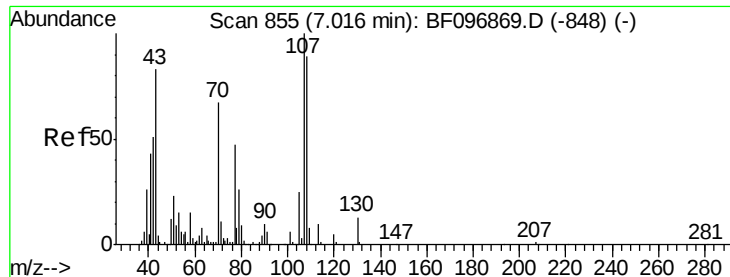

#19
n-Nitroso-di-n-propylamine
Concen: 11.89 ng
RT: 7.08 min Scan# 883
Delta R.T. 0.11 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17


Instrument :
BNA_F
ClientSampleId :
CEMETERY-11-(0-2)


Tot Ion	Ratio	Lower	Upper
70	100		
42	61.4	47.2	70.8
101	0.0	7.2	10.8#
130	2.3	15.9	23.9#

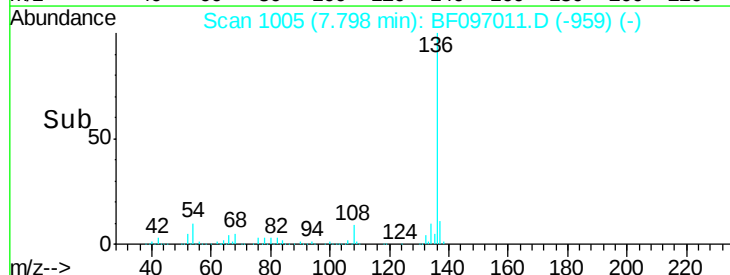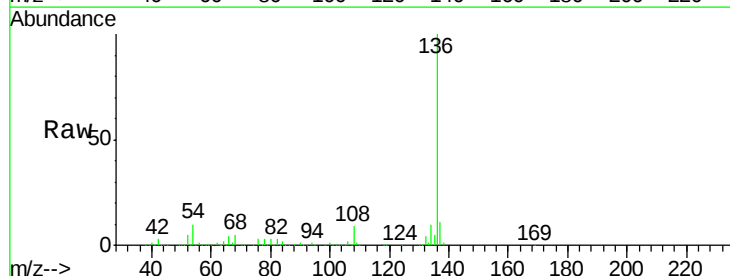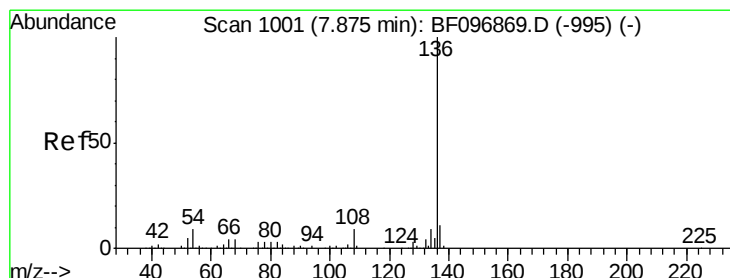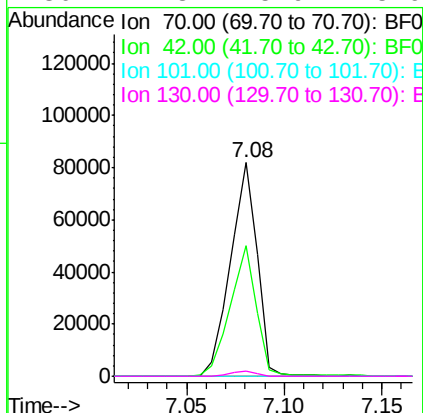

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.80 min Scan# 1005
Delta R.T. -0.03 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17

Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.5	12.7
54	9.9	4.9	7.3#
68	5.2	4.1	6.1

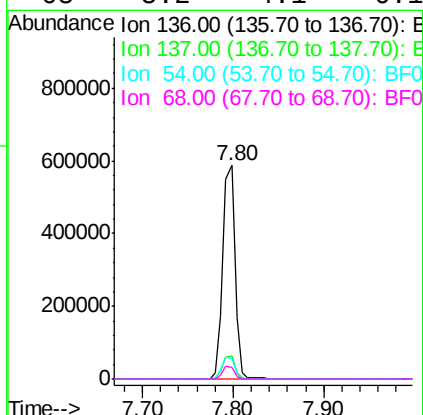







#23
 Nitrobenzene-d5
 Concen: 67.33 ng
 RT: 7.08 min Scan# 883
 Delta R.T. -0.04 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Instrument :
 BNA_F
 ClientSampleId :
 CEMETERY-11-(0-2)

Tot Ion	82	Resp	589892
Ion Ratio	Lower	Upper	
82	100		
128	46.4	34.0	51.0
54	66.9	42.2	63.2#

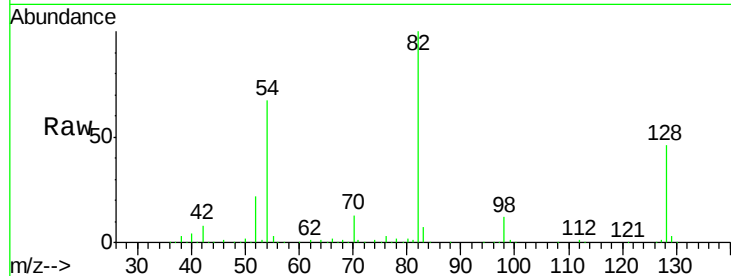


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

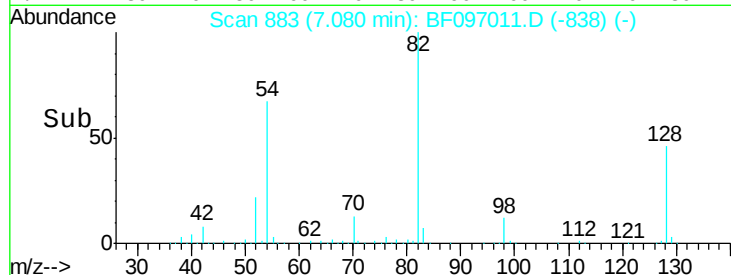
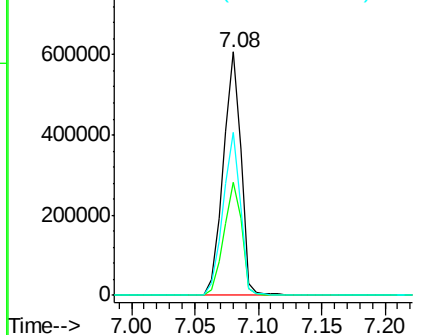



#25
 Isophorone
 Concen: 35.97 ng
 RT: 7.08 min Scan# 883
 Delta R.T. -0.29 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Tgt Ion	82	Resp	586190
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.3	7.9#
138	0.0	13.1	19.7#

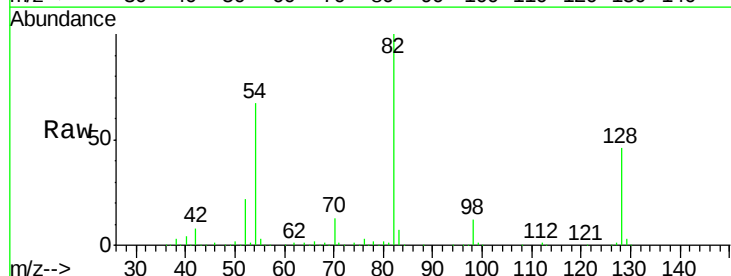

Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0

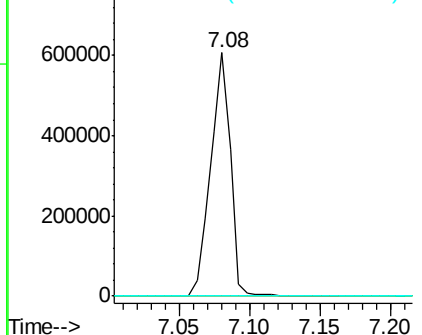

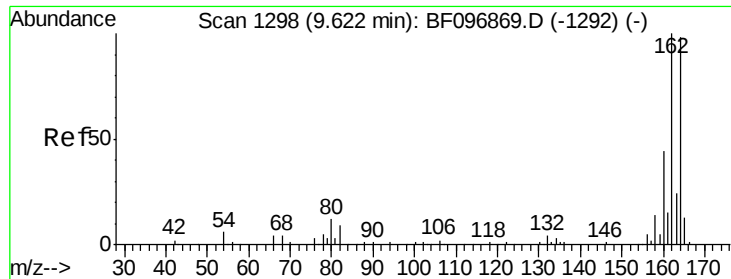

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.54 min Scan# 1301

Delta R.T. -0.04 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17

Instrument :

BNA_F

ClientSampleId :

CEMETERY-11-(0-2)


Tot Ion:164 Resp: 219006

Ion Ratio Lower Upper

164 100

162 103.8 82.6 123.8




160 44.7 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

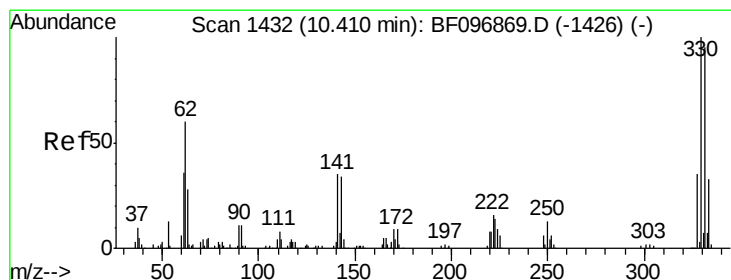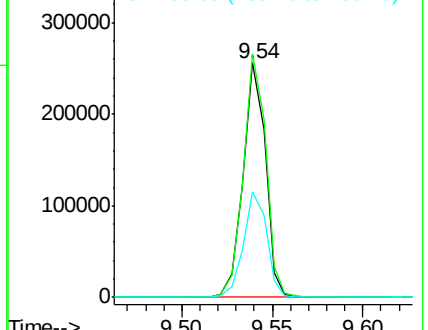

#41

2,4,6-Tribromophenol

Concen: 82.76 ng

RT: 10.33 min Scan# 1435

Delta R.T. -0.04 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17


Tgt Ion:330 Resp: 154710

Ion Ratio Lower Upper

330 100

332 94.8 76.6 115.0



141 39.1 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




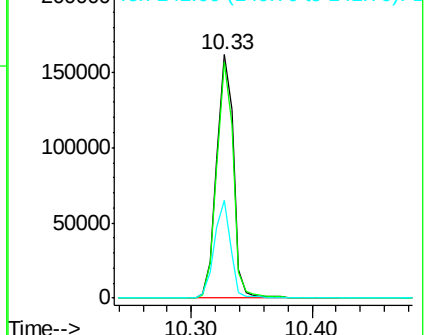


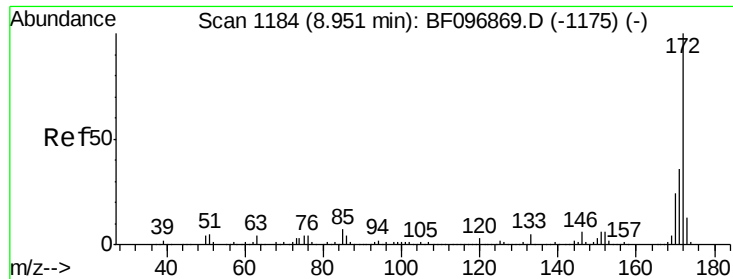

#44
 2-Fluorobiphenyl
 Concen: 65.24 ng
 RT: 8.87 min Scan# 1188
 Delta R.T. -0.04 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17




Instrument :
 BNA_F
 ClientSampleId :
 CEMETERY-11-(0-2)

Tot Ion:172 Resp: 904370
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.6 44.4
 170 24.3 19.8 29.8

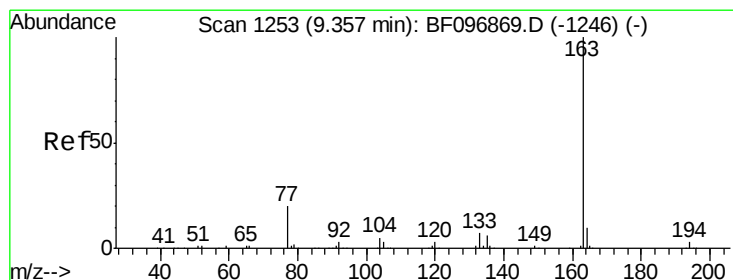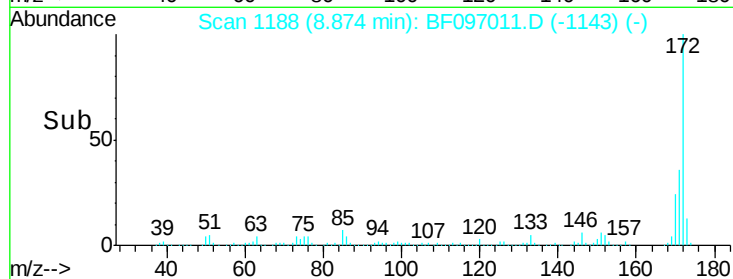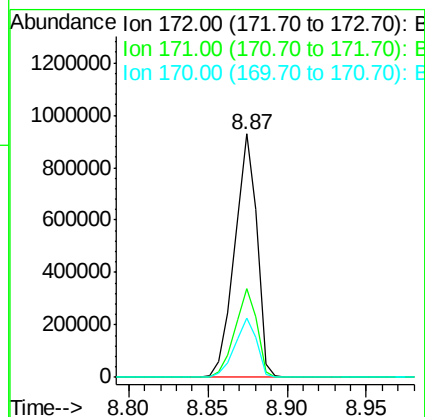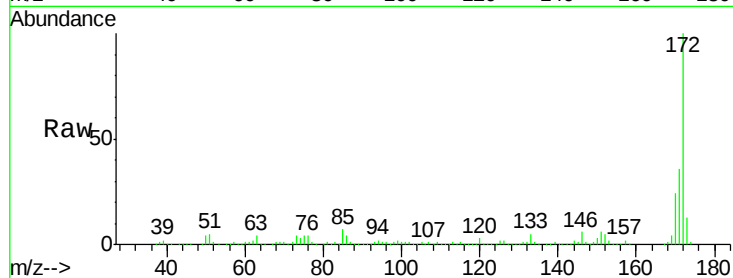

#49
 Dimethylphthalate
 Concen: 7.21 ng
 RT: 9.27 min Scan# 1255
 Delta R.T. -0.05 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Tgt Ion:163 Resp: 118869
 Ion Ratio Lower Upper
 163 100
 194 3.1 2.6 4.0
 164 10.2 8.4 12.6

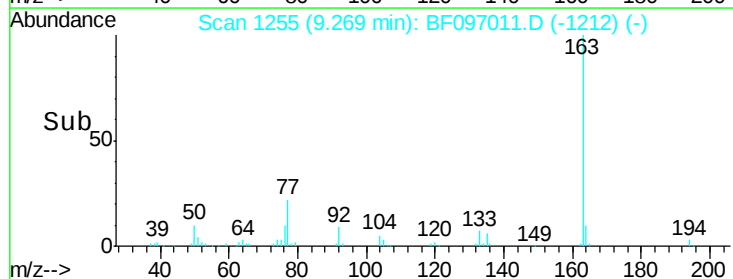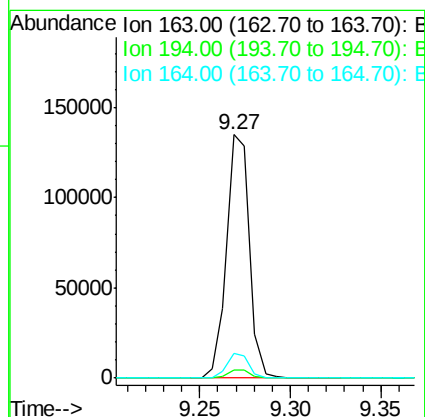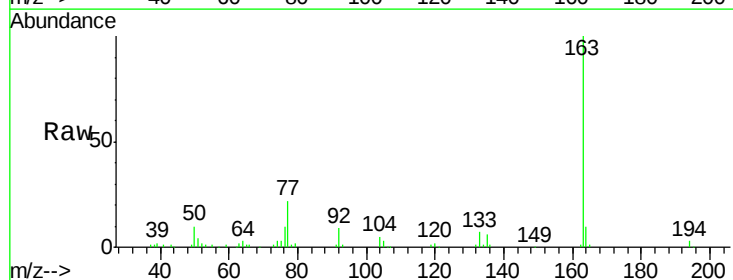







#56
 2,4-Dinitrotoluene
 Concen: 6.03 ng
 RT: 9.54 min Scan# 1301
 Delta R.T. -0.24 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Instrument :
 BNA_F
 ClientSampleId :
 CEMETERY-11-(0-2)

Tot Ion:	165	Resp:	27683
Ion	Ratio	Lower	Upper
165	100		
63	0.9	25.4	38.0#
89	0.0	46.4	69.6#
182	0.0	1.8	2.6#




Abundance Ion 165.00 (164.70 to 165.70): E


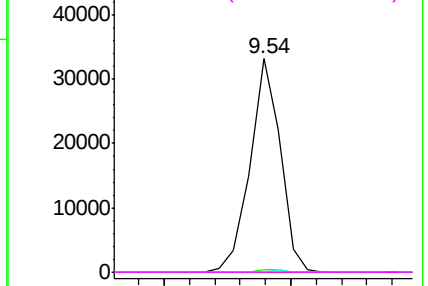



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.02 min Scan# 1552
 Delta R.T. -0.04 min
 Lab File: BF097011.D
 Acq: 25 Jul 2017 3:17

Tgt Ion:	188	Resp:	321784
Ion	Ratio	Lower	Upper
188	100		
94	10.5	9.4	14.2
80	10.7	10.2	15.2



Abundance Ion 188.00 (187.70 to 188.70): E

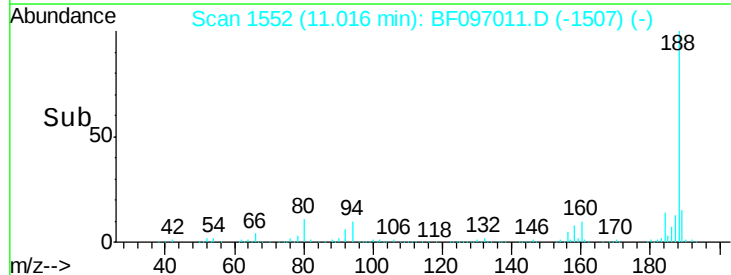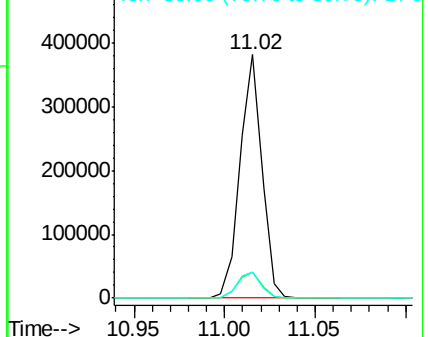


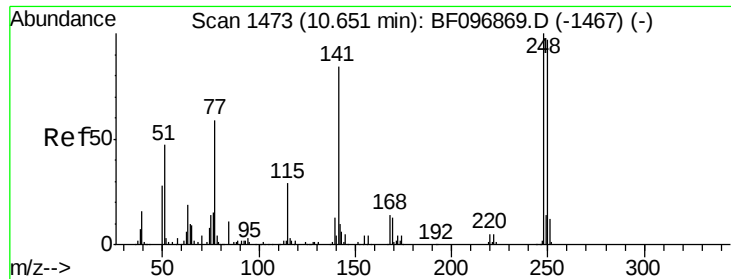




#66
4-Bromophenyl-phenylether
Concen: 2.98 ng
RT: 10.33 min Scan# 1435
Delta R.T. -0.28 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17

Instrument :
BNA_F
ClientSampleId :
CEMETERY-11-(0-2)

Tot Ion:248 Resp: 9798
Ion Ratio Lower Upper
248 100
250 186.2 76.8 115.2#
141 591.5 68.6 103.0#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

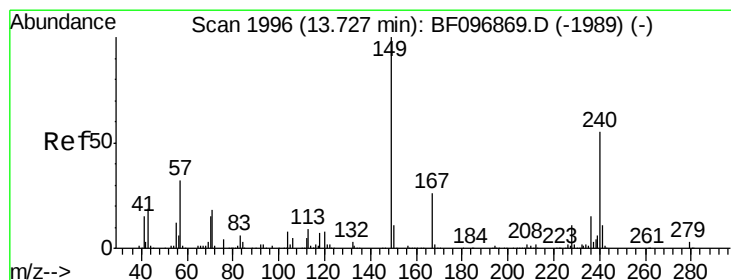
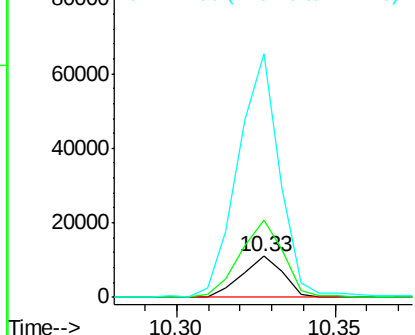



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.64 min Scan# 1998
Delta R.T. -0.04 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17

Tgt Ion:240 Resp: 246252
Ion Ratio Lower Upper
240 100
120 15.2 5.8 8.8#
236 25.7 20.5 30.7

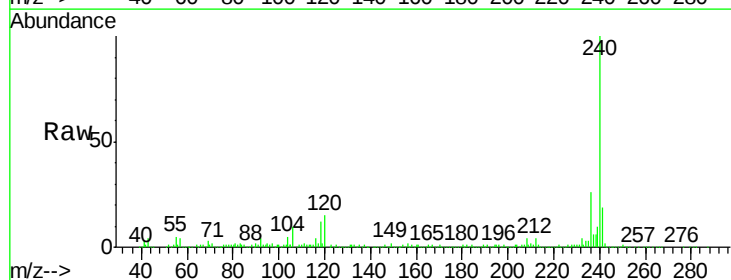

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

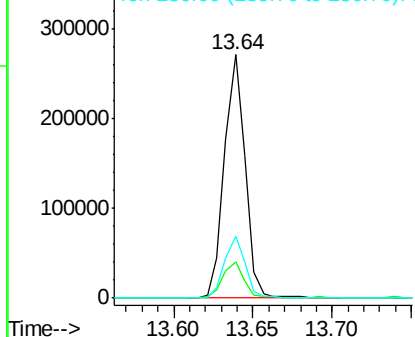



#78

Terphenyl-d14

Concen: 38.20 ng

RT: 12.60 min Scan# 1821

Delta R.T. -0.04 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17

Instrument :

BNA_F

ClientSampleId :

CEMETERY-11-(0-2)


Tot Ion:244 Resp: 542376

Ion Ratio Lower Upper

244 100

212 6.9 6.0 9.0




122 15.2 10.3 15.5



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

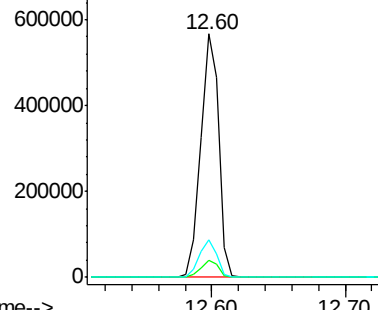

#85

Indeno(1,2,3-cd)pyrene

Concen: 3.90 ng

RT: 16.23 min Scan# 2439

Delta R.T. -0.06 min

Lab File: BF097011.D

Acq: 25 Jul 2017 3:17


Tgt Ion:276 Resp: 8252

Ion Ratio Lower Upper

276 100

138 50.0 27.8 41.6#



277 24.7 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




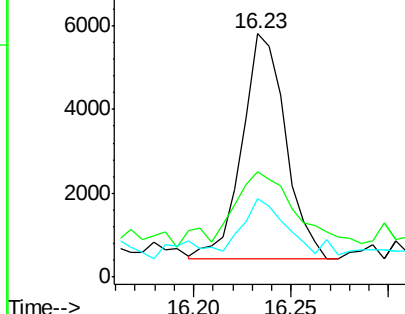


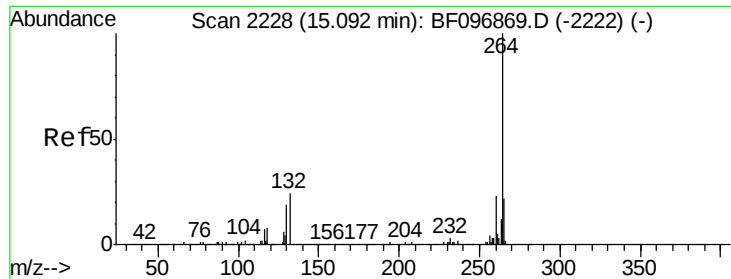

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.00 min Scan# 2229
Delta R.T. -0.04 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17

Instrument :
BNA_F
ClientSampleId :
CEMETERY-11-(0-2)

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.8	19.5	29.3
265	21.6	17.2	25.8

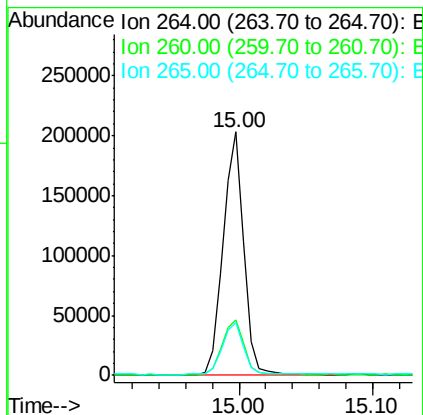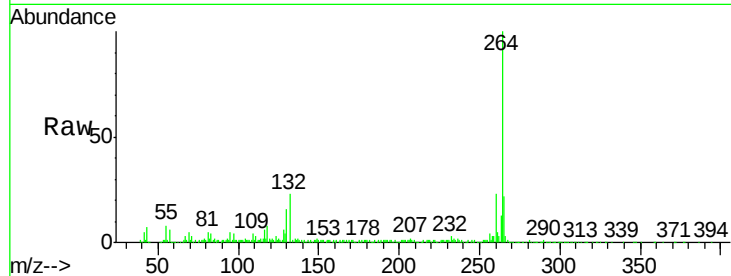

#88
Benzo(k)fluoranthene
Concen: 2.08 ng
RT: 14.63 min Scan# 2167
Delta R.T. -0.06 min
Lab File: BF097011.D
Acq: 25 Jul 2017 3:17

Tgt Ion	Ratio	Lower	Upper
252	100		
253	36.5	18.4	27.6#
125	34.9	13.1	19.7#

