
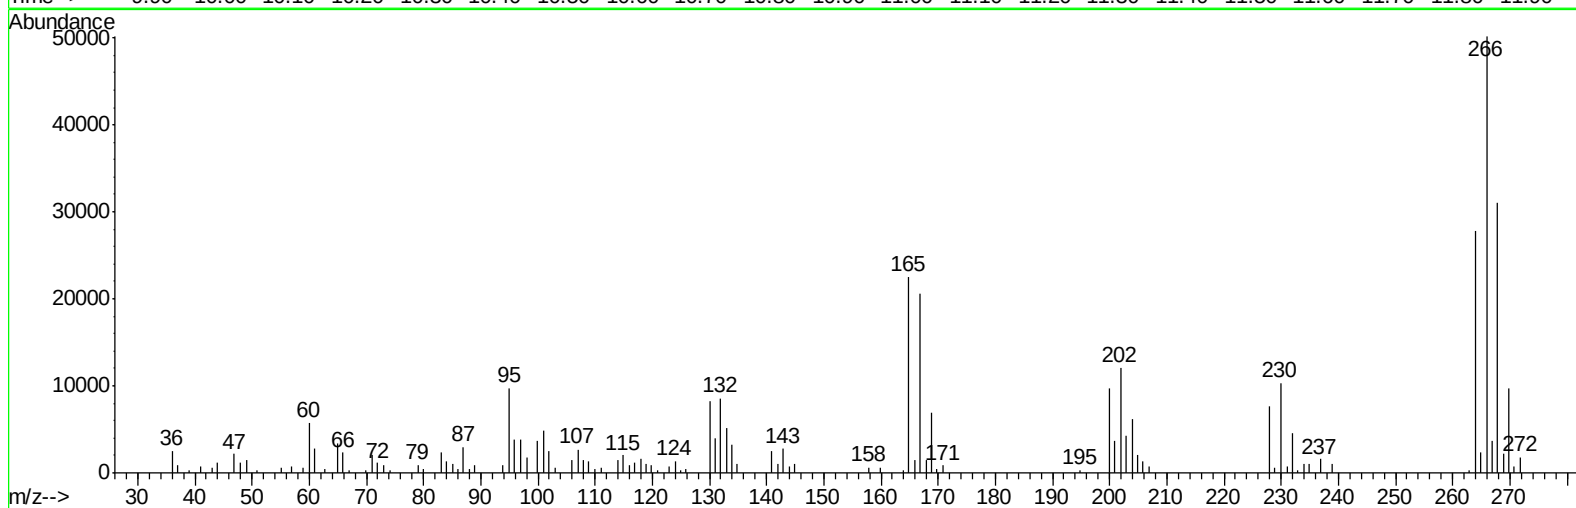


Data Path : Z:\HPCHEM1\BNA F\Data\BF072417\  
Data File : BF096982.D  
Acq On : 24 Jul 2017 10:26  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :

Quant Time: Jul 25 01:28:53 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 18 13:33:22 2017  
Response via : Initial Calibration

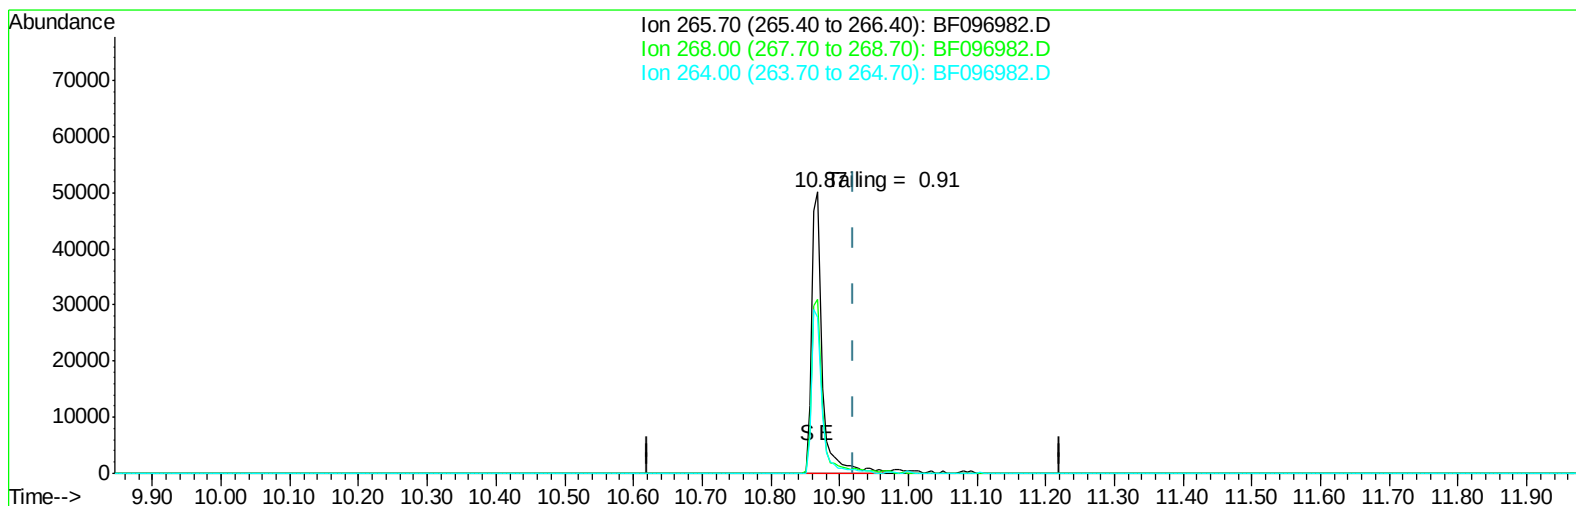

TIC: BF096982.D

(69) Pentachlorophenol (C)

10.869min (-0.053) 68007.73ng



response 51555

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 61.75 |
| 264.00 | 64.60 | 55.52 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF072417\  
 Data File : BF096982.D  
 Acq On : 24 Jul 2017 10:26  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :

Quant Time: Jul 25 01:28:53 2017  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 18 13:33:22 2017  
 Response via : Initial Calibration

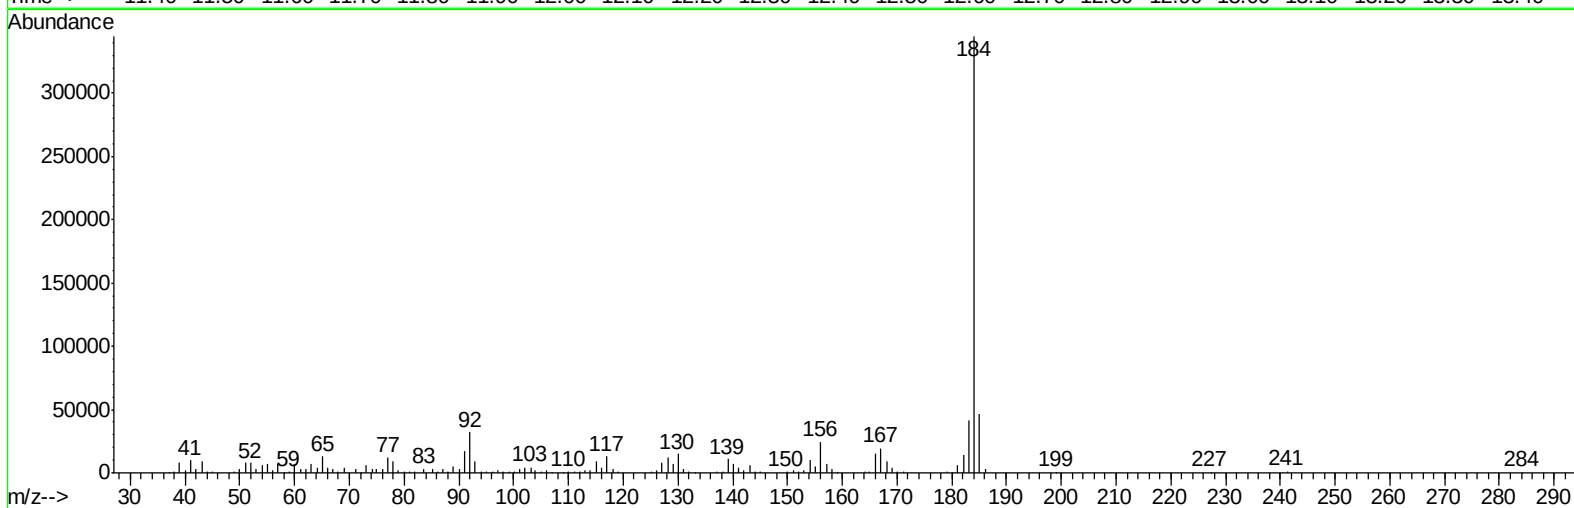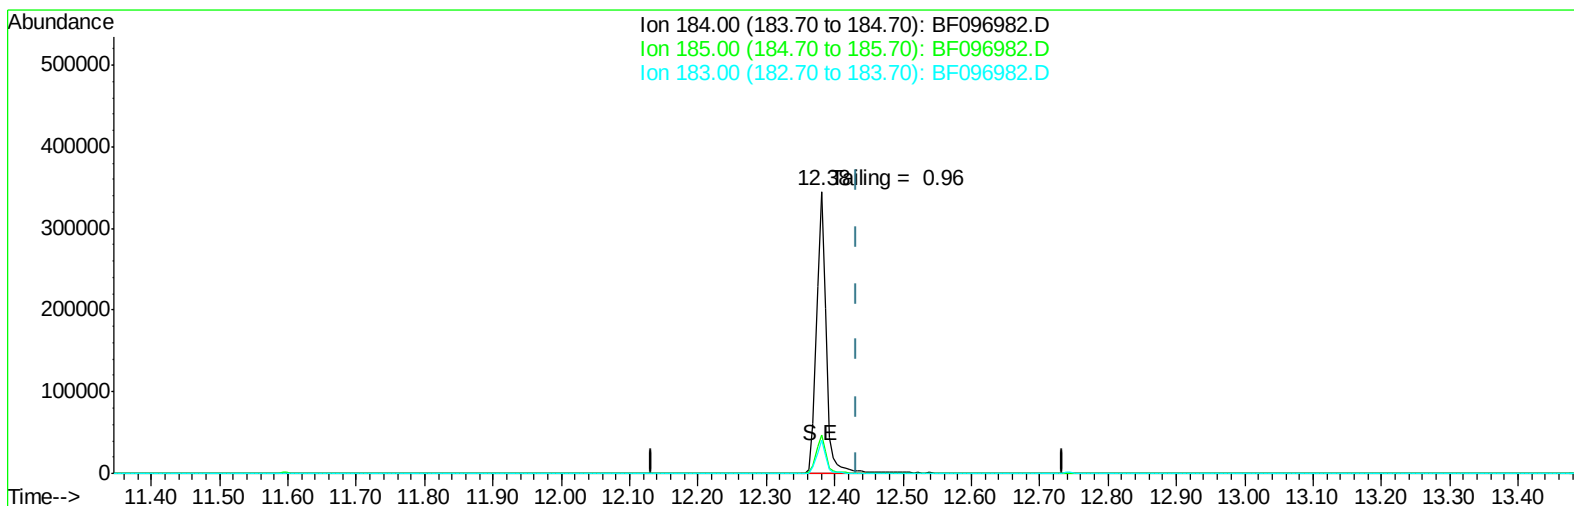

TIC: BF096982.D

(76) Benzidine

12.380min (-0.053) 0.00ng

response 334563

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 13.61# |
| 183.00 | 12.20 | 12.03  |
| 0.00   | 0.00  | 0.00   |