
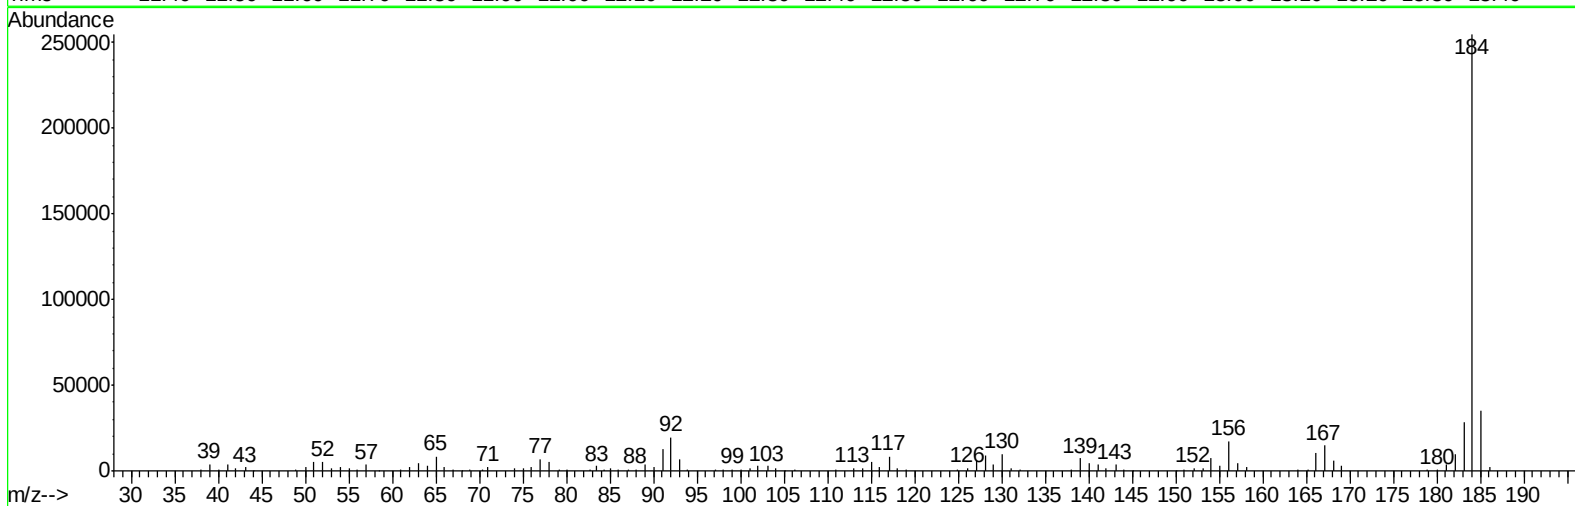


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\
Data File : BF096990.D
Acq On : 24 Jul 2017 17:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 06:57:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:37:00 2017
Response via : Initial Calibration

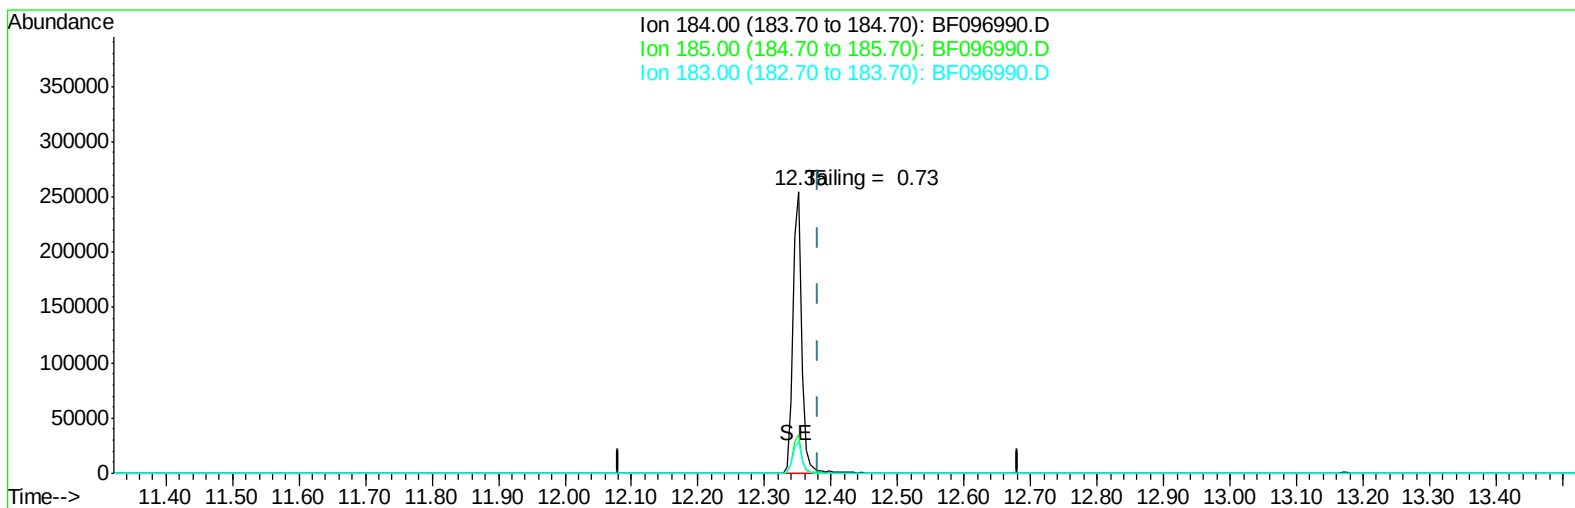

TIC: BF096990.D

(76) Benzidine



12.351min (-0.029) 0.00ng

response 240762

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.72#
183.00	12.20	11.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072417\
Data File : BF096990.D
Acq On : 24 Jul 2017 17:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 06:57:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:37:00 2017
Response via : Initial Calibration

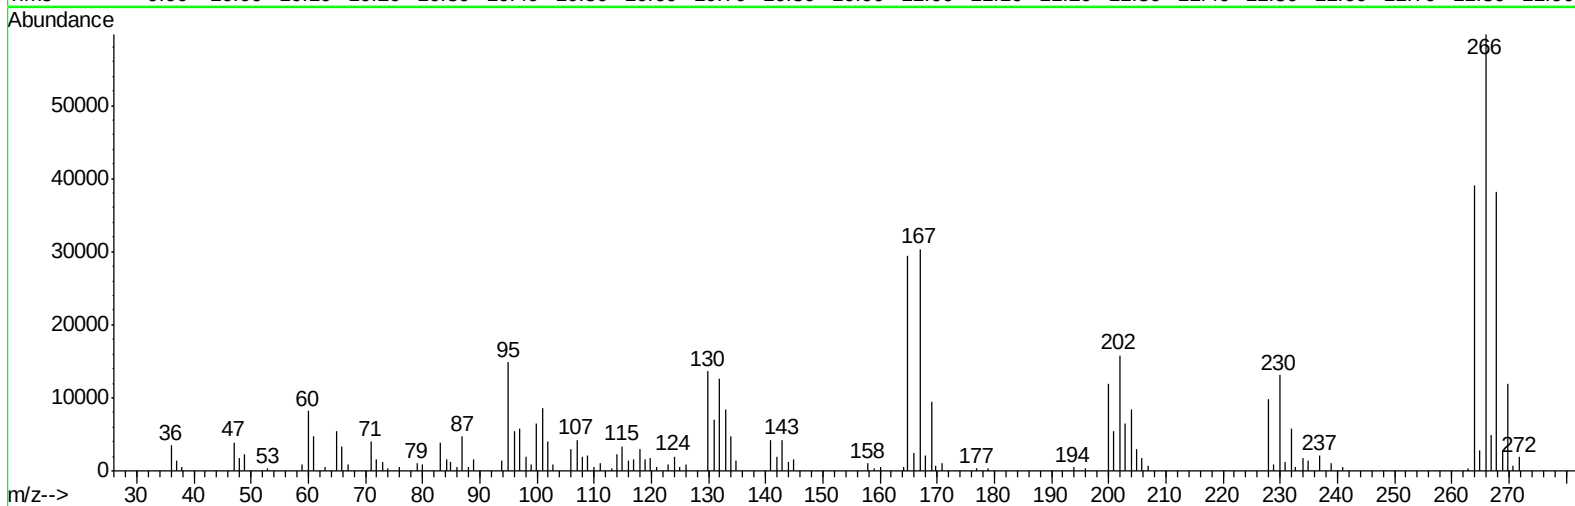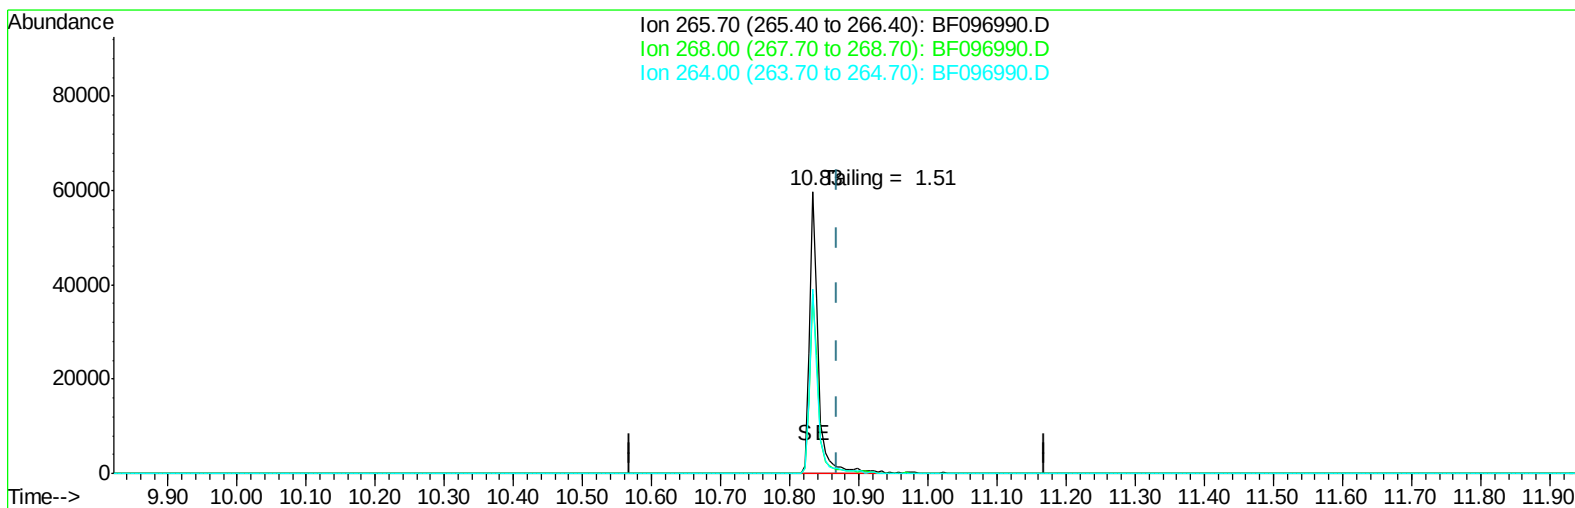

TIC: BF096990.D

(69) Pentachlorophenol (C)

10.833min (-0.035) 70574.75ng

response 53501

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.82
264.00	64.60	65.47
0.00	0.00	0.00