


Data Path : Z:\HPCHEM1\BNA F\Data\BF072417\
 Data File : BF096982.D
 Acq On : 24 Jul 2017 10:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

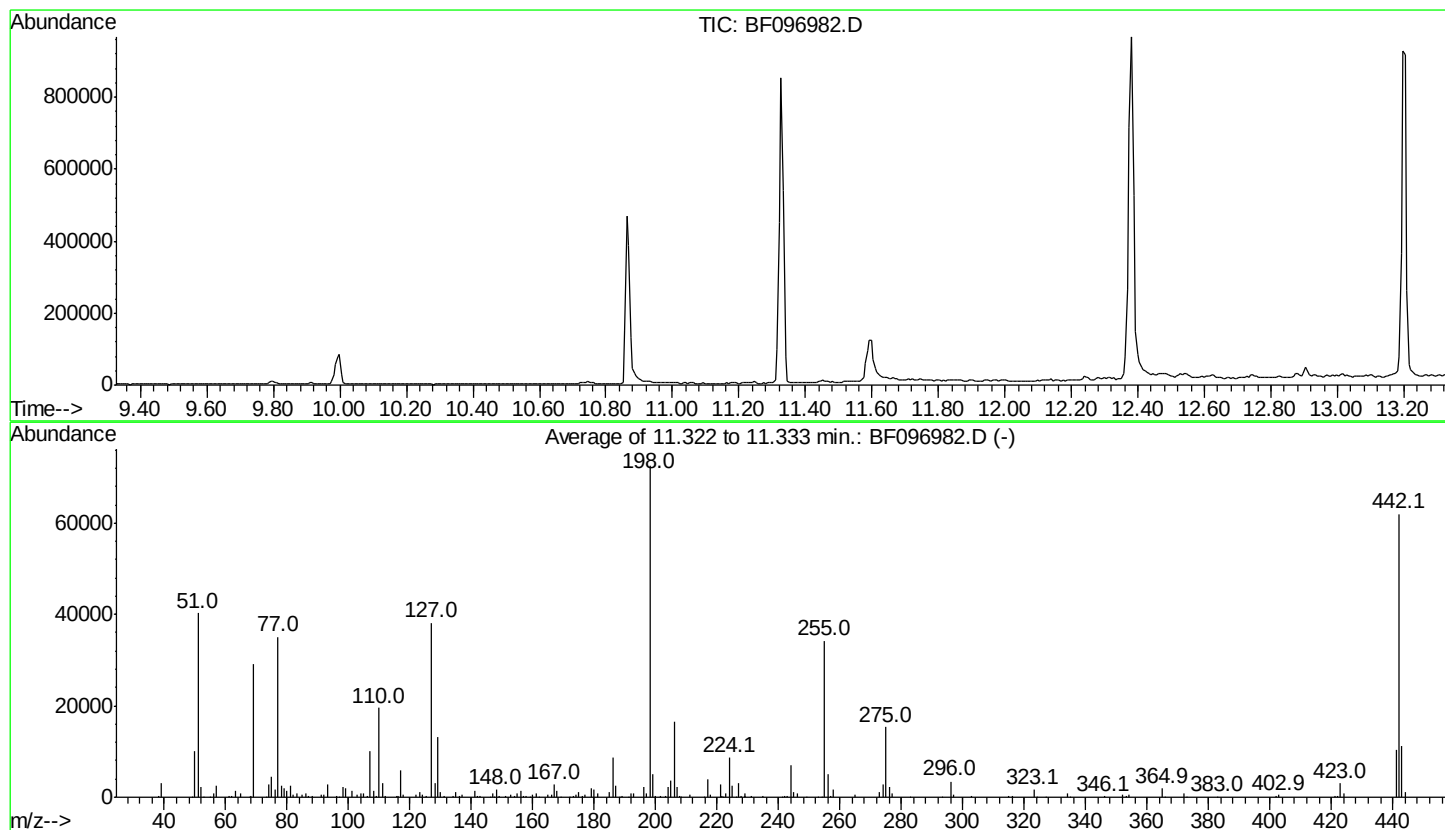

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	40224	PASS
68	69	0.00	2	1.1	319	PASS
69	198	0.00	100	40.2	29172	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	38122	PASS
197	198	0.00	2	1.3	958	PASS
198	198	100	100	100.0	72549	PASS
199	198	5	9	7.0	5054	PASS
275	198	10	60	21.2	15399	PASS
365	198	1	100	2.6	1886	PASS
441	442	0.01	24	16.5	10235	PASS
442	198	50	100	85.4	61946	PASS
443	442	15	24	18.2	11289	PASS