


Data Path : Z:\HPCHEM1\BNA F\Data\BF072417\
 Data File : BF096990.D
 Acq On : 24 Jul 2017 17:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

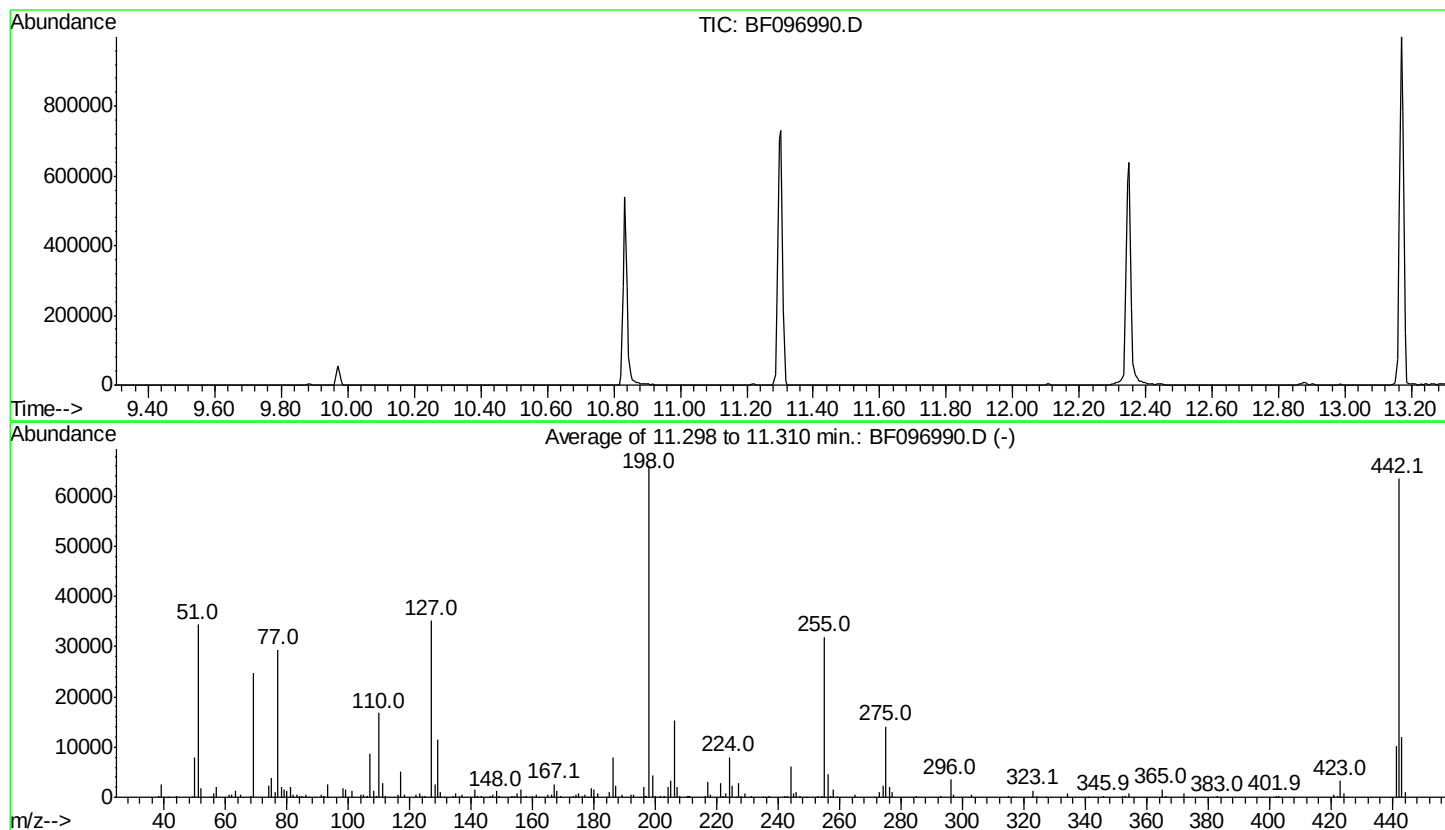

AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	34392	PASS
68	69	0.00	2	1.4	336	PASS
69	198	0.00	100	37.6	24836	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	35122	PASS
197	198	0.00	2	0.4	273	PASS
198	198	100	100	100.0	66096	PASS
199	198	5	9	6.6	4372	PASS
275	198	10	60	21.3	14098	PASS
365	198	1	100	2.4	1557	PASS
441	442	0.01	24	15.9	10093	PASS
442	198	50	100	96.0	63474	PASS
443	442	15	24	18.8	11940	PASS