
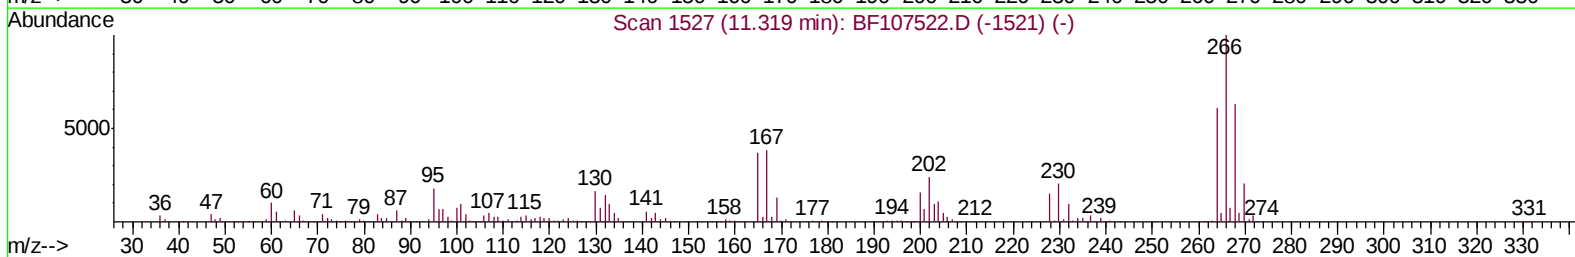
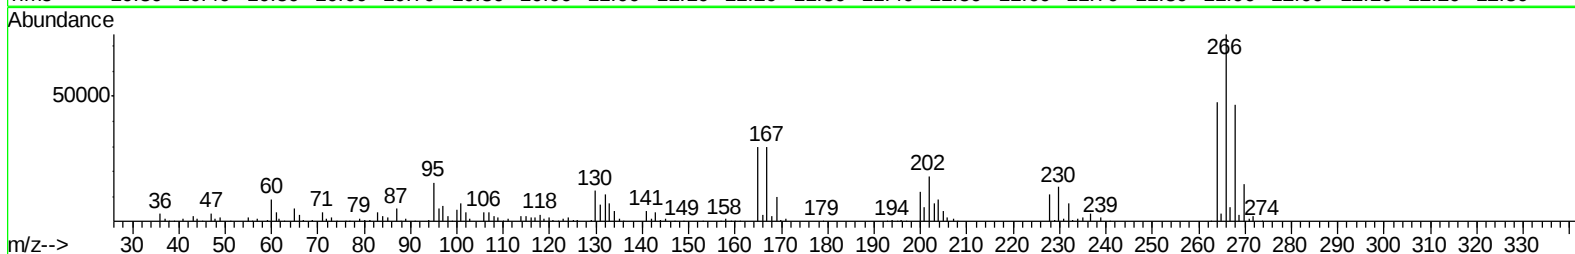


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072418\
Data File : BF107612.D
Acq On : 24 Jul 2018 11:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:01:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

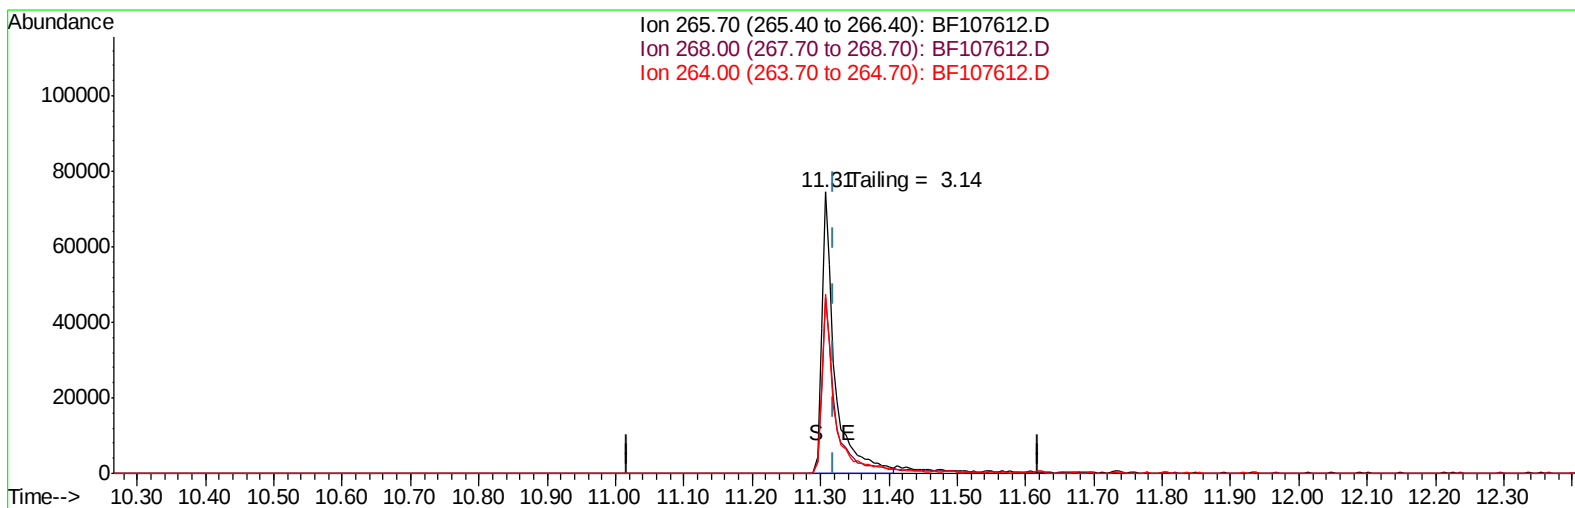

TIC: BF107612.D

(69) Pentachlorophenol (C)

11.307min (-0.012) 33465.85ng

response 100448

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.46
264.00	61.90	63.54
0.00	0.00	0.00

