
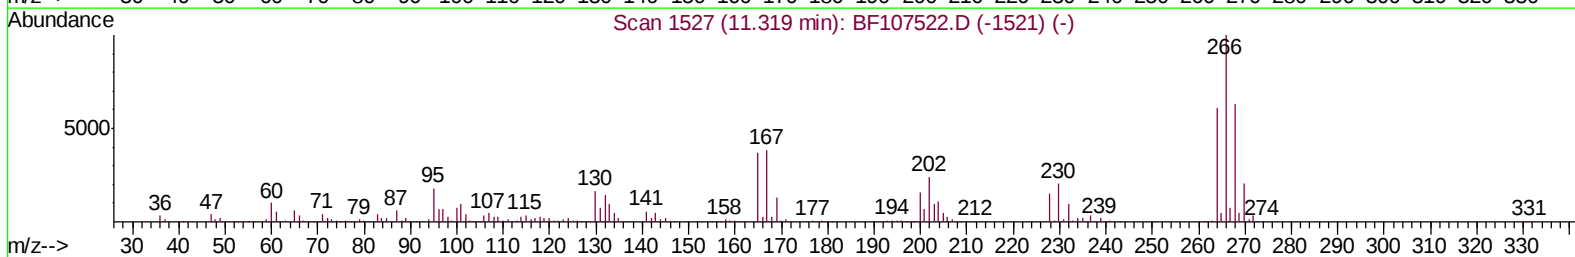
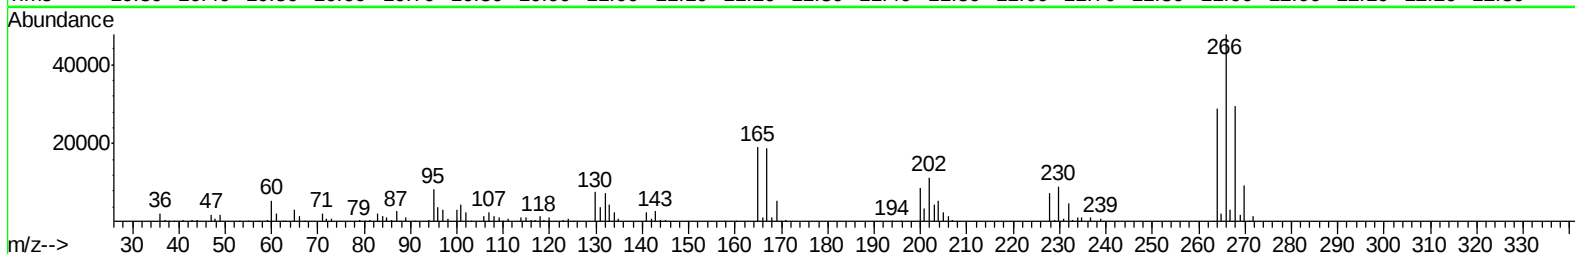


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072418\
Data File : BF107638.D
Acq On : 25 Jul 2018 1:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:04:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

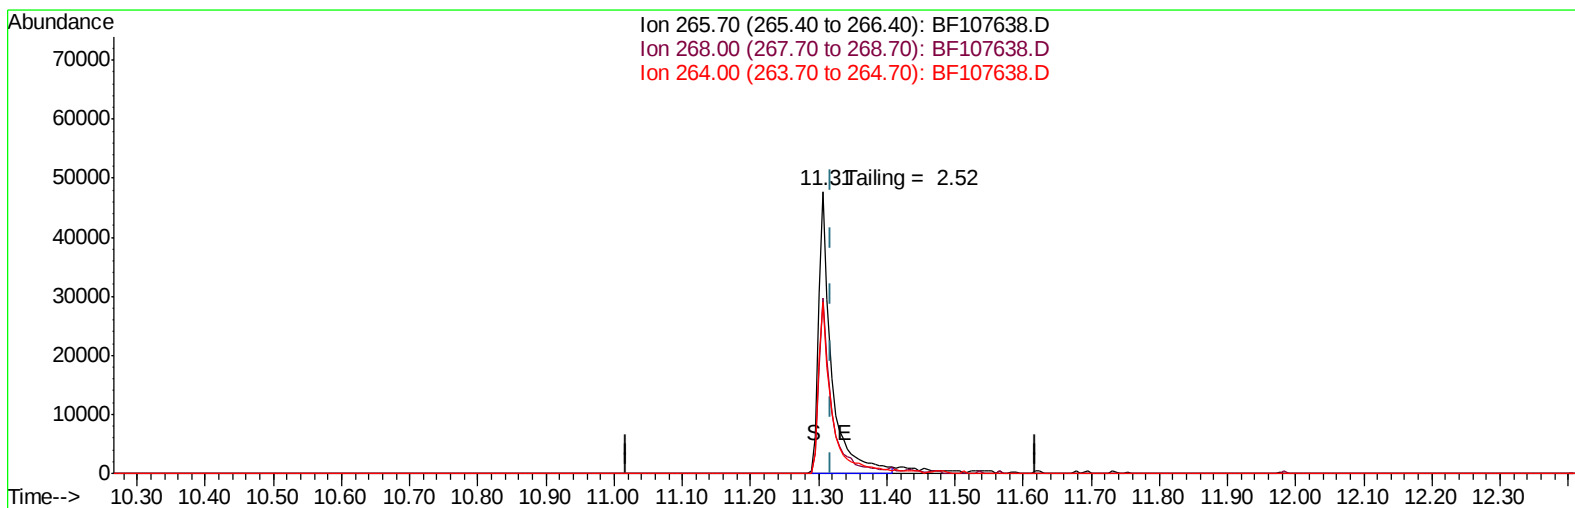

TIC: BF107638.D

(69) Pentachlorophenol (C)




11.307min (-0.012) 24340.06ng

response 63014

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.13
264.00	61.90	60.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072418\
 Data File : BF107638.D
 Acq On : 25 Jul 2018 1:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:04:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

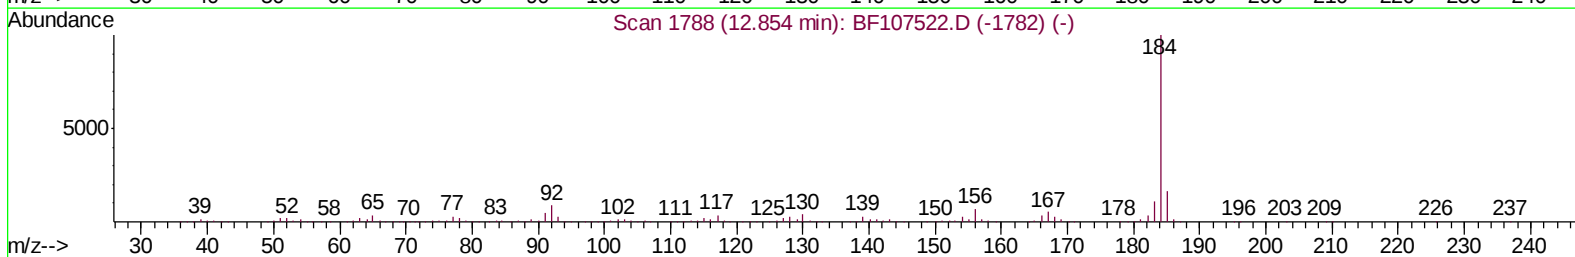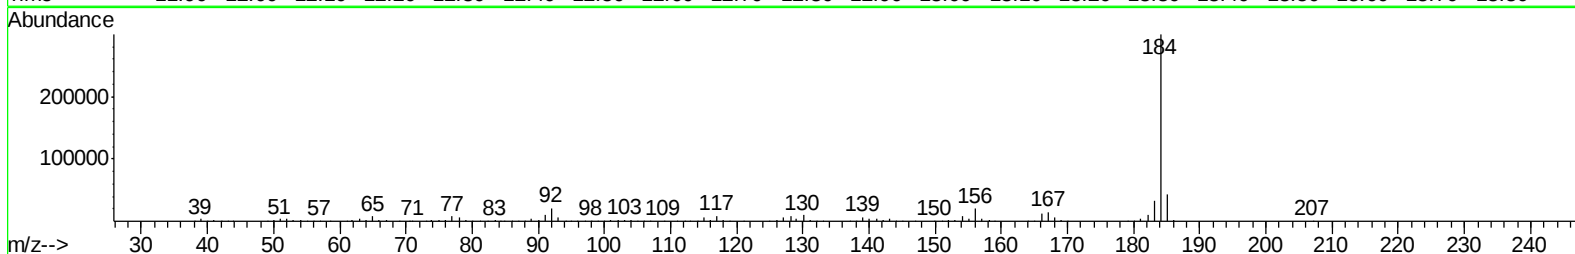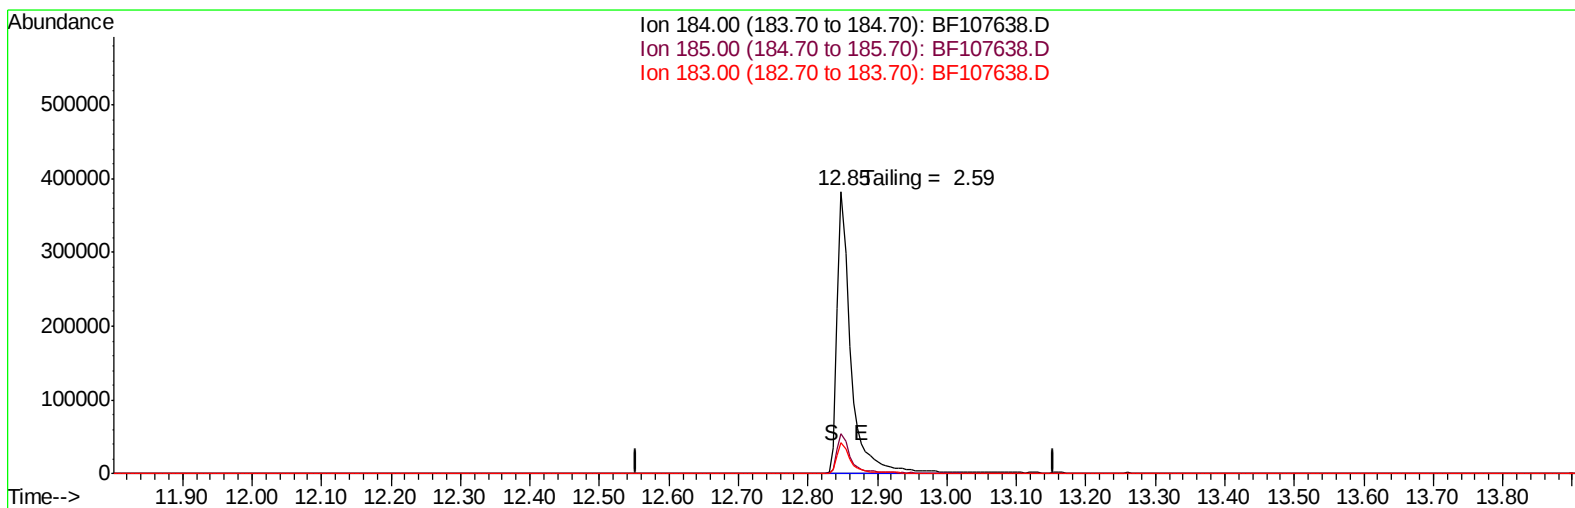

TIC: BF107638.D

(76) Benzidine

12.854min (-12.854) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00