

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072418\
 Data File : BF107616.D
 Acq On : 24 Jul 2018 14:04
 Operator : JU/SJ
 Sample : J3991-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1-A

Quant Time: Jul 25 02:17:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	249384	20.00	ng	-0.01
21) Naphthalene-d8	8.25	136	1014972	20.00	ng	-0.01
38) Acenaphthene-d10	10.01	164	456947	20.00	ng	-0.01
63) Phenanthrene-d10	11.50	188	949914	20.00	ng	-0.01
75) Chrysene-d12	14.15	240	658223	20.00	ng	-0.02
86) Perylene-d12	15.68	264	604964	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	1453020	93.68	ng	0.00
7) Phenol-d6	6.60	99	1803514	96.84	ng	-0.01
23) Nitrobenzene-d5	7.53	82	1136969	75.60	ng	-0.02
41) 2,4,6-Tribromophenol	10.80	330	528965	101.80	ng	-0.02
44) 2-Fluorobiphenyl	9.32	172	1988190	71.22	ng	-0.01
78) Terphenyl-d14	13.09	244	1981009	77.05	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.71	163	383314	11.130	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072418\
Data File : BF107616.D
Acq On : 24 Jul 2018 14:04
Operator : JU/SJ
Sample : J3991-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1-A

Quant Time: Jul 25 02:17:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

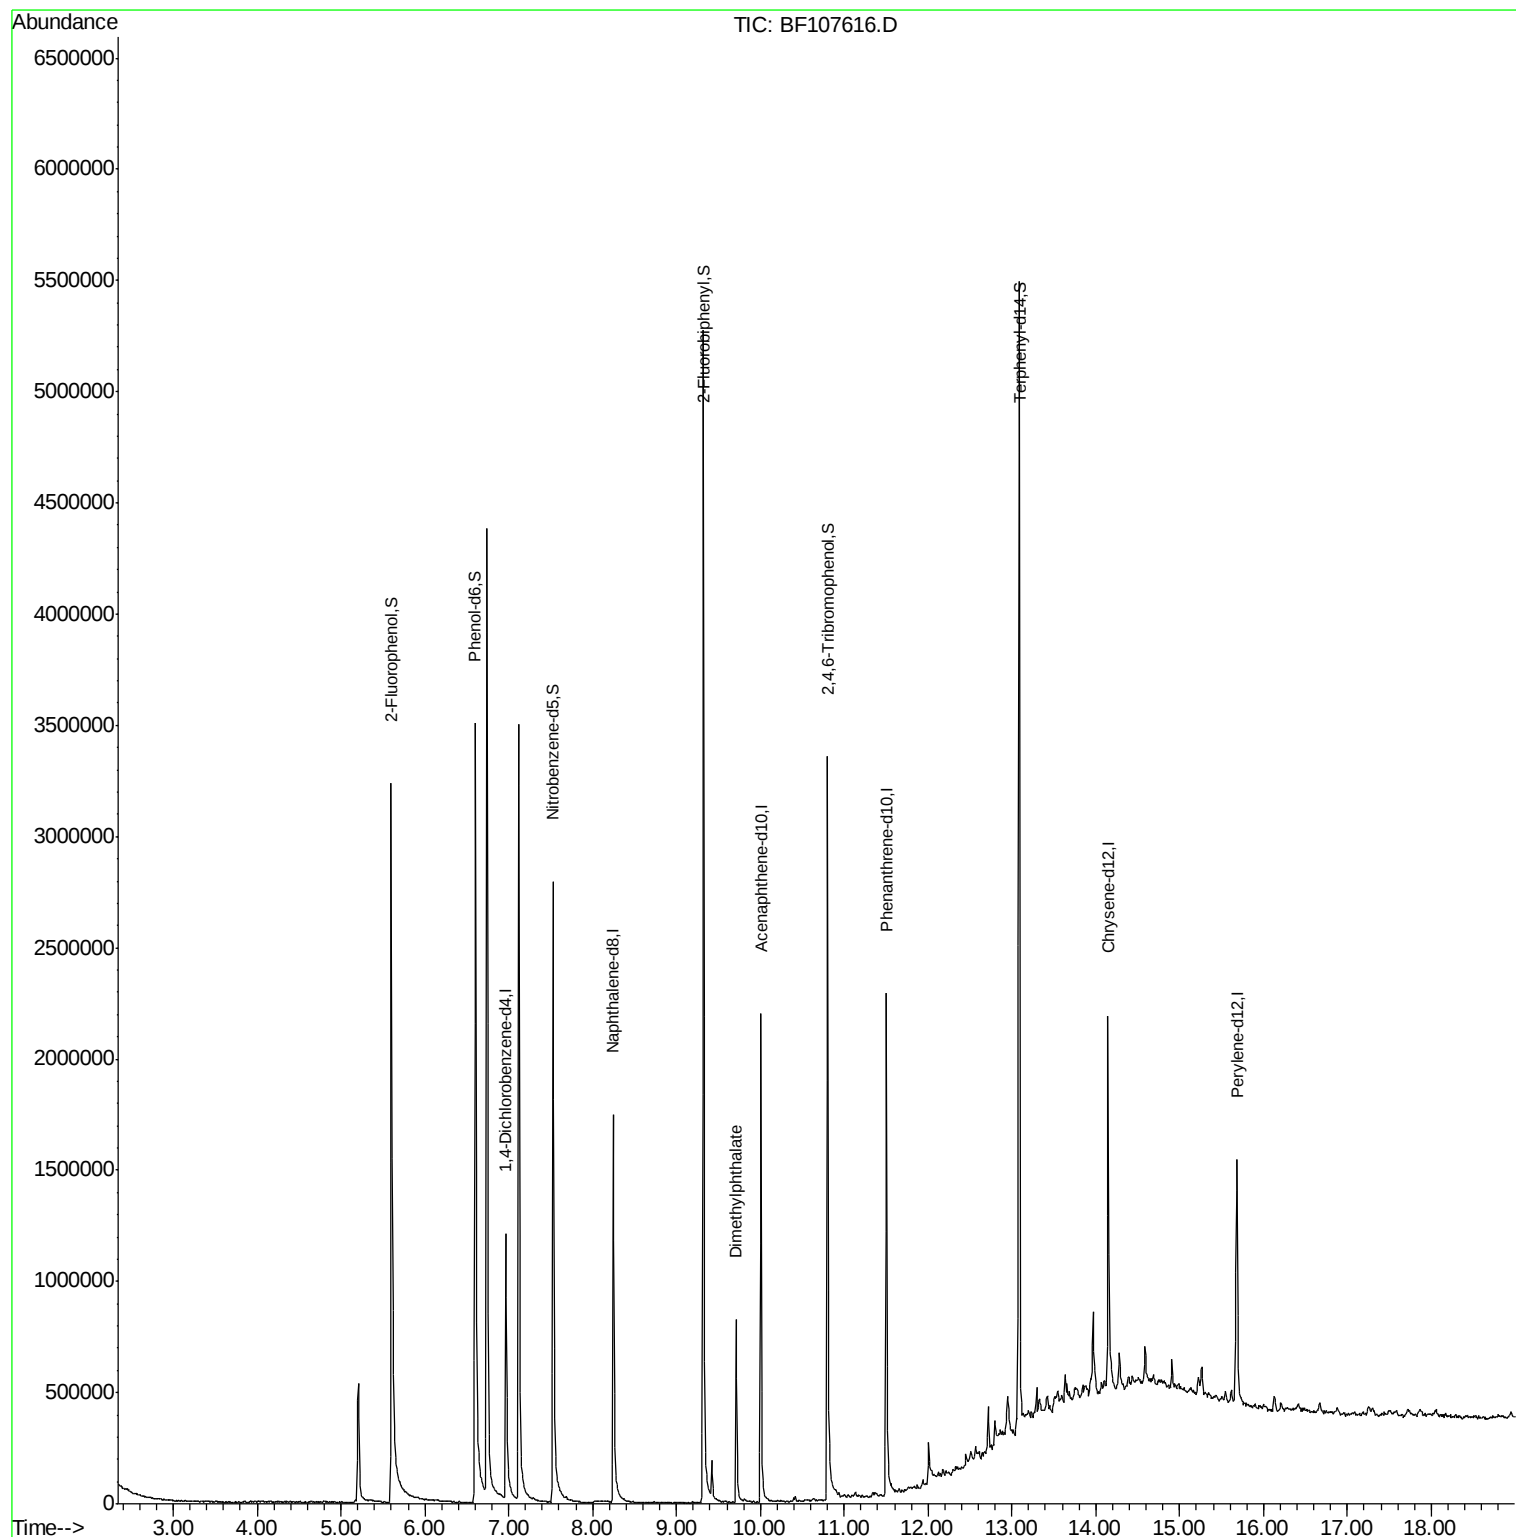

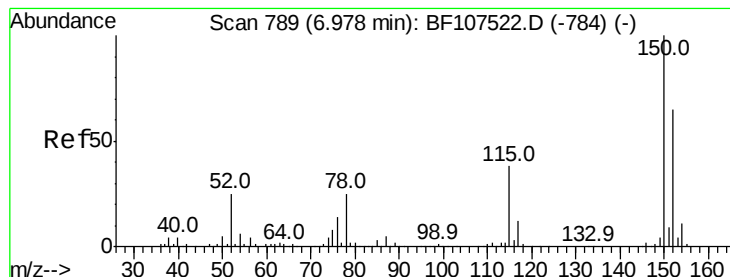


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. -0.01 min
Lab File: BF107616.D
Acq: 24 Jul 2018 14:04

Instrument :
BNA_F
ClientSampled :
SB-1-A

Tot Ion:152 Resp: 249384
Ion Ratio Lower Upper
152 100
150 160.1 124.6 186.8
115 61.0 50.1 75.1

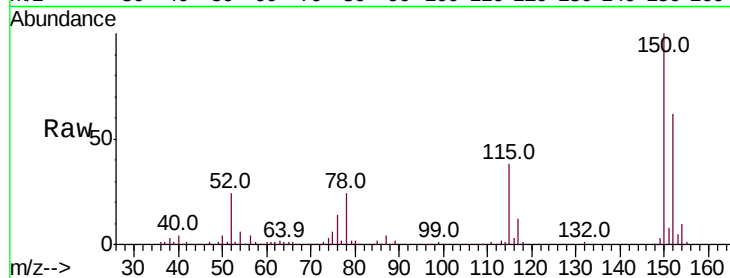


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

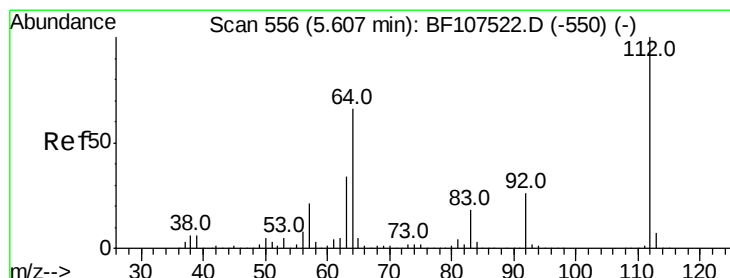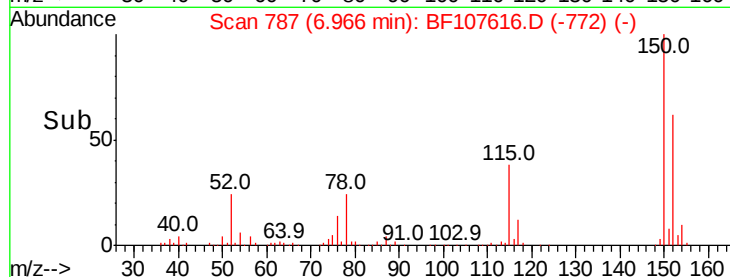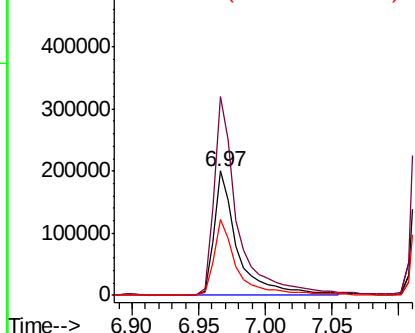



#5


2-Fluorophenol
Concen: 93.678 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.01 min
Lab File: BF107616.D
Acq: 24 Jul 2018 14:04

Tgt Ion:112 Resp: 1453020
Ion Ratio Lower Upper
112 100
64 66.3 47.9 71.9
63 34.6 23.7 35.5

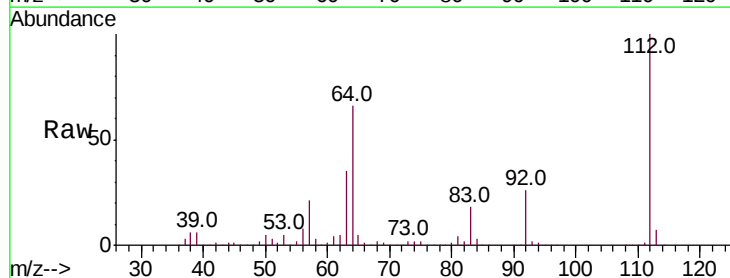

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

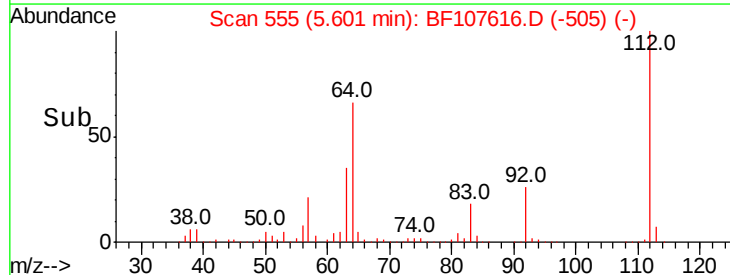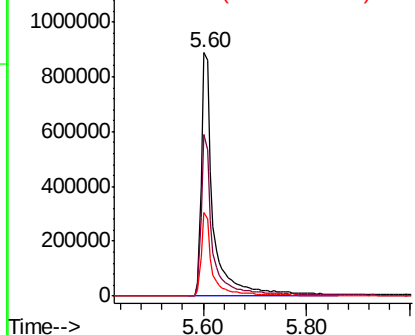

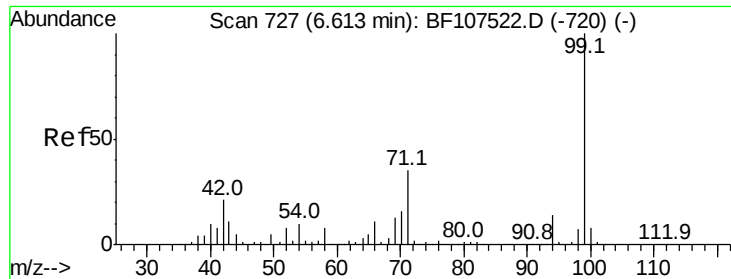

#7

Phenol-d6

Concen: 96.836 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04

Instrument :

BNA_F

ClientSampleId :

SB-1-A


Tot Ion: 99 Resp: 1803514

Ion Ratio Lower Upper




99 100

42 20.0 14.5 21.7

71 35.7 25.4 38.0

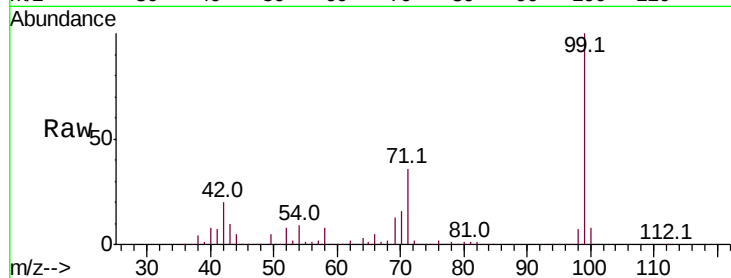

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

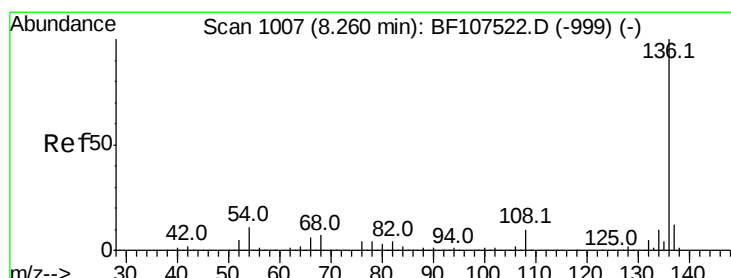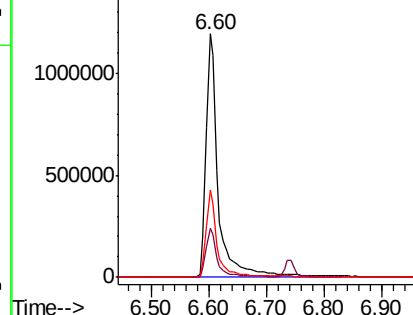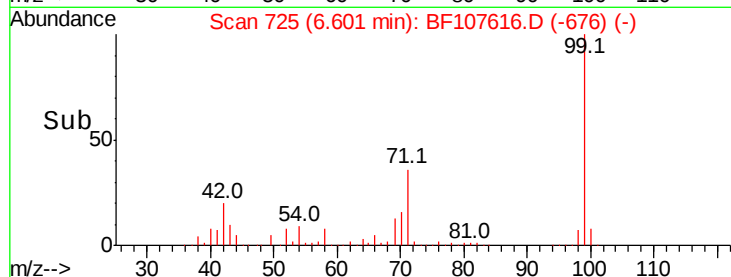

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. -0.01 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04

Tgt Ion: 136 Resp: 1014972


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 9.7 6.6 9.8

68 5.9 5.0 7.4

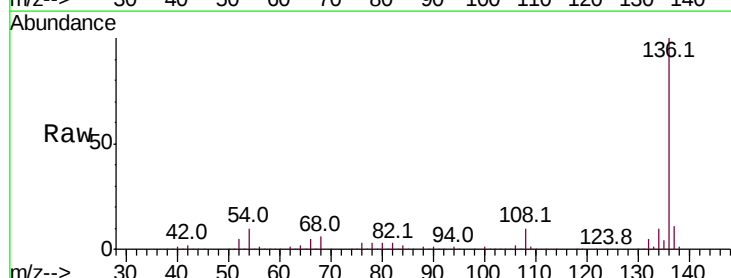

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



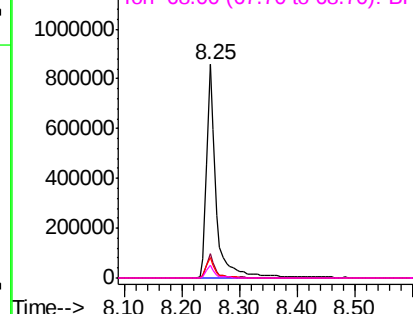
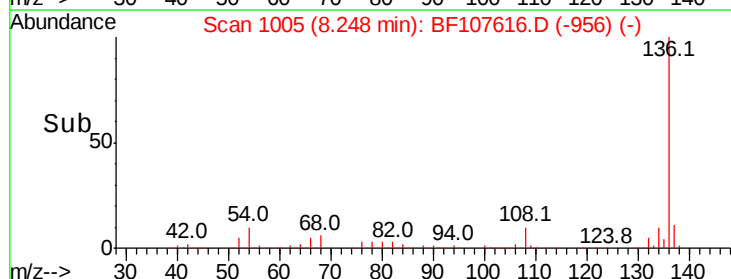


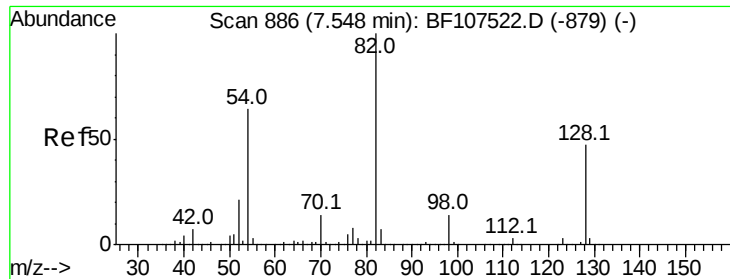

#23
 Nitrobenzene-d5
 Concen: 75.599 ng
 RT: 7.53 min Scan# 883
 Delta R.T. -0.02 min
 Lab File: BF107616.D
 Acq: 24 Jul 2018 14:04




Instrument :
 BNA_F
 ClientSampleId :
 SB-1-A


Tot Ion: 82 Resp: 1136969
 Ion Ratio Lower Upper
 82 100
 128 46.5 36.1 54.1
 54 61.7 41.4 62.2

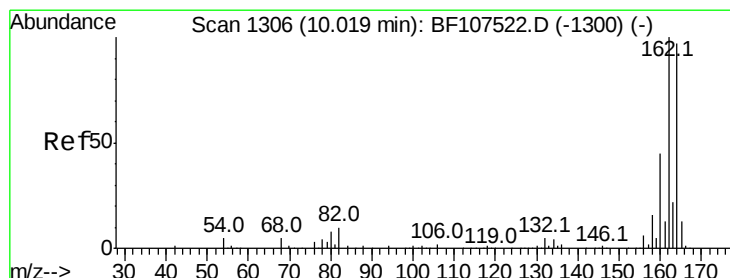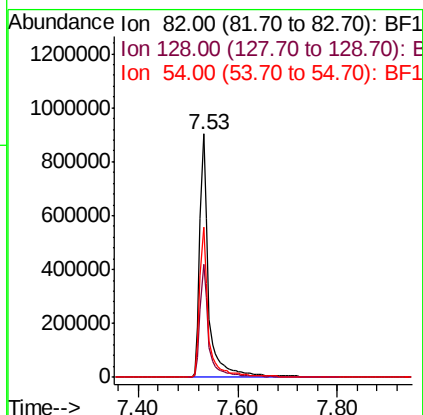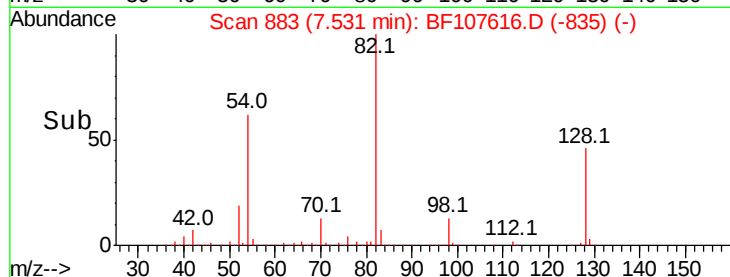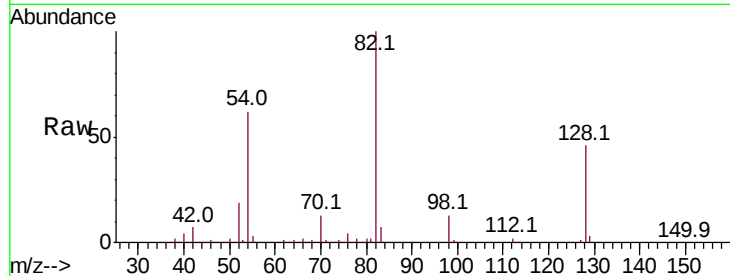

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.01 min Scan# 1304
 Delta R.T. -0.01 min
 Lab File: BF107616.D
 Acq: 24 Jul 2018 14:04

Tgt Ion:164 Resp: 456947
 Ion Ratio Lower Upper
 164 100
 162 104.3 86.1 129.1
 160 47.4 38.3 57.5

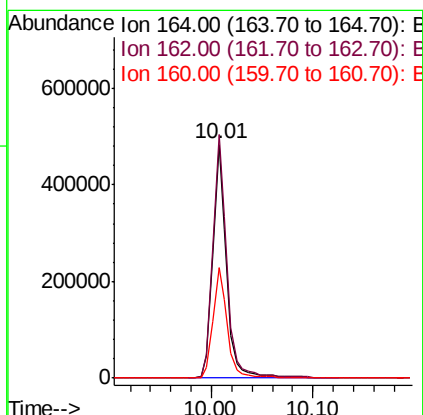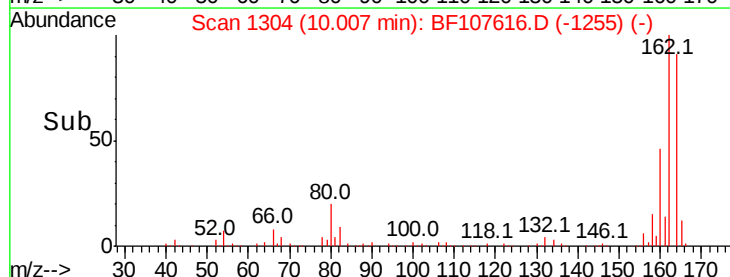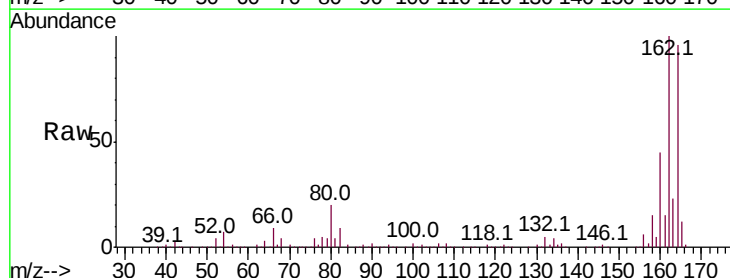


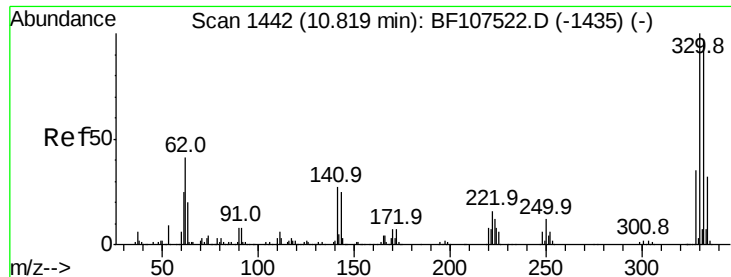

#41
 2,4,6-Tribromophenol
 Concen: 101.798 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.02 min
 Lab File: BF107616.D
 Acq: 24 Jul 2018 14:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-1-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.0	115.6
141	29.1	29.9	44.9#



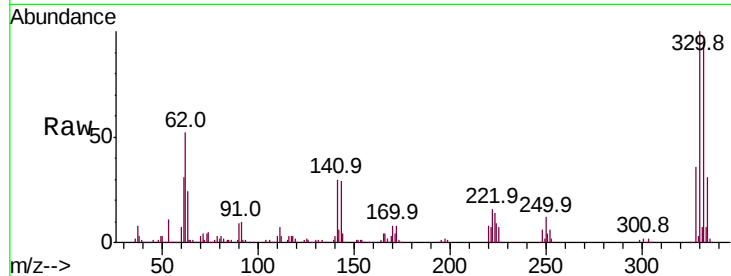


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

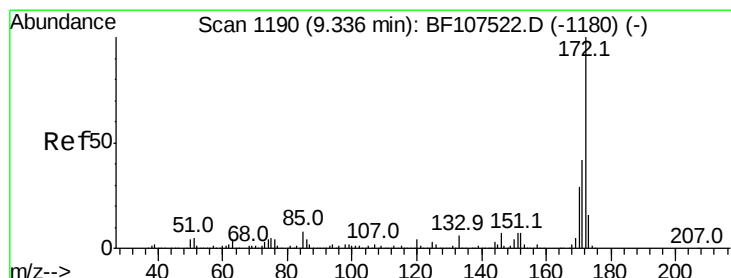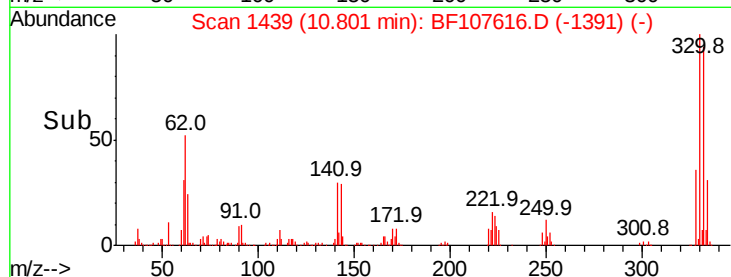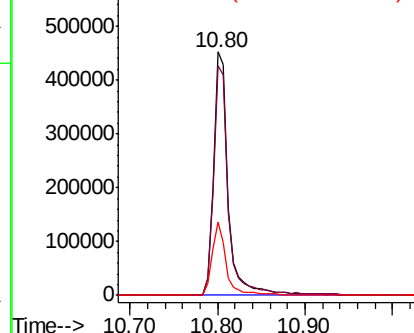

#44
 2-Fluorobiphenyl
 Concen: 71.222 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. -0.01 min
 Lab File: BF107616.D
 Acq: 24 Jul 2018 14:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.1	29.7	44.5
170	25.6	19.6	29.4


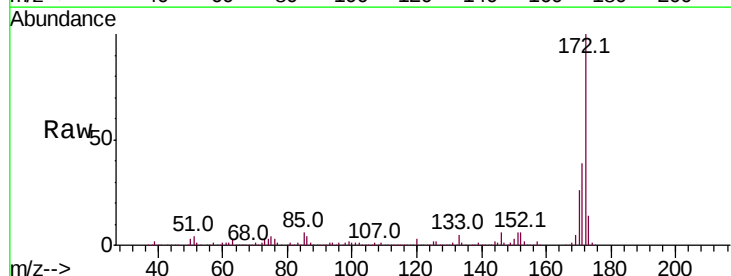



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

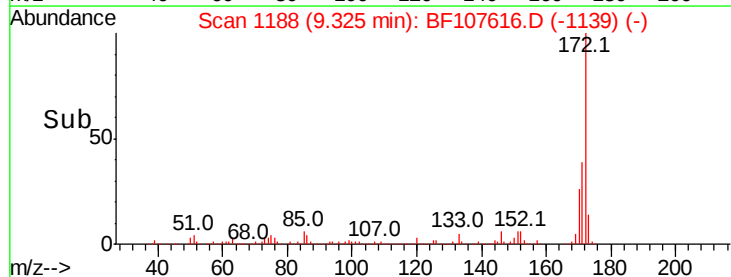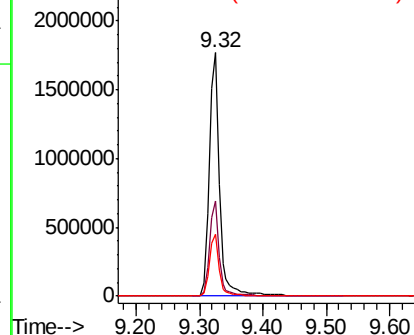

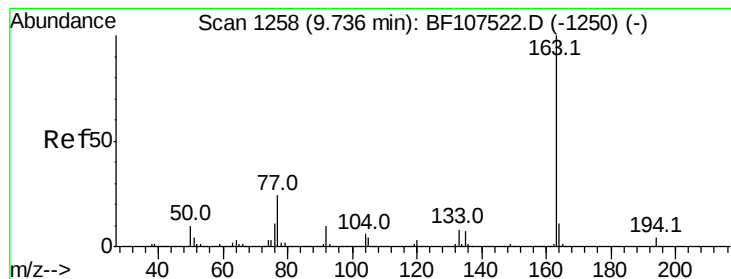

#49

Dimethylphthalate

Concen: 11.130 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.02 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04

Instrument :

BNA_F

ClientSampleId :

SB-1-A


Tot Ion:163 Resp: 383314

Ion Ratio Lower Upper

163 100

194 3.8 2.7 4.1




164 10.2 8.2 12.2

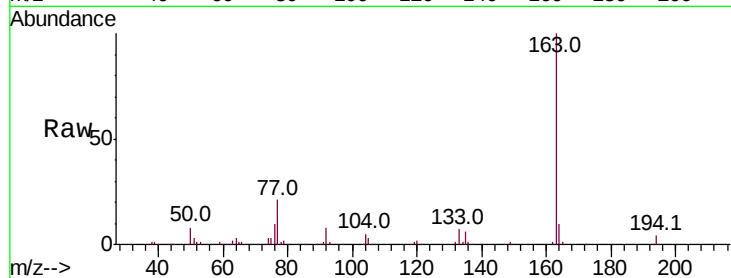

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

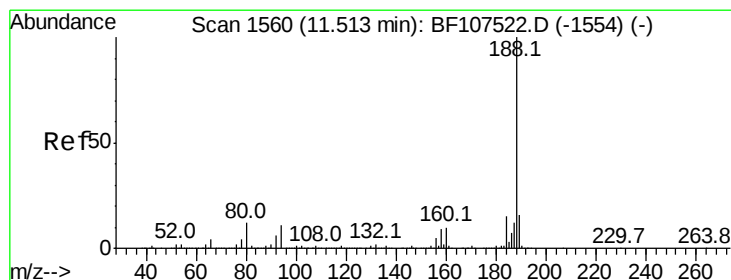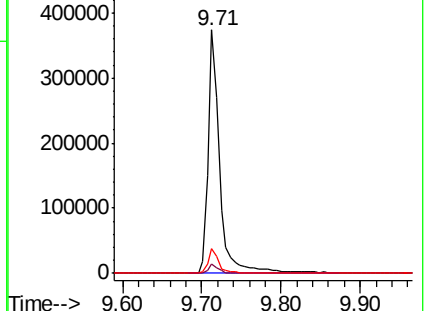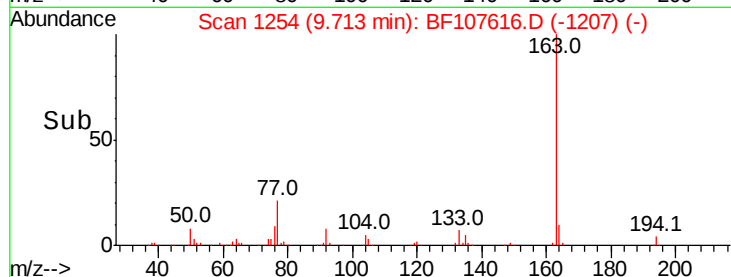

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1558

Delta R.T. -0.01 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04


Tgt Ion:188 Resp: 949914

Ion Ratio Lower Upper

188 100

94 9.3 8.5 12.7



80 10.6 9.2 13.8

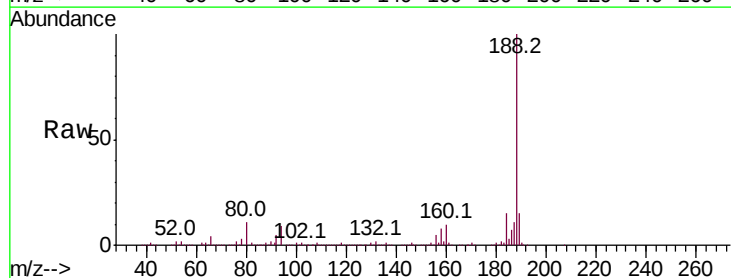


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

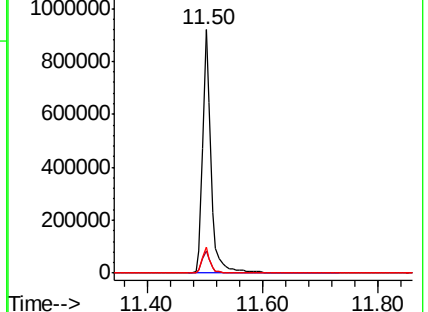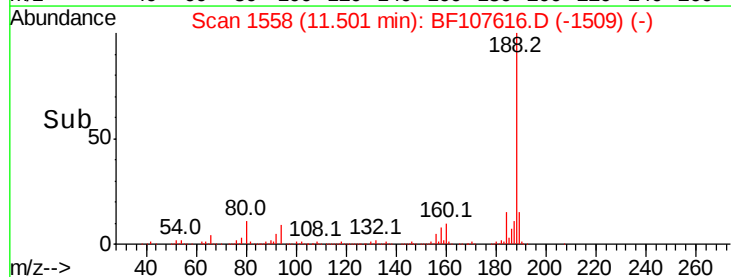

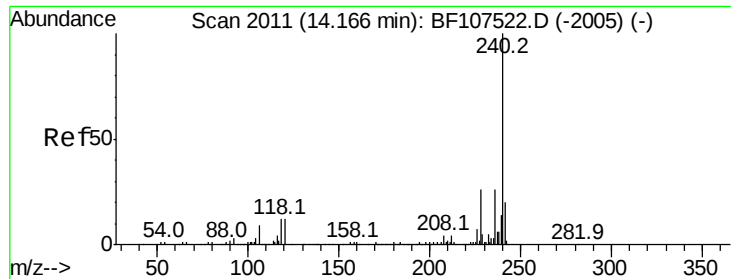

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.02 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04

Instrument :

BNA_F

ClientSampleId :

SB-1-A


Tot Ion:240 Resp: 658223

Ion Ratio Lower Upper

240 100

120 12.2 9.5 14.3




236 26.3 20.7 31.1

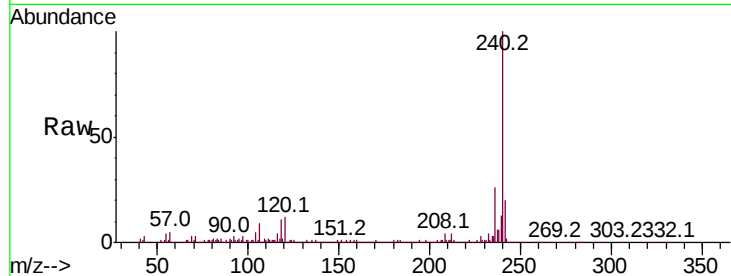

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

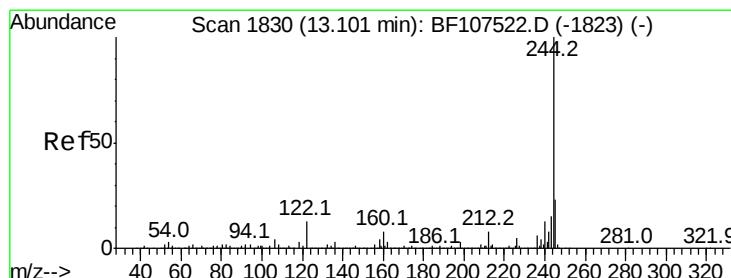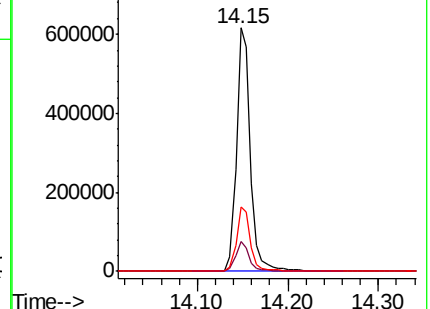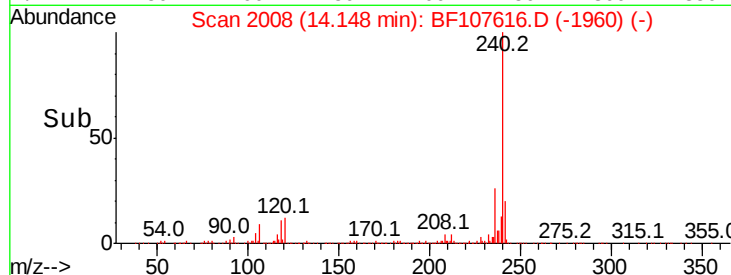

#78

Terphenyl-d14

Concen: 77.049 ng

RT: 13.09 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BF107616.D

Acq: 24 Jul 2018 14:04


Tgt Ion:244 Resp: 1981009

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.3 11.0 16.4

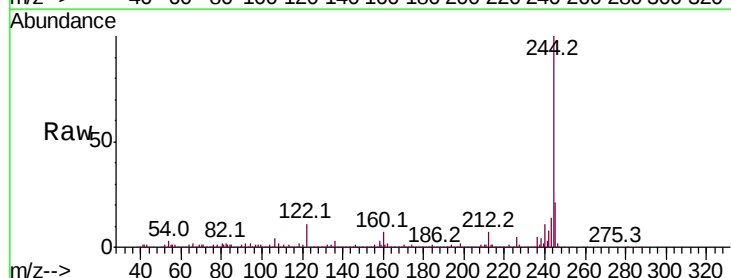


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

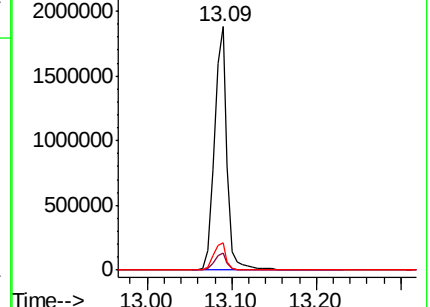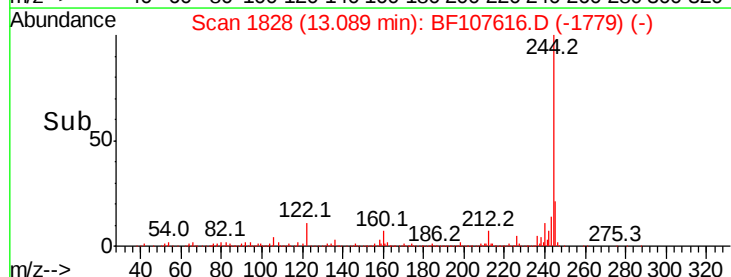

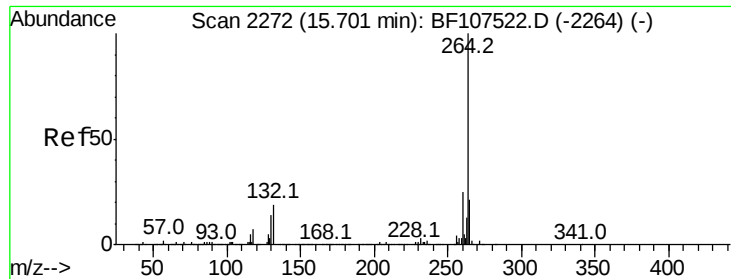

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2269
Delta R.T. -0.02 min
Lab File: BF107616.D
Acq: 24 Jul 2018 14:04

Instrument :
BNA_F
ClientSampleId :
SB-1-A

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.2	28.8
265	22.2	17.5	26.3

